

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
 Data File : PP033385.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Feb 2021 20:00
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:25:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 23:16:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.725	3.997	3036470	1968726	49.517	48.145
2)	SA Decachlor...	10.536f	9.255	2268654	1747537	52.080	52.165m
Target Compounds							
21)	L5 AR-1248-1	6.022	5.240	484737	334941	506.273	515.027
22)	L5 AR-1248-2	6.314	5.501	647954	461734	488.996	481.295
23)	L5 AR-1248-3	6.528	5.545	806097	494482	497.812	486.333
24)	L5 AR-1248-4	6.954	5.730	864937	577073	502.682	465.654
25)	L5 AR-1248-5	6.992	6.150	832757	569264	478.595	504.072

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
Data File : PP033385.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Feb 2021 20:00
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 23:16:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

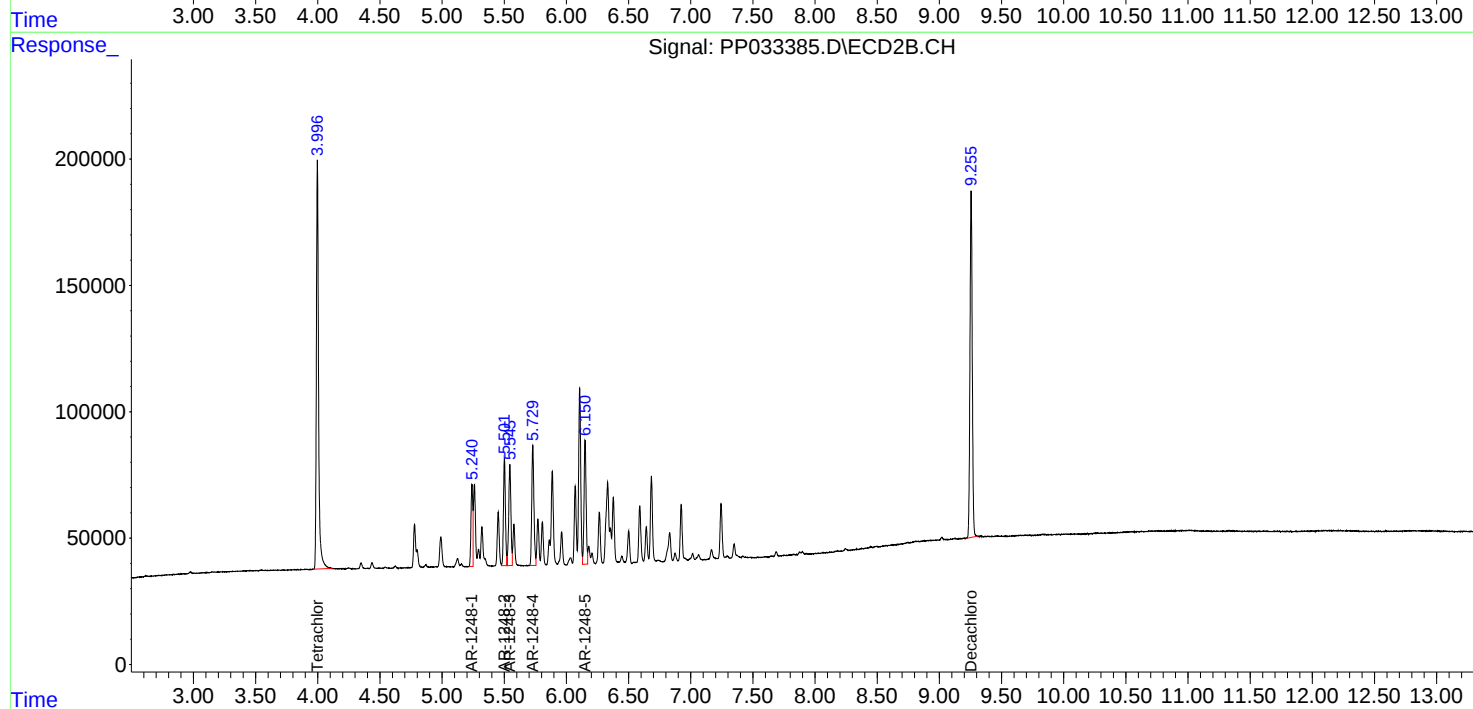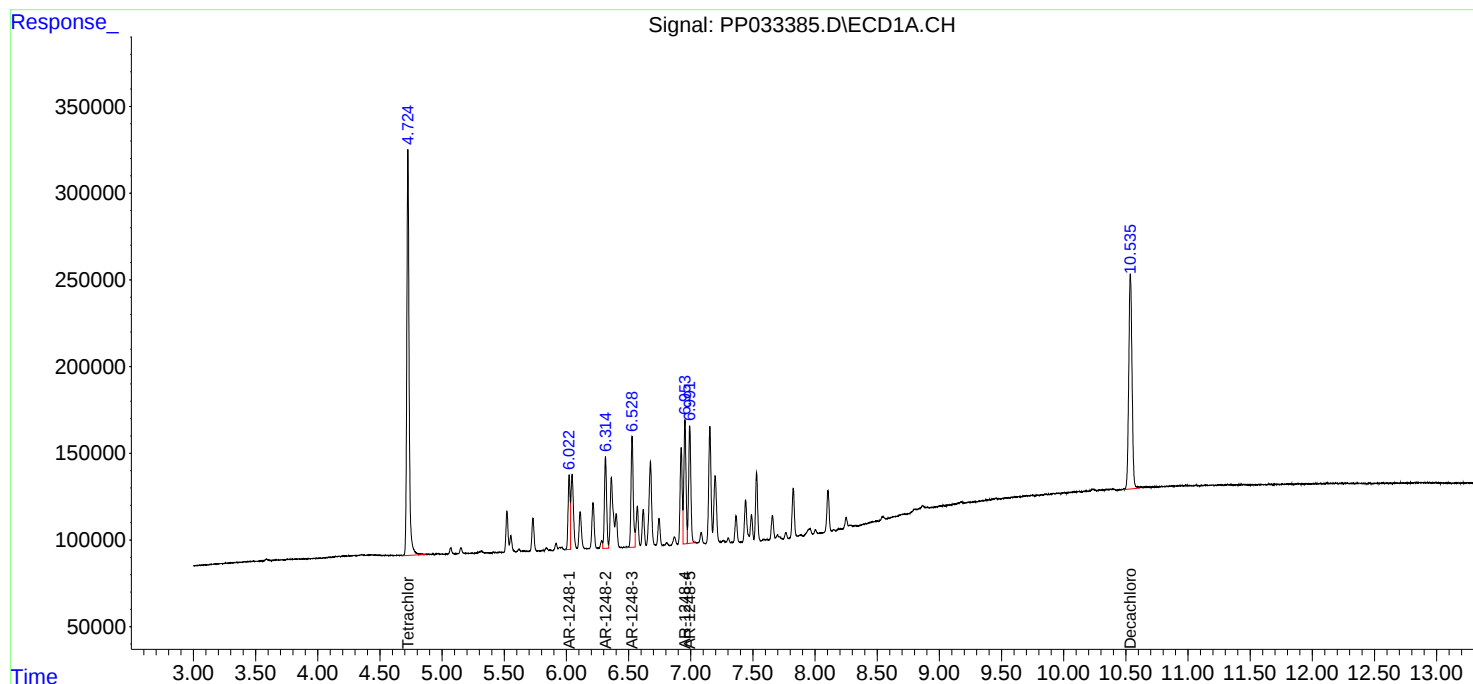

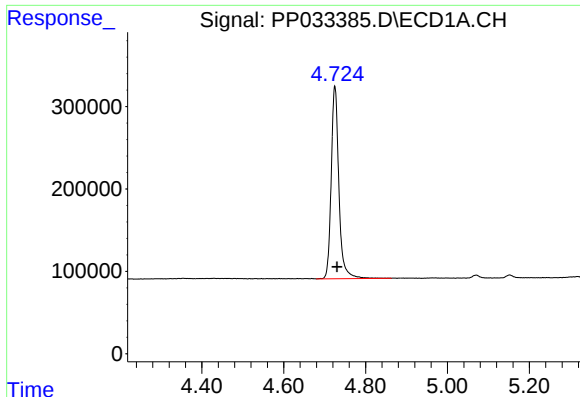


#1 Tetrachloro-m-xylene

R.T.: 4.725 min
Delta R.T.: -0.005 min
Response: 3036470
Conc: 49.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:42 AM

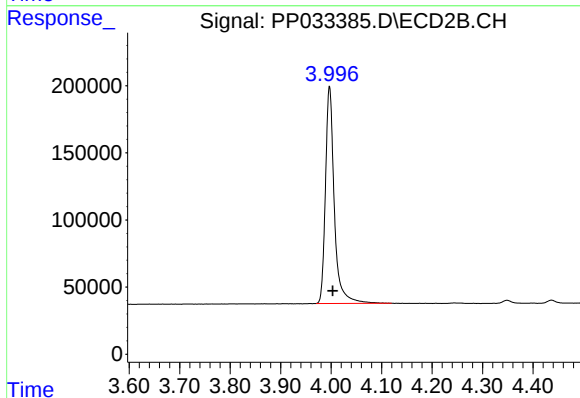


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 1968726
Conc: 48.14 ng/ml

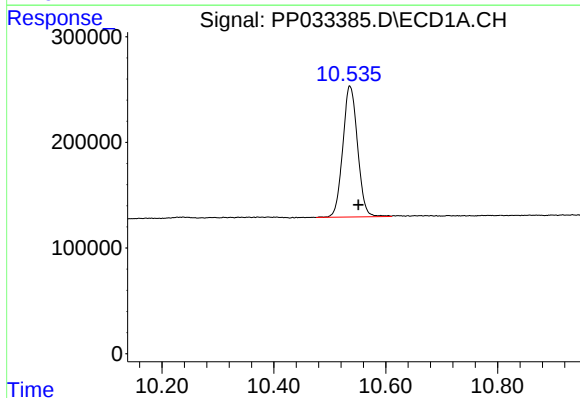


#2 Decachlorobiphenyl

R.T.: 10.536 min
Delta R.T.: -0.015 min
Response: 2268654
Conc: 52.08 ng/ml

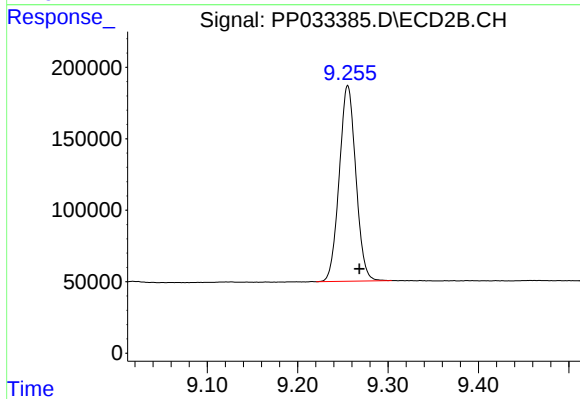

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.013 min
Response: 1747537
Conc: 52.17 ng/ml m

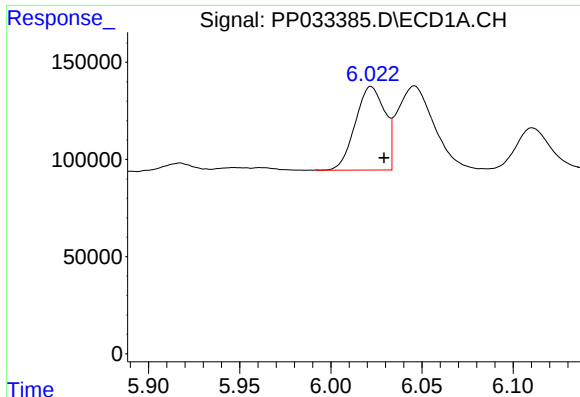


#21 AR-1248-1

R.T.: 6.022 min
Delta R.T.: -0.007 min
Response: 484737
Conc: 506.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:42 AM

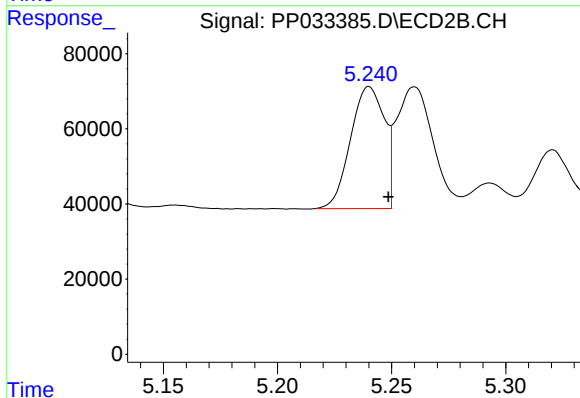


#21 AR-1248-1

R.T.: 5.240 min
Delta R.T.: -0.008 min
Response: 334941
Conc: 515.03 ng/ml

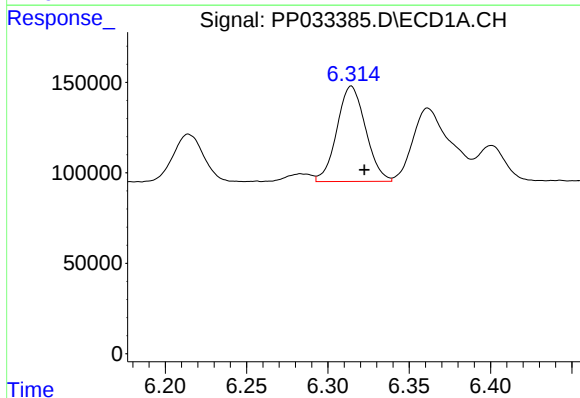


#22 AR-1248-2

R.T.: 6.314 min
Delta R.T.: -0.008 min
Response: 647954
Conc: 489.00 ng/ml

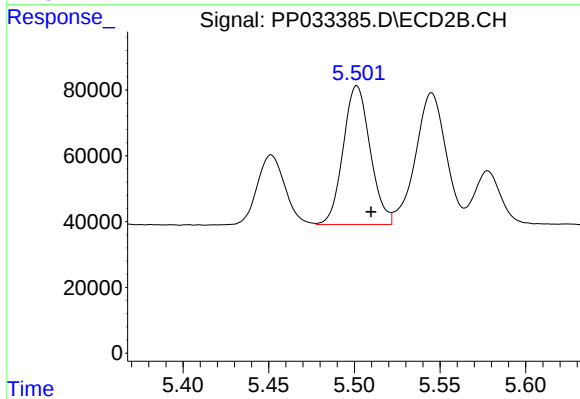

#22 AR-1248-2

R.T.: 5.501 min
Delta R.T.: -0.008 min
Response: 461734
Conc: 481.29 ng/ml

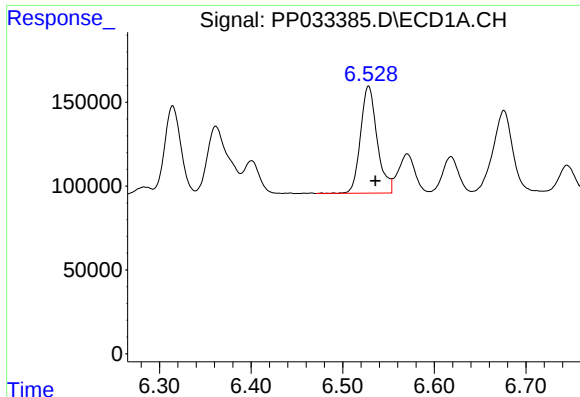


#23 AR-1248-3

R.T.: 6.528 min
Delta R.T.: -0.007 min
Response: 806097
Conc: 497.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:42 AM

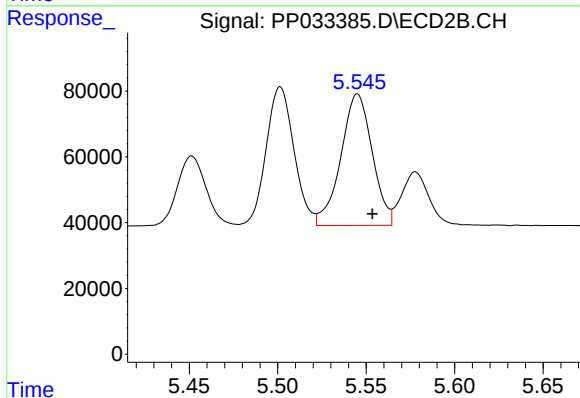


#23 AR-1248-3

R.T.: 5.545 min
Delta R.T.: -0.008 min
Response: 494482
Conc: 486.33 ng/ml

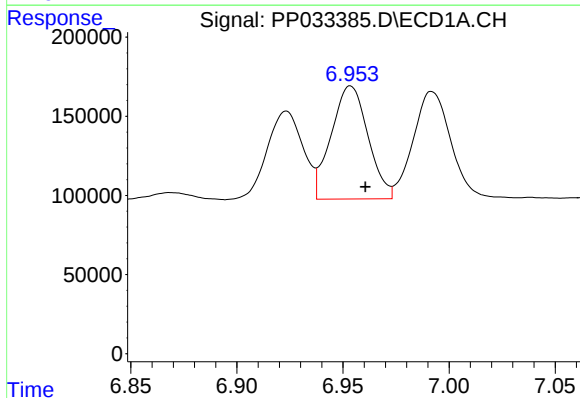


#24 AR-1248-4

R.T.: 6.954 min
Delta R.T.: -0.007 min
Response: 864937
Conc: 502.68 ng/ml

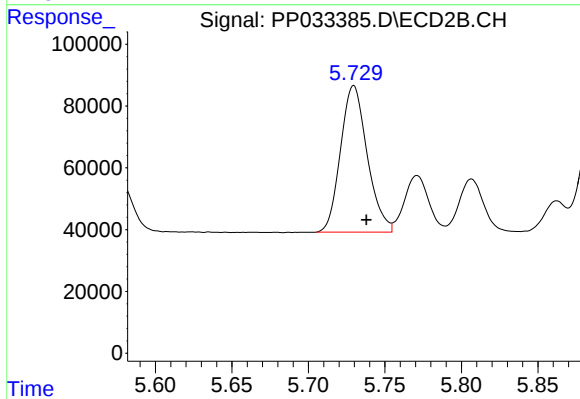

#24 AR-1248-4

R.T.: 5.730 min
Delta R.T.: -0.008 min
Response: 577073
Conc: 465.65 ng/ml

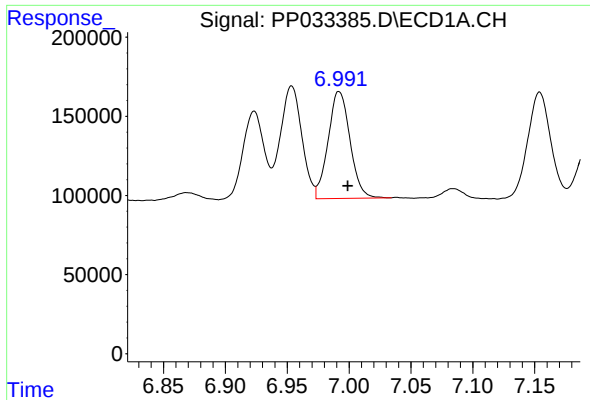


#25 AR-1248-5

R.T.: 6.992 min
Delta R.T.: -0.007 min
Response: 832757
Conc: 478.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:42 AM

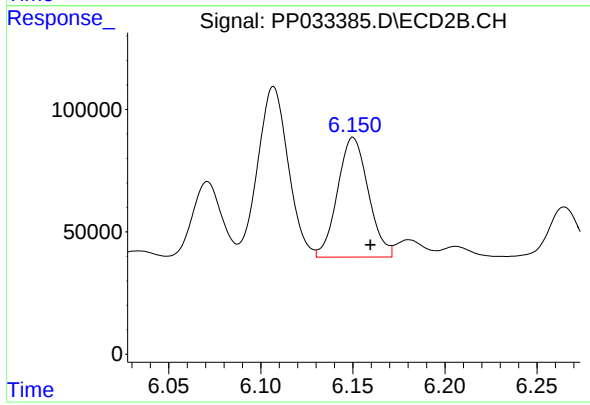

#25 AR-1248-5

R.T.: 6.150 min
Delta R.T.: -0.009 min
Response: 569264
Conc: 504.07 ng/ml