

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
 Data File : PP033386.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Feb 2021 20:17
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:25:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 23:16:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.724	3.997	2982645	1933870	48.639m	47.292
2) SA Decachlor...	10.537	9.255	2218302	1698199	50.924	50.692m
Target Compounds						
26) L6 AR-1254-1	6.923	6.106	869114	882466	462.904	461.746
27) L6 AR-1254-2	7.152	6.265	1383527	759979	471.911	463.508
28) L6 AR-1254-3	7.530	6.683	1446162	1249222	476.135	464.795
29) L6 AR-1254-4	7.824	6.923	1158514	742032	500.812	496.977
30) L6 AR-1254-5	8.250	7.349	1162096	1141992	480.248	471.628

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021721\
Data File : PP033386.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Feb 2021 20:17
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 23:16:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

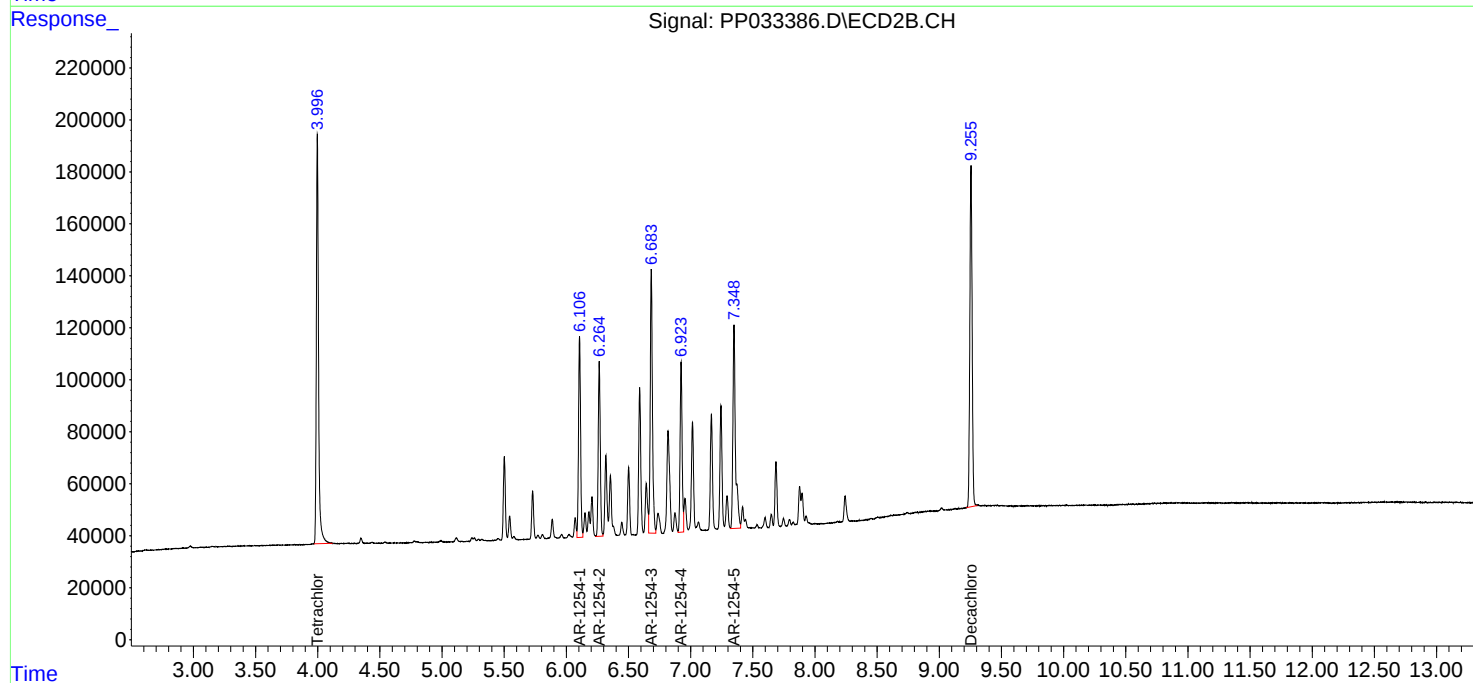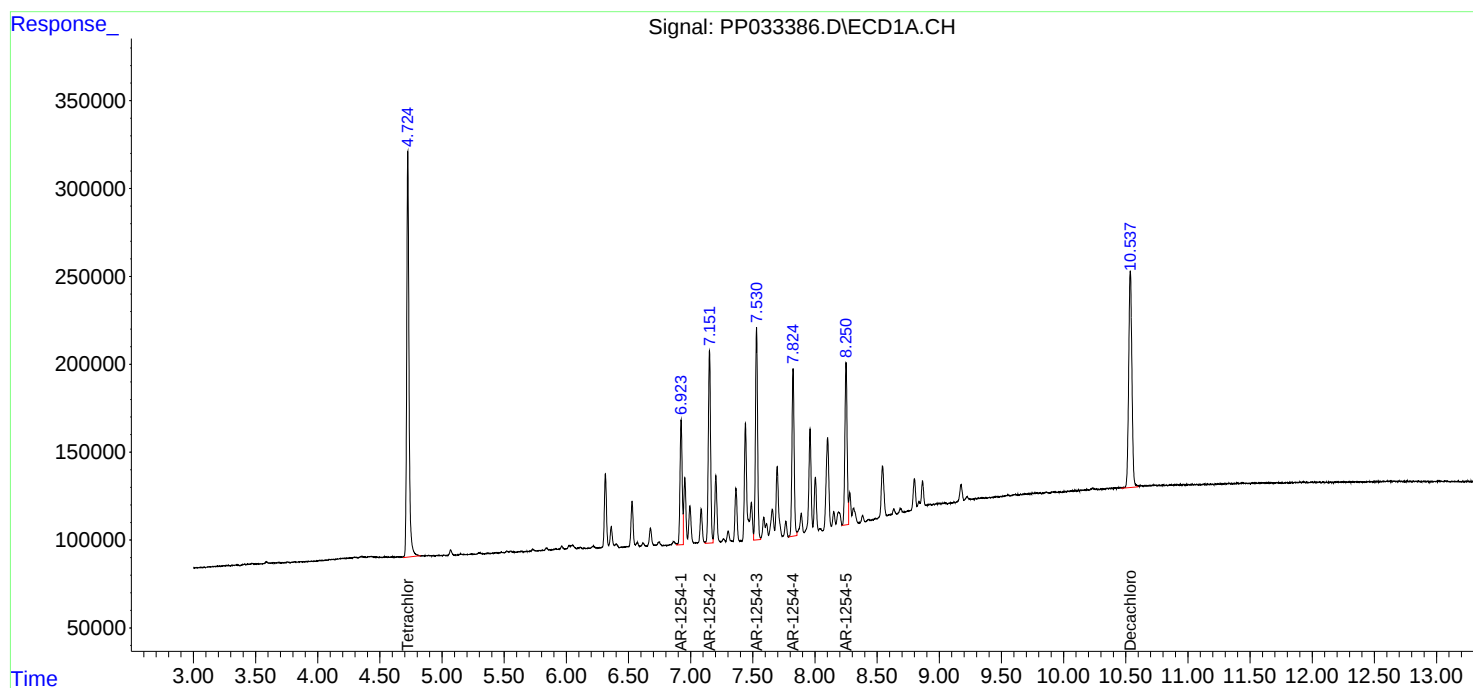

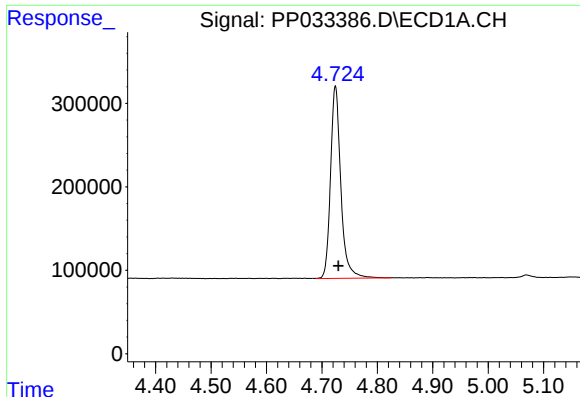


#1 Tetrachloro-m-xylene

R.T.: 4.724 min
Delta R.T.: -0.006 min
Response: 2982645
Conc: 48.64 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:44 AM

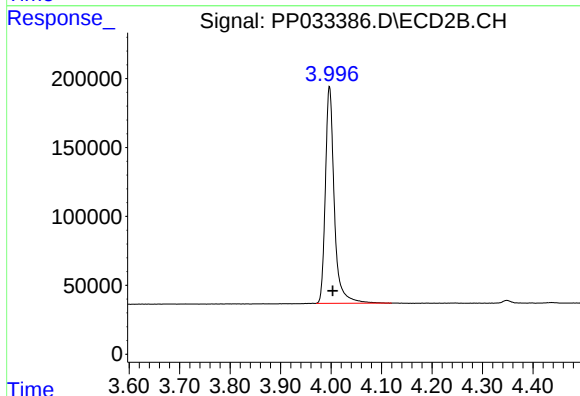


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 1933870
Conc: 47.29 ng/ml

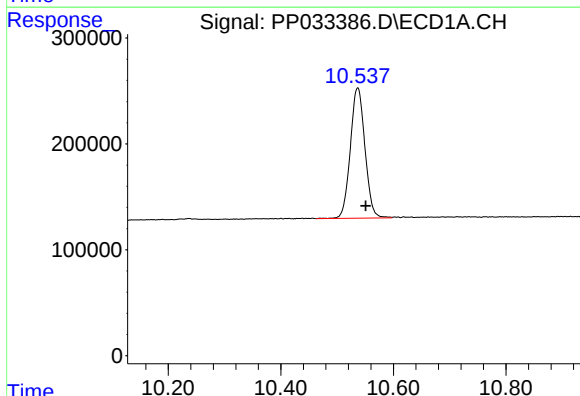


#2 Decachlorobiphenyl

R.T.: 10.537 min
Delta R.T.: -0.014 min
Response: 2218302
Conc: 50.92 ng/ml

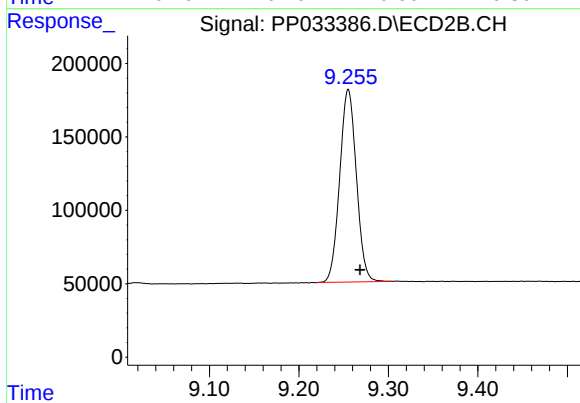

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.014 min
Response: 1698199
Conc: 50.69 ng/ml m

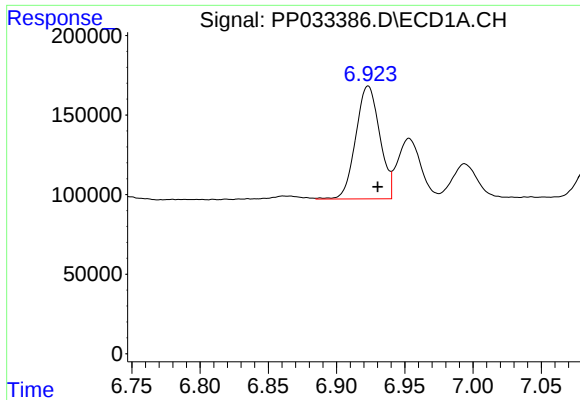


#26 AR-1254-1

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 869114
Conc: 462.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:44 AM

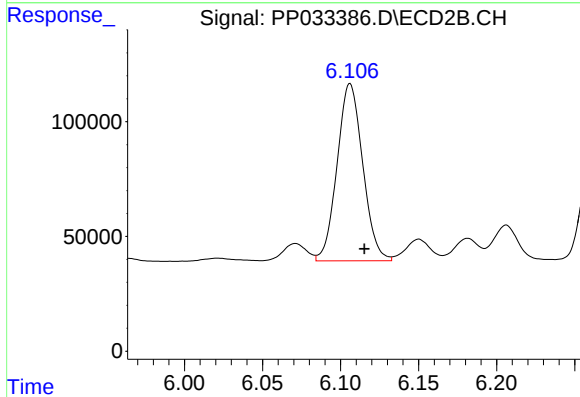


#26 AR-1254-1

R.T.: 6.106 min
Delta R.T.: -0.009 min
Response: 882466
Conc: 461.75 ng/ml

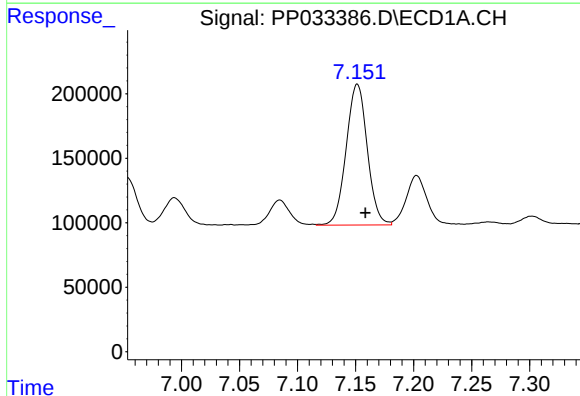


#27 AR-1254-2

R.T.: 7.152 min
Delta R.T.: -0.007 min
Response: 1383527
Conc: 471.91 ng/ml

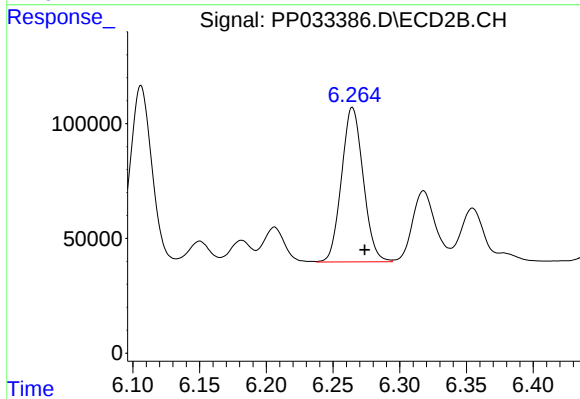

#27 AR-1254-2

R.T.: 6.265 min
Delta R.T.: -0.009 min
Response: 759979
Conc: 463.51 ng/ml

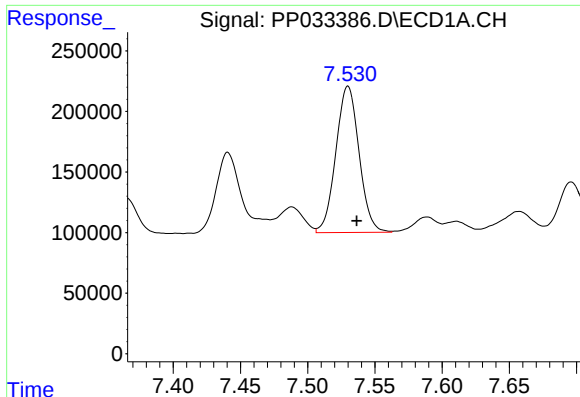


#28 AR-1254-3

R.T.: 7.530 min
Delta R.T.: -0.007 min
Response: 1446162
Conc: 476.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:44 AM

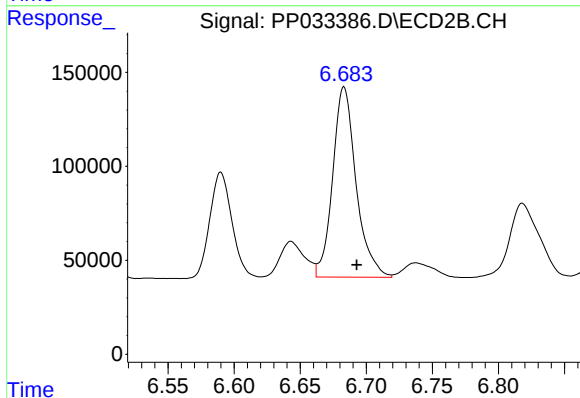


#28 AR-1254-3

R.T.: 6.683 min
Delta R.T.: -0.010 min
Response: 1249222
Conc: 464.80 ng/ml

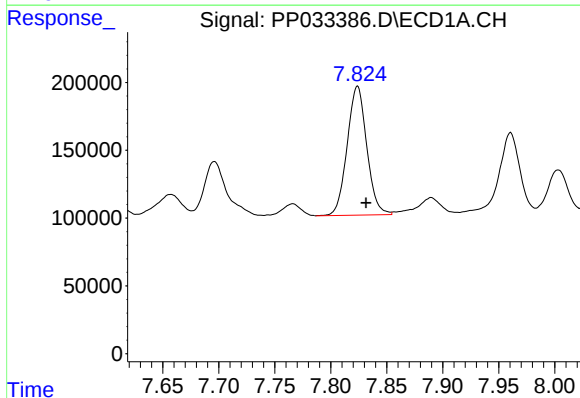


#29 AR-1254-4

R.T.: 7.824 min
Delta R.T.: -0.008 min
Response: 1158514
Conc: 500.81 ng/ml

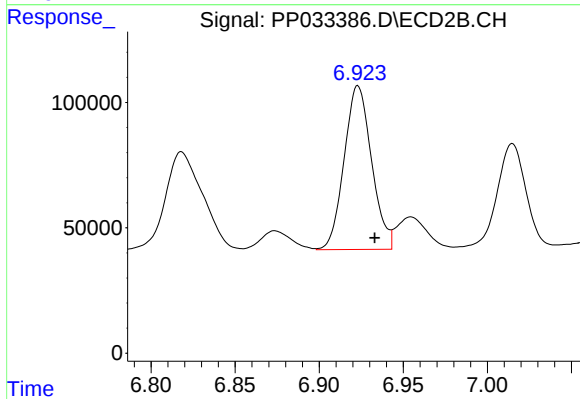

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.010 min
Response: 742032
Conc: 496.98 ng/ml

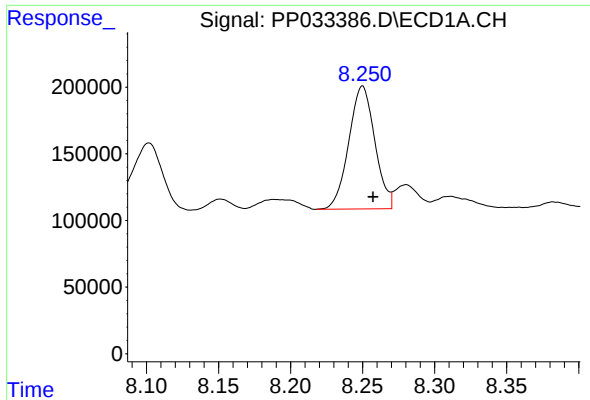


#30 AR-1254-5

R.T.: 8.250 min
Delta R.T.: -0.007 min
Response: 1162096
Conc: 480.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
2/19/2021 9:25:44 AM

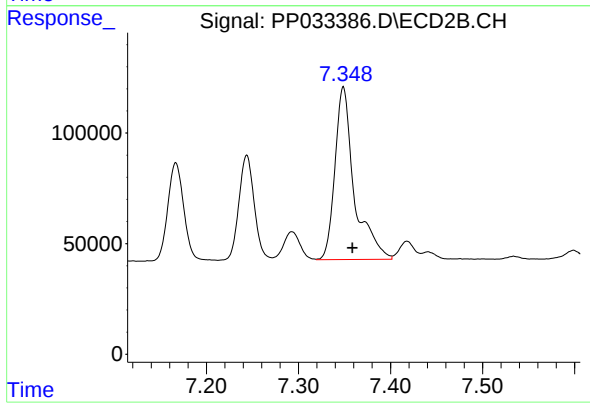

#30 AR-1254-5

R.T.: 7.349 min
Delta R.T.: -0.010 min
Response: 1141992
Conc: 471.63 ng/ml