

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021722\
 Data File : PP043785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2022 11:00
 Operator : YP\AJ
 Sample : N1553-03 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-02A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/18/2022
 Supervised By :Ankita Jodhani 02/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:35:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.918	3.172	2631374	3048942	1.190m	1.623m#
2) SA Decachlor...	10.061	8.547	2293842	2688388	1.931m	1.657

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021722\
Data File : PP043785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2022 11:00
Operator : YP\AJ
Sample : N1553-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
LAW-2022-02A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2022
Supervised By :Ankita Jodhani 02/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:35:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

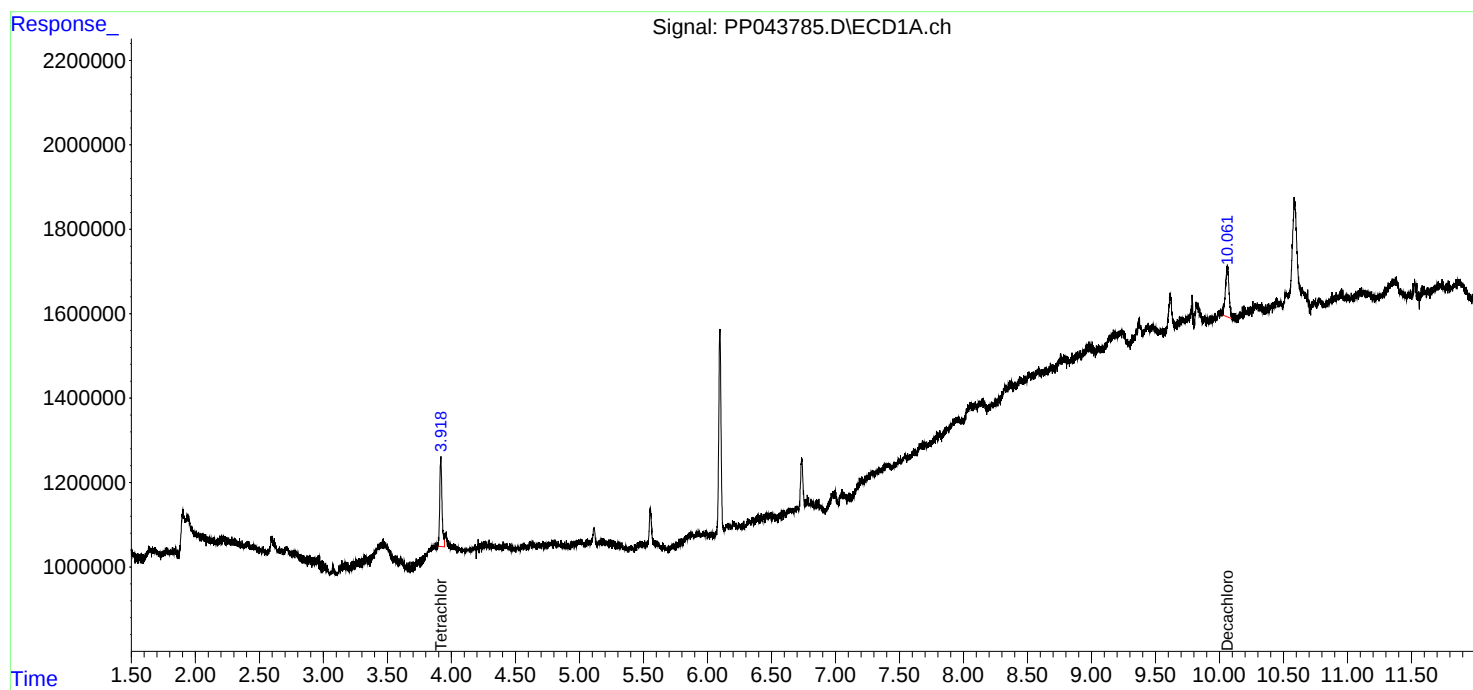

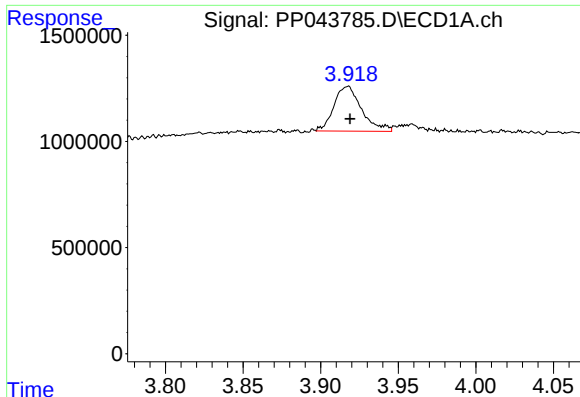


#1 Tetrachloro-m-xylene

R.T.: 3.918 min
Delta R.T.: -0.001 min
Response: 2631374
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-02A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2022
Supervised By :Ankita Jodhani 02/18/2022

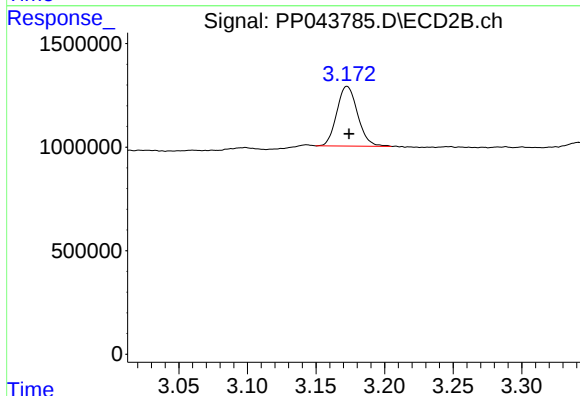


#1 Tetrachloro-m-xylene

R.T.: 3.172 min
Delta R.T.: -0.002 min
Response: 3048942
Conc: 1.62 ng/ml m

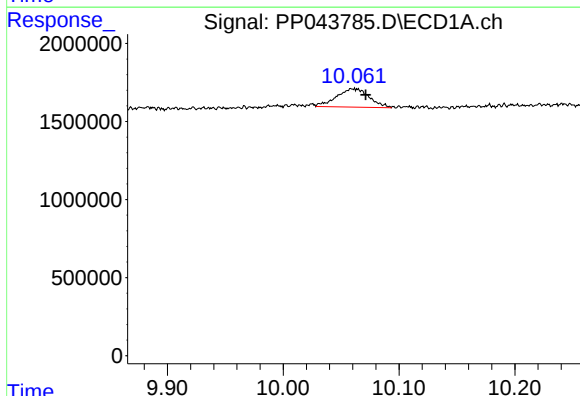

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: -0.010 min
Response: 2293842
Conc: 1.93 ng/ml m

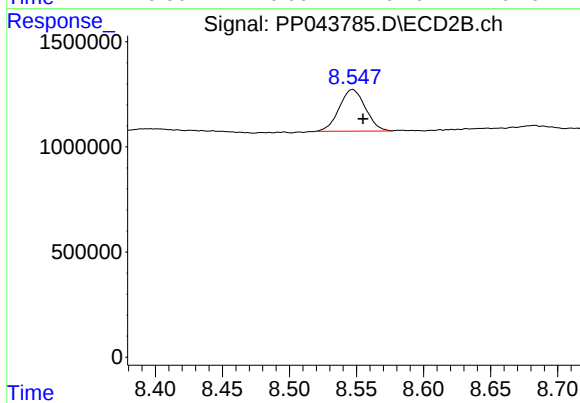

#2 Decachlorobiphenyl

R.T.: 8.547 min
Delta R.T.: -0.008 min
Response: 2688388
Conc: 1.66 ng/ml