

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021722\
 Data File : PP043800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2022 15:03
 Operator : YP\AJ
 Sample : N1534-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NAPL-SOCK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/18/2022
 Supervised By :Ankita Jodhani 02/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:41:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.923	3.160	134.3E6	1705.7E6	60.725m	908.138 #
2) SA Decachlor...	10.062	8.556	38857120	72692882	32.711	44.806 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021722\
Data File : PP043800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2022 15:03
Operator : YP\AJ
Sample : N1534-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NAPL-SOCK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2022
Supervised By :Ankita Jodhani 02/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:41:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

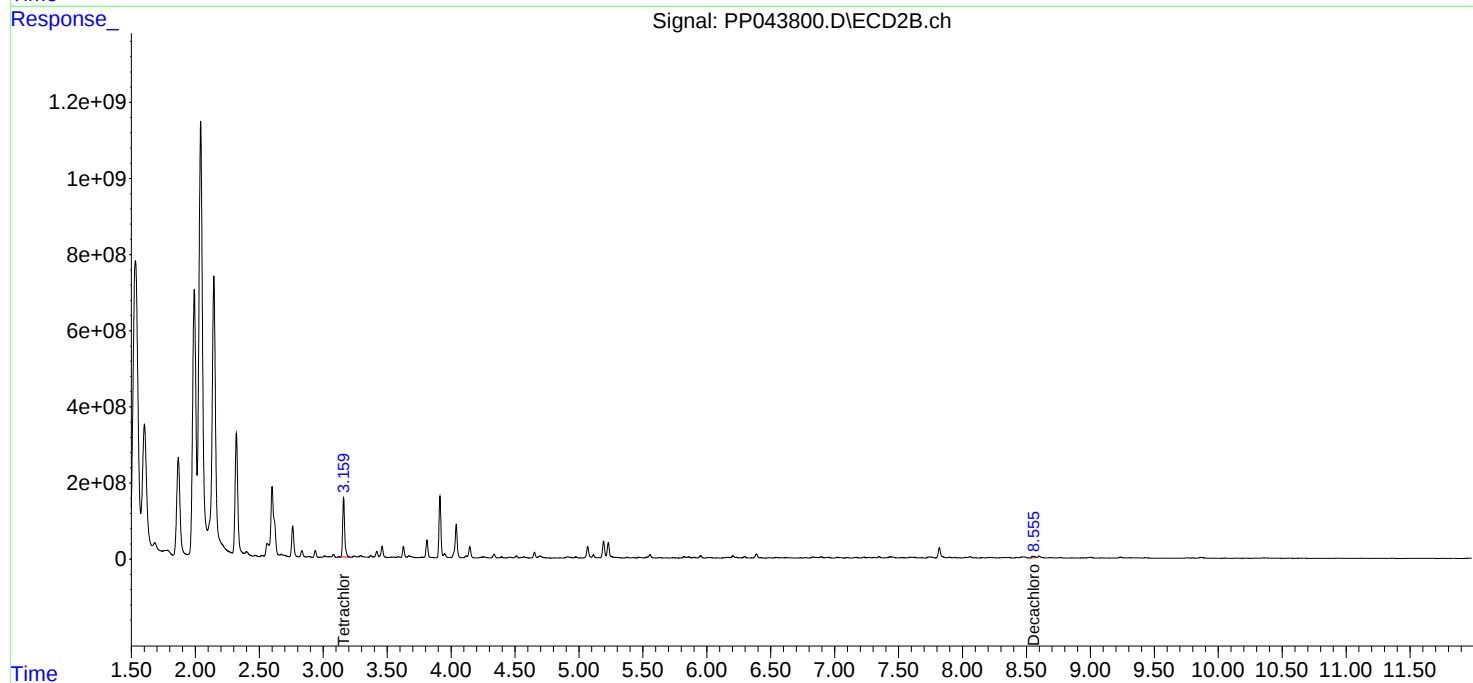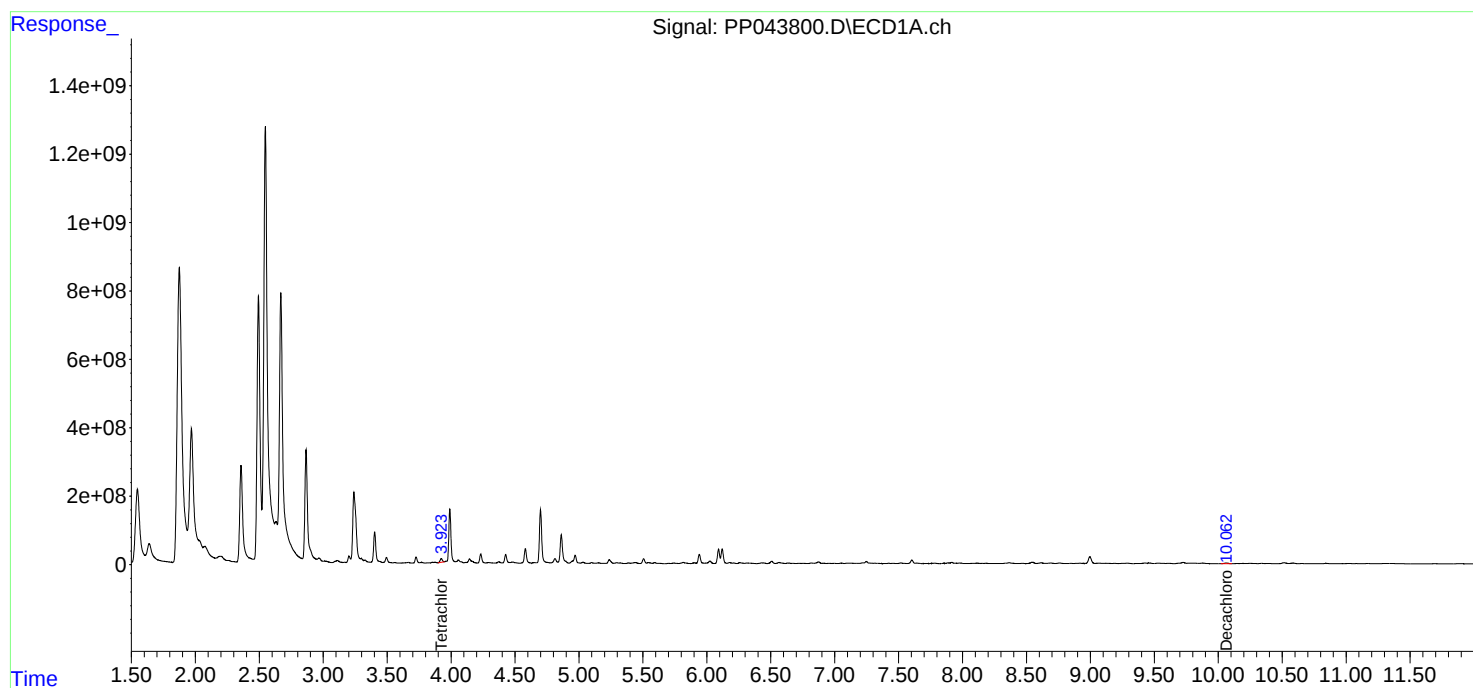

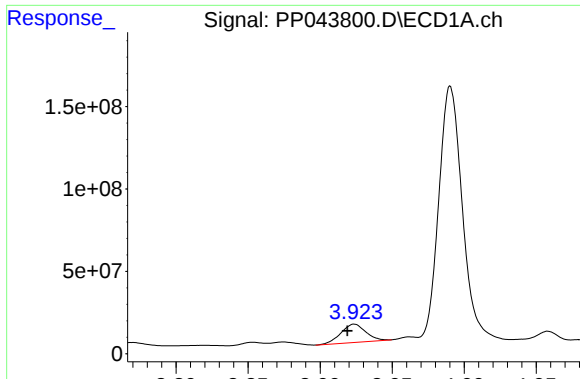


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: 0.004 min
Response: 134265021
Conc: 60.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
NAPL-SOCK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2022
Supervised By :Ankita Jodhani 02/18/2022

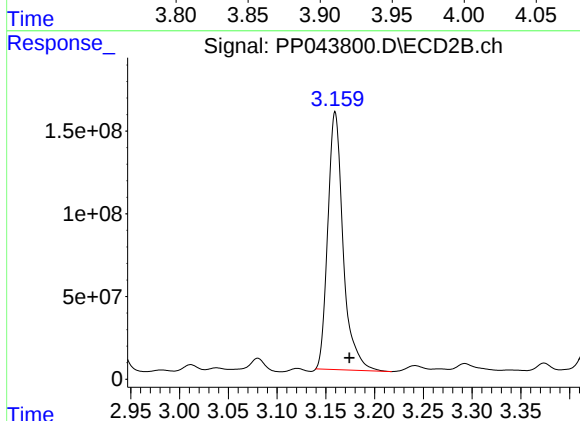


#1 Tetrachloro-m-xylene

R.T.: 3.160 min
Delta R.T.: -0.015 min
Response: 1705727467
Conc: 908.14 ng/ml

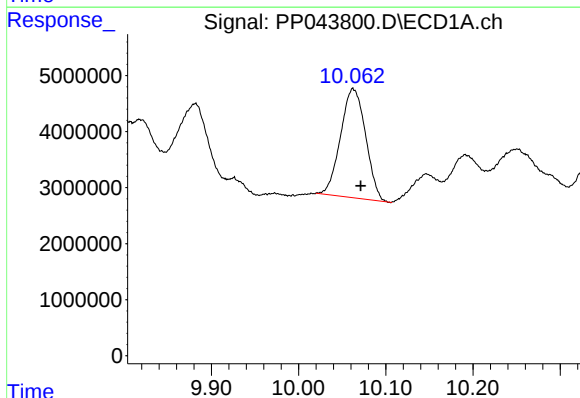

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.009 min
Response: 38857120
Conc: 32.71 ng/ml

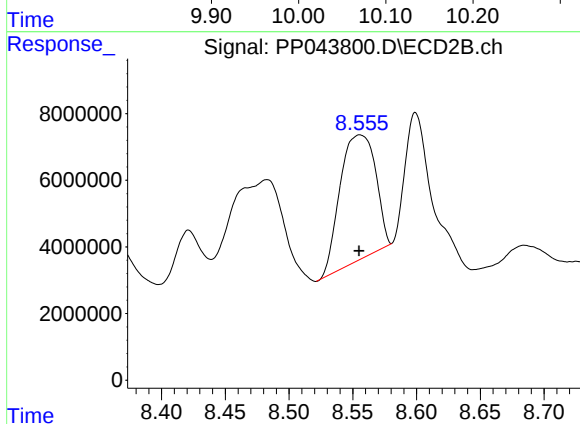

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: 0.000 min
Response: 72692882
Conc: 44.81 ng/ml