

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021725\
 Data File : PP069793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2025 18:13
 Operator : YP\AJ
 Sample : Q1371-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-25-0013

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/18/2025
 Supervised By :Ankita Jodhani 02/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 02:33:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.831	60701742	20481742	42.405m	22.948m#
2) SA Decachlor...	10.255	8.893	10996855	10726442	10.062m	9.590

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021725\
Data File : PP069793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2025 18:13
Operator : YP\AJ
Sample : Q1371-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-25-0013


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2025
Supervised By :Ankita Jodhani 02/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 02:33:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

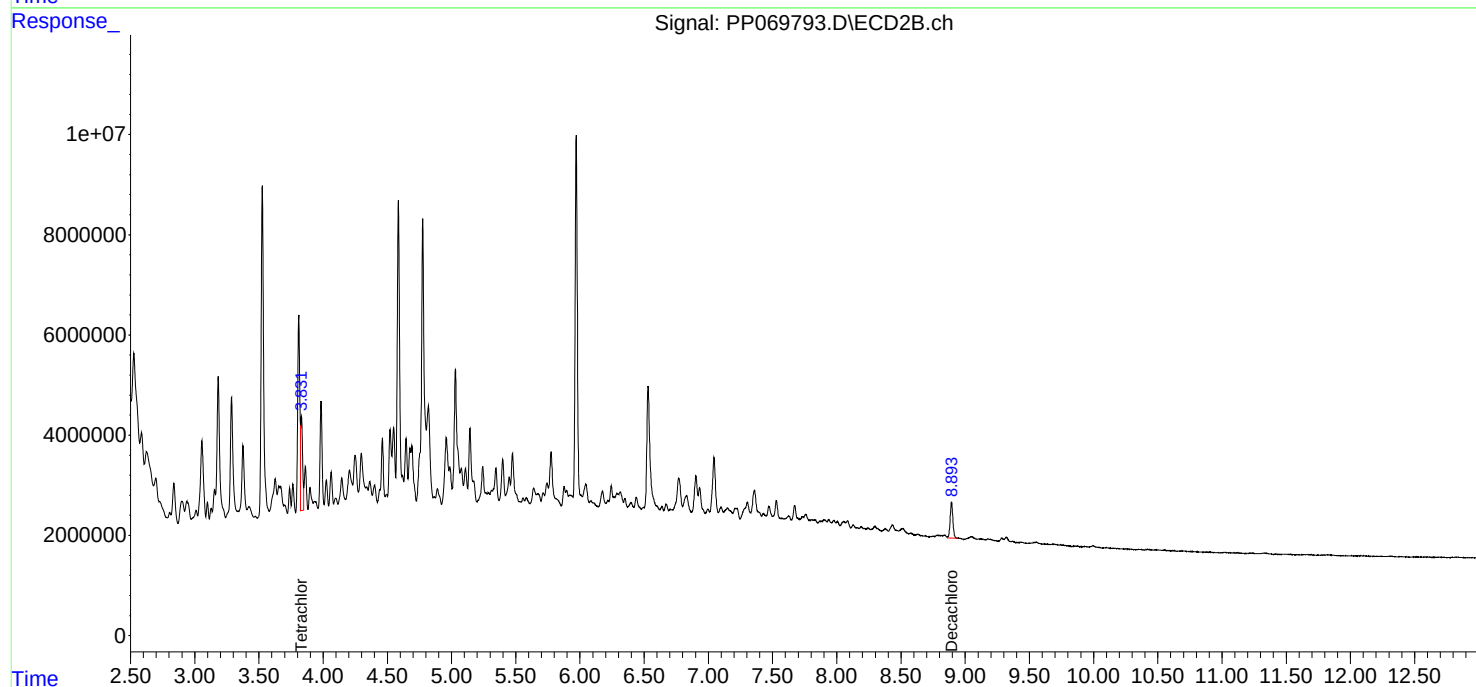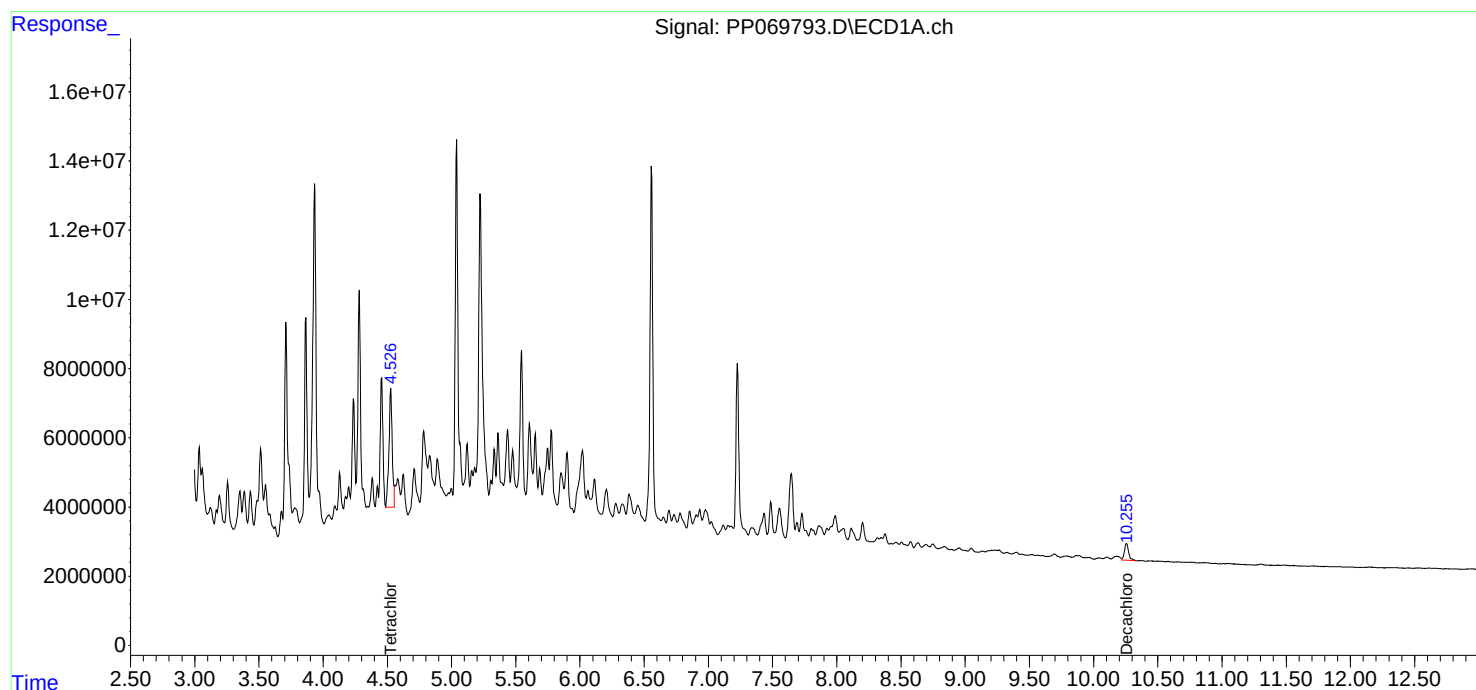

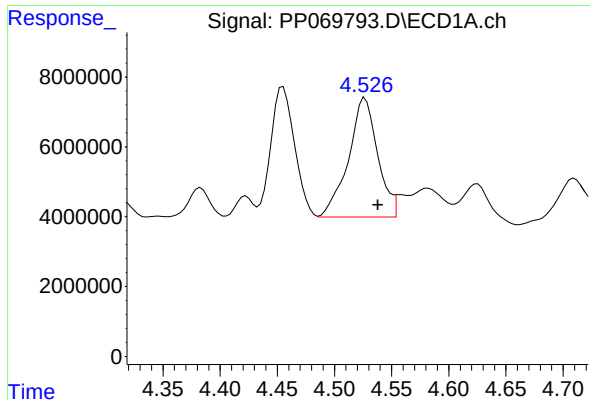


#1 Tetrachloro-m-xylene

R.T.: 4.526 min
Delta R.T.: -0.013 min
Response: 60701742
Conc: 42.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-25-0013


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/18/2025
Supervised By :Ankita Jodhani 02/18/2025

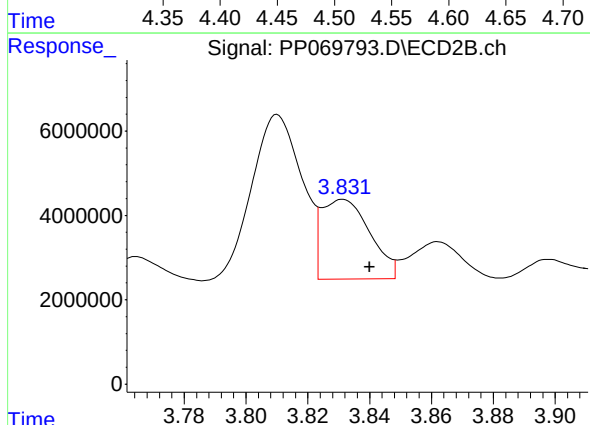


#1 Tetrachloro-m-xylene

R.T.: 3.831 min
Delta R.T.: -0.009 min
Response: 20481742
Conc: 22.95 ng/ml

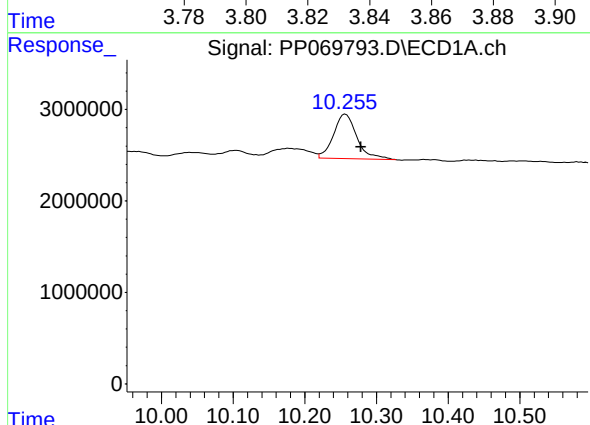

#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: -0.023 min
Response: 10996855
Conc: 10.06 ng/ml

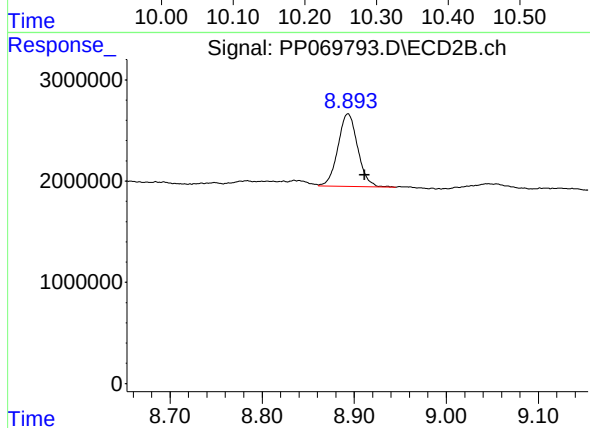

#2 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.018 min
Response: 10726442
Conc: 9.59 ng/ml