

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
 Data File : PP033388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2021 8:49
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 12:55:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
2)	SA Decachlor...	10.539	0.000	77363	0	1.776	N.D. #
Target Compounds							
20)	L4 AR-1242-5	0.000	6.130	0	41586	N.D.	49.251 #
24)	L5 AR-1248-4	6.938f	0.000	221296	0	128.612	N.D. #
25)	L5 AR-1248-5	0.000	6.130f	0	41586	N.D.	36.824 #
26)	L6 AR-1254-1	6.938	6.130	221296	41586	117.866	21.760 #
28)	L6 AR-1254-3	7.543	0.000	671763	0	221.171	N.D. #
29)	L6 AR-1254-4	7.829	0.000	371853	0	160.747	N.D. #
30)	L6 AR-1254-5	8.231f	0.000	37877	0	15.653	N.D. #
31)	L7 AR-1260-1	7.714	0.000	1215516	0	555.197	N.D. #
34)	L7 AR-1260-4	8.564	0.000	32004	0	13.100	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
Data File : PP033388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2021 8:49
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 12:55:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

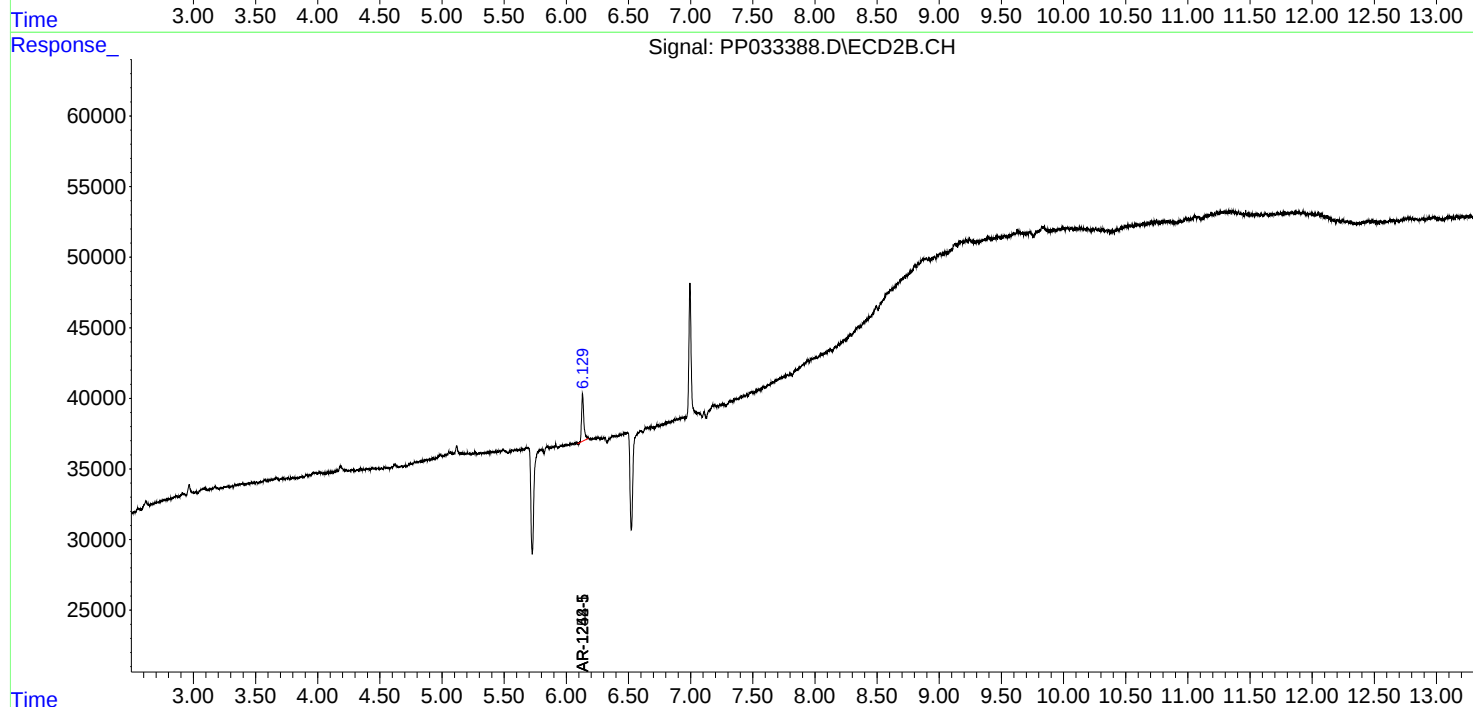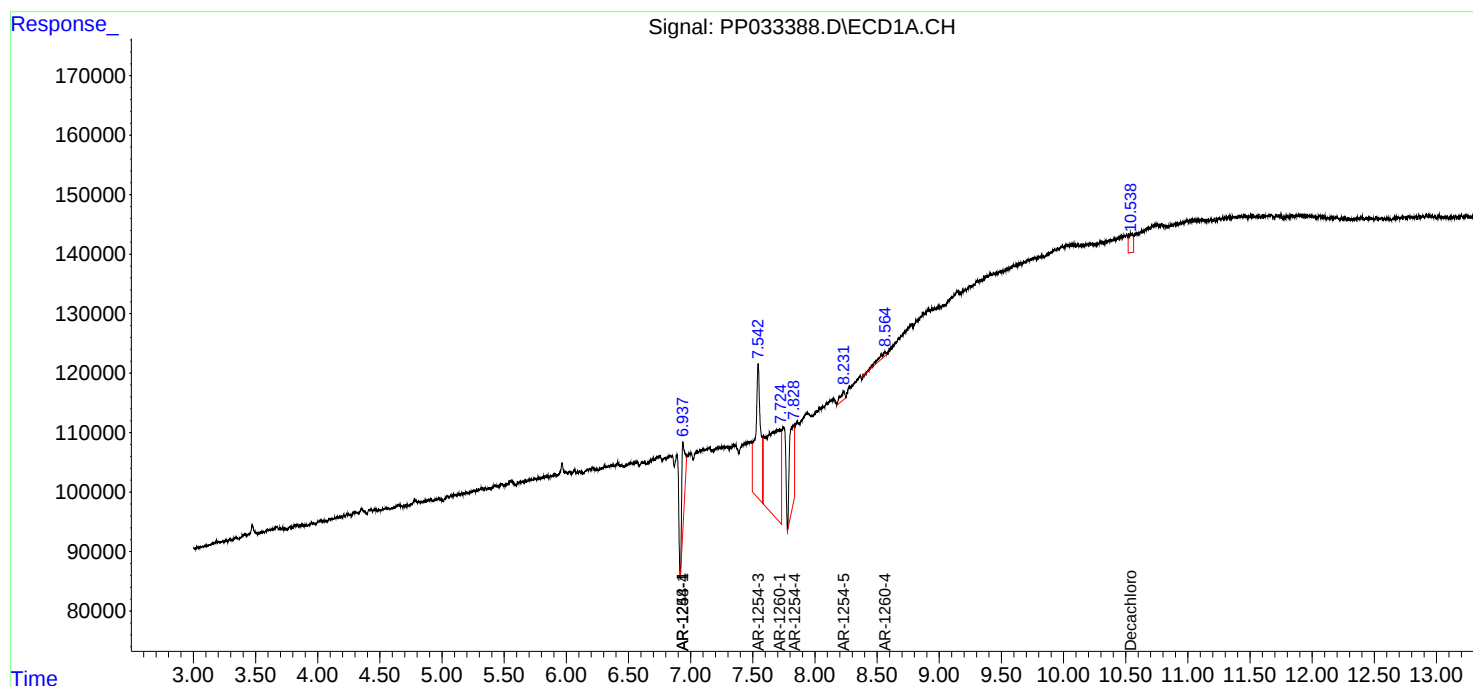


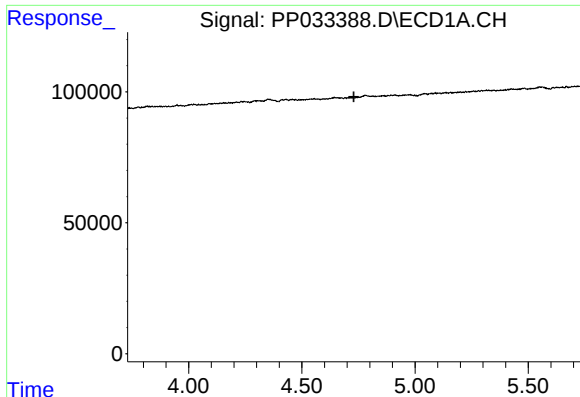

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.730 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

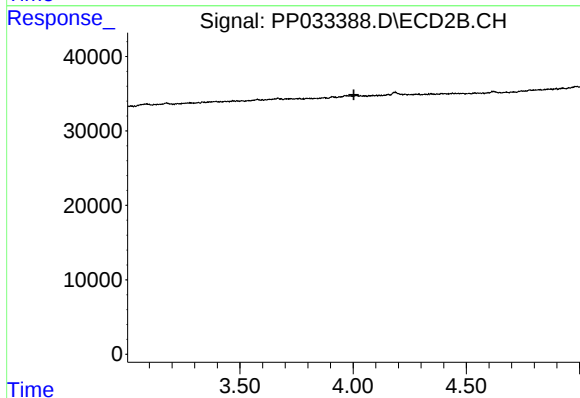


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.003 min
Response: 0
Conc: N.D.

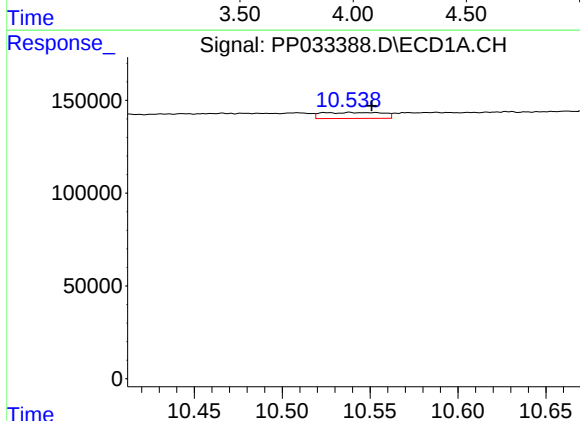


#2 Decachlorobiphenyl

R.T.: 10.539 min
Delta R.T.: -0.012 min
Response: 77363
Conc: 1.78 ng/ml

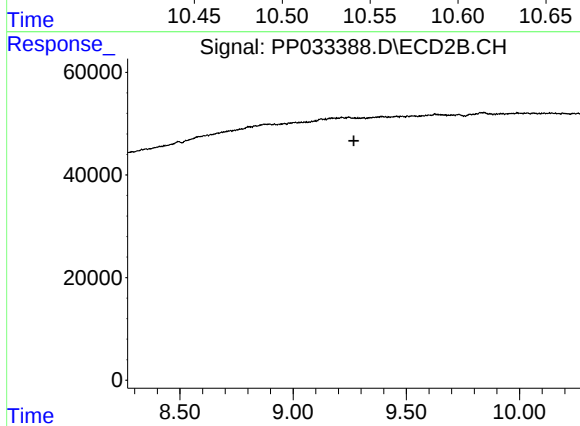

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.268 min
Response: 0
Conc: N.D.

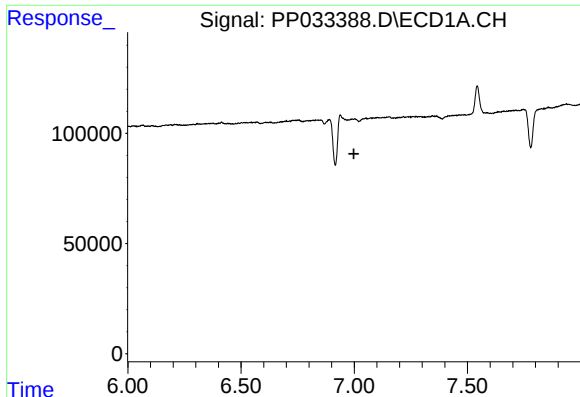

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

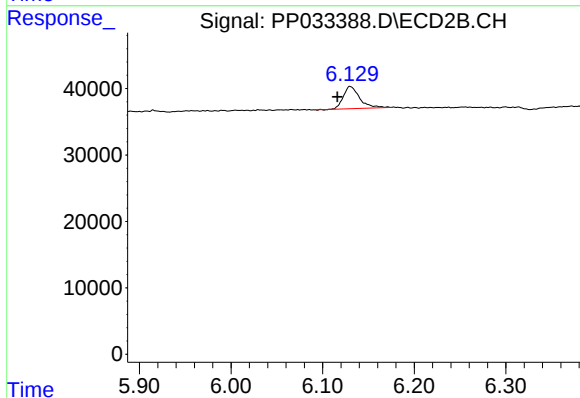


#20 AR-1242-5

R.T.: 6.130 min
Delta R.T.: 0.014 min
Response: 41586
Conc: 49.25 ng/ml

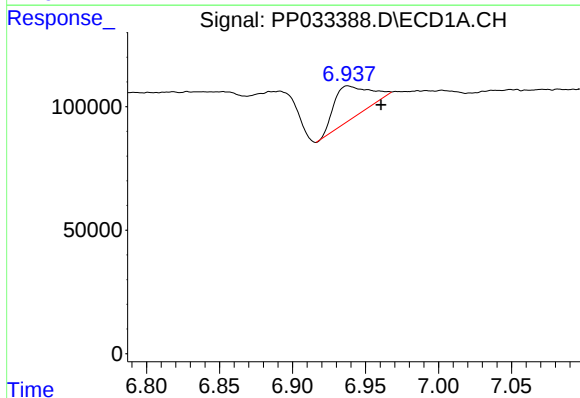


#24 AR-1248-4

R.T.: 6.938 min
Delta R.T.: -0.023 min
Response: 221296
Conc: 128.61 ng/ml

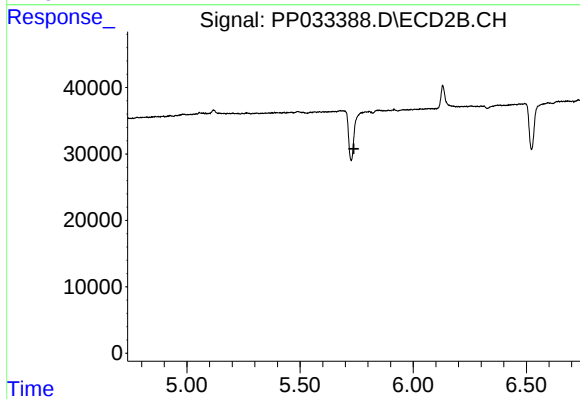

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.738 min
Response: 0
Conc: N.D.

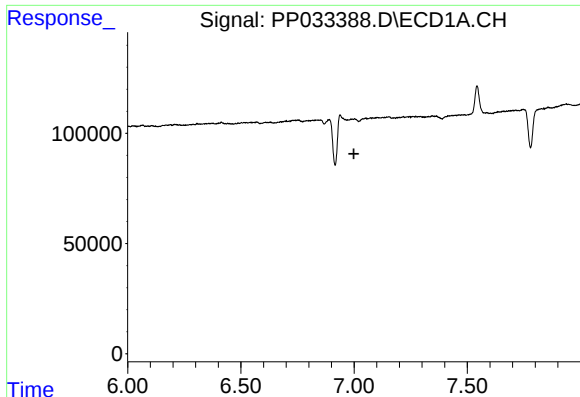

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

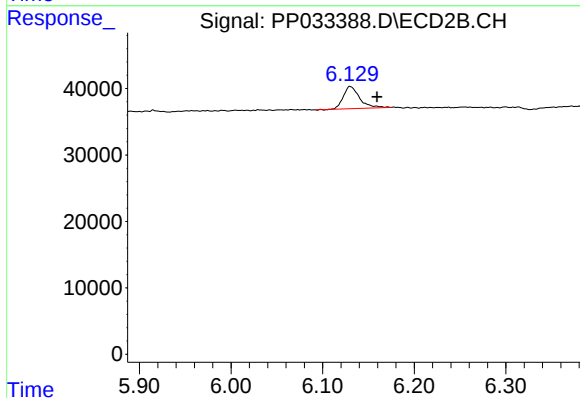


#25 AR-1248-5

R.T.: 6.130 min
Delta R.T.: -0.029 min
Response: 41586
Conc: 36.82 ng/ml

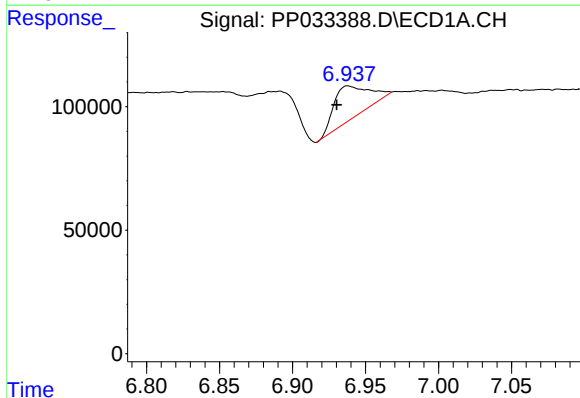


#26 AR-1254-1

R.T.: 6.938 min
Delta R.T.: 0.008 min
Response: 221296
Conc: 117.87 ng/ml

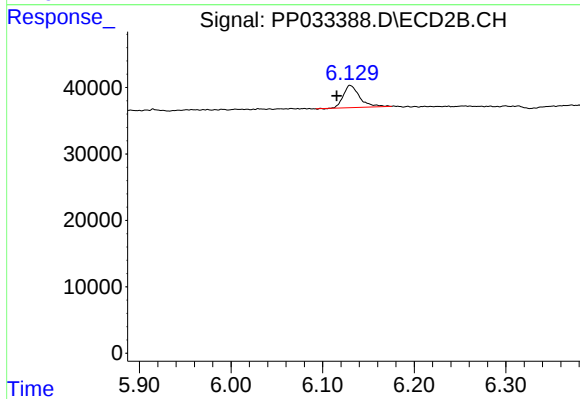

#26 AR-1254-1


R.T.: 6.130 min
Delta R.T.: 0.015 min
Response: 41586
Conc: 21.76 ng/ml

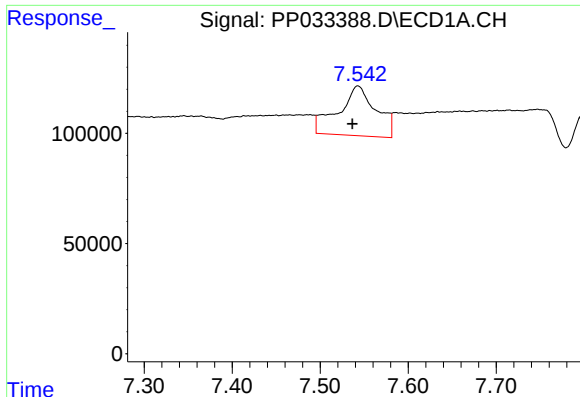

#28 AR-1254-3


R.T.: 7.543 min
Delta R.T.: 0.006 min
Response: 671763
Conc: 221.17 ng/ml

Instrument :
ECD_P
ClientSampleId :

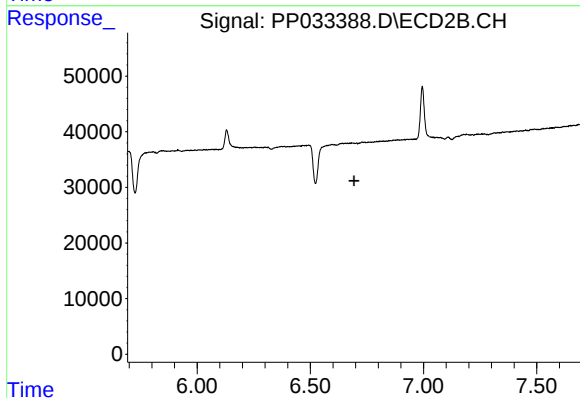


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

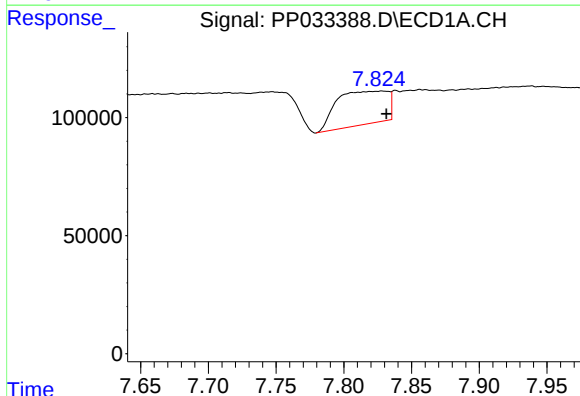


#29 AR-1254-4

R.T.: 7.829 min
Delta R.T.: -0.003 min
Response: 371853
Conc: 160.75 ng/ml

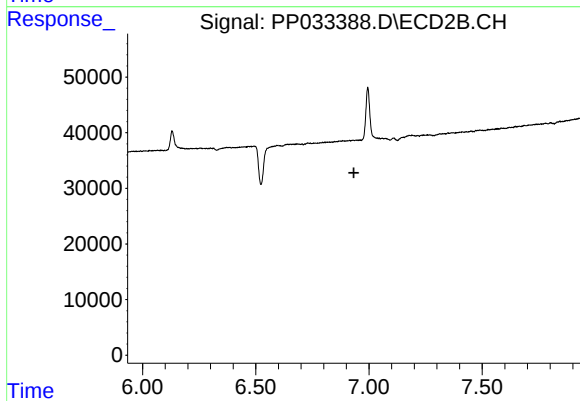

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

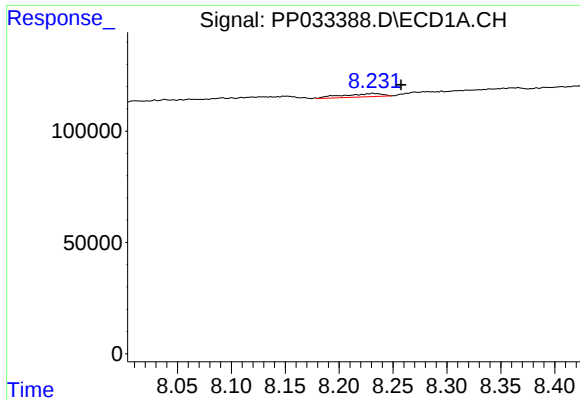

#30 AR-1254-5


R.T.: 8.231 min
Delta R.T.: -0.026 min
Response: 37877
Conc: 15.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

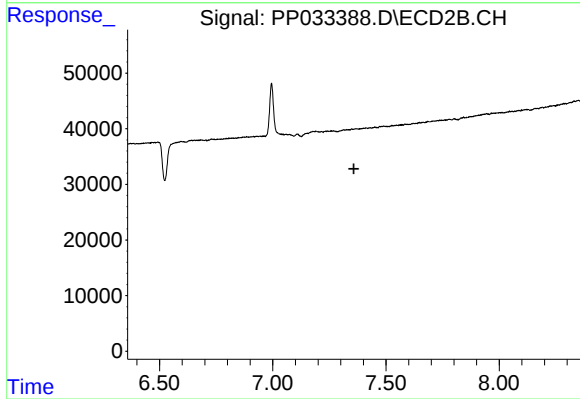


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

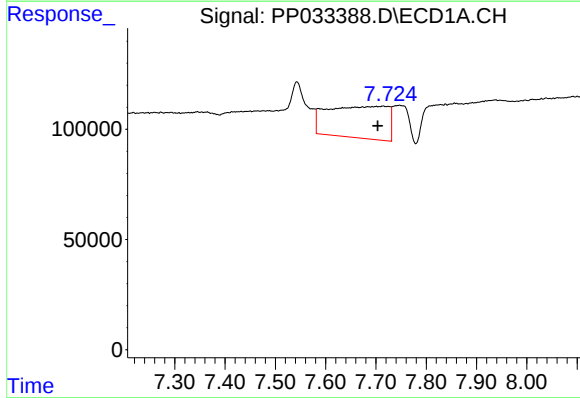


#31 AR-1260-1

R.T.: 7.714 min
Delta R.T.: 0.010 min
Response: 1215516
Conc: 555.20 ng/ml

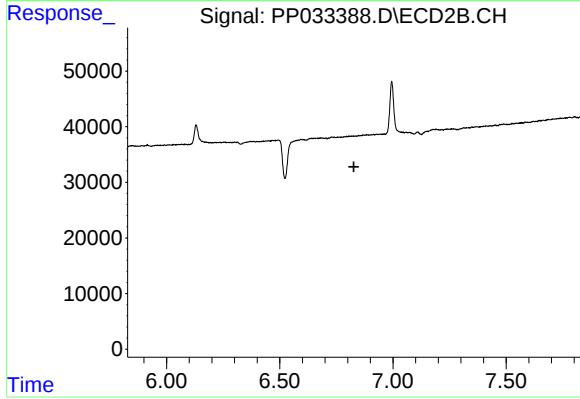

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.828 min
Response: 0
Conc: N.D.

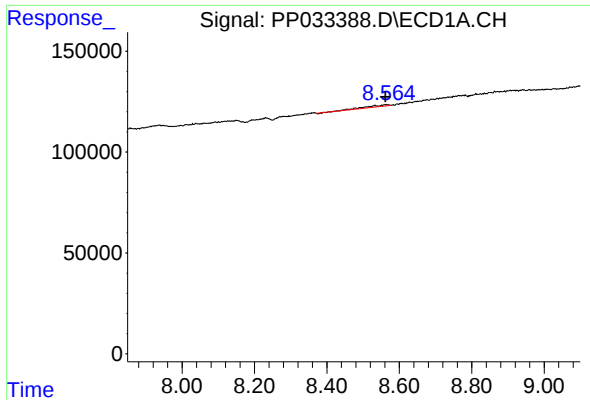

#34 AR-1260-4

R.T.: 8.564 min
Delta R.T.: 0.002 min
Response: 32004
Conc: 13.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

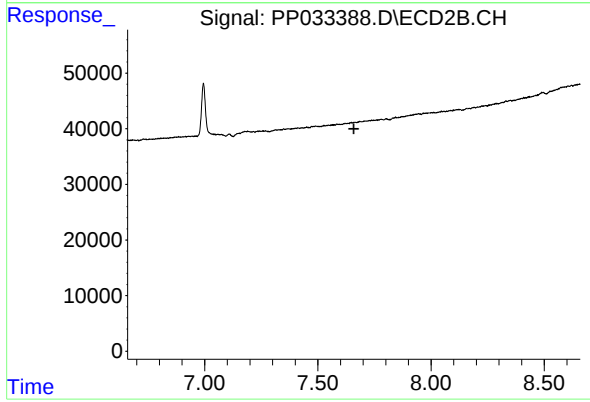

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.