

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
 Data File : PP033397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2021 16:06
 Operator : DD\AJ
 Sample : PB134714BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 00:30:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.727	3.998	1721407	971781	28.071	23.765
2)	SA Decachlor...	10.542	9.257	1247726	901093	28.643	26.898
Target Compounds							
9)	L2 AR-1221-2	5.072	0.000	24785	0	53.279	N.D. #
20)	L4 AR-1242-5	6.974f	0.000	2211	0	2.128	N.D. #
24)	L5 AR-1248-4	6.955	0.000	9309	0	5.410	N.D. #
25)	L5 AR-1248-5	6.974f	0.000	2211	0	1.270	N.D. #
26)	L6 AR-1254-1	6.942	0.000	15650	0	8.335	N.D. #
28)	L6 AR-1254-3	7.545	0.000	33945	0	11.176	N.D. #
29)	L6 AR-1254-4	7.806f	0.000	5557	0	2.402	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
Data File : PP033397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2021 16:06
Operator : DD\AJ
Sample : PB134714BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 00:30:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

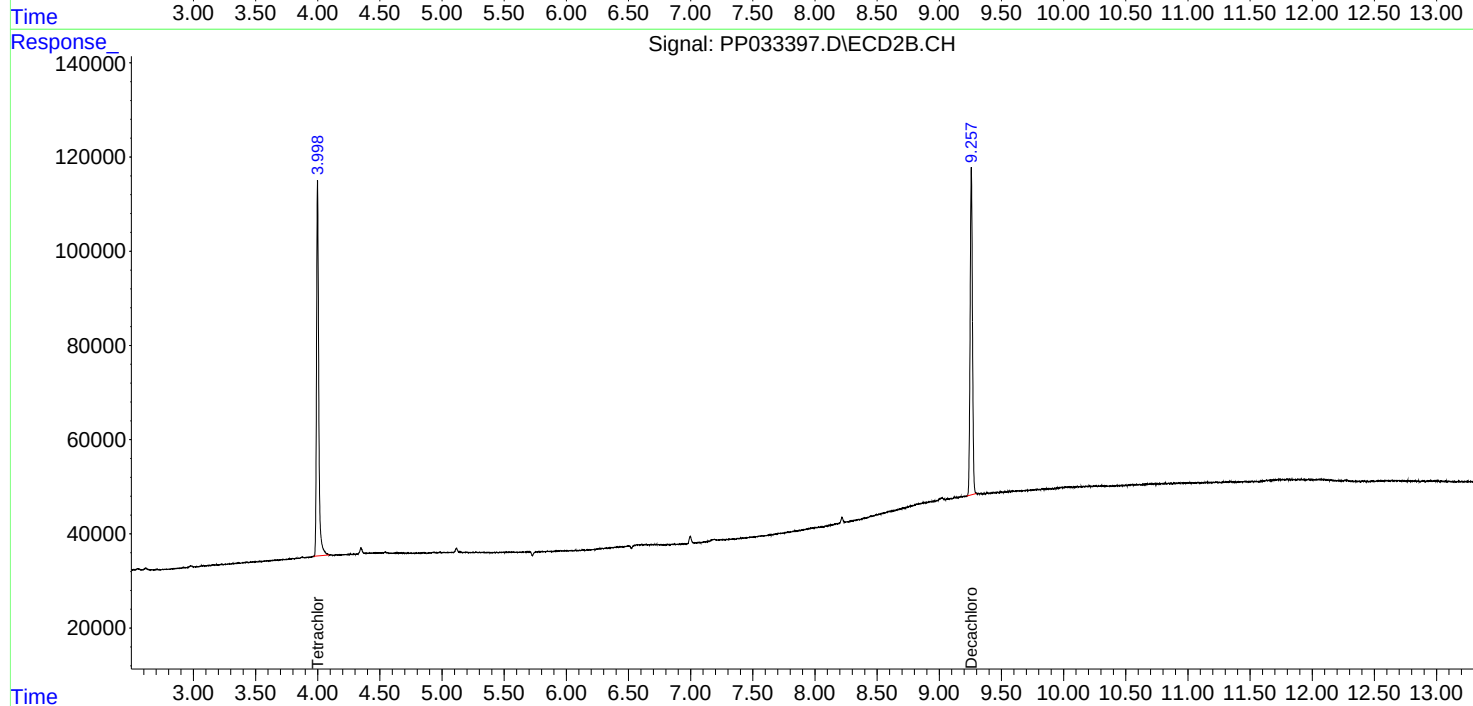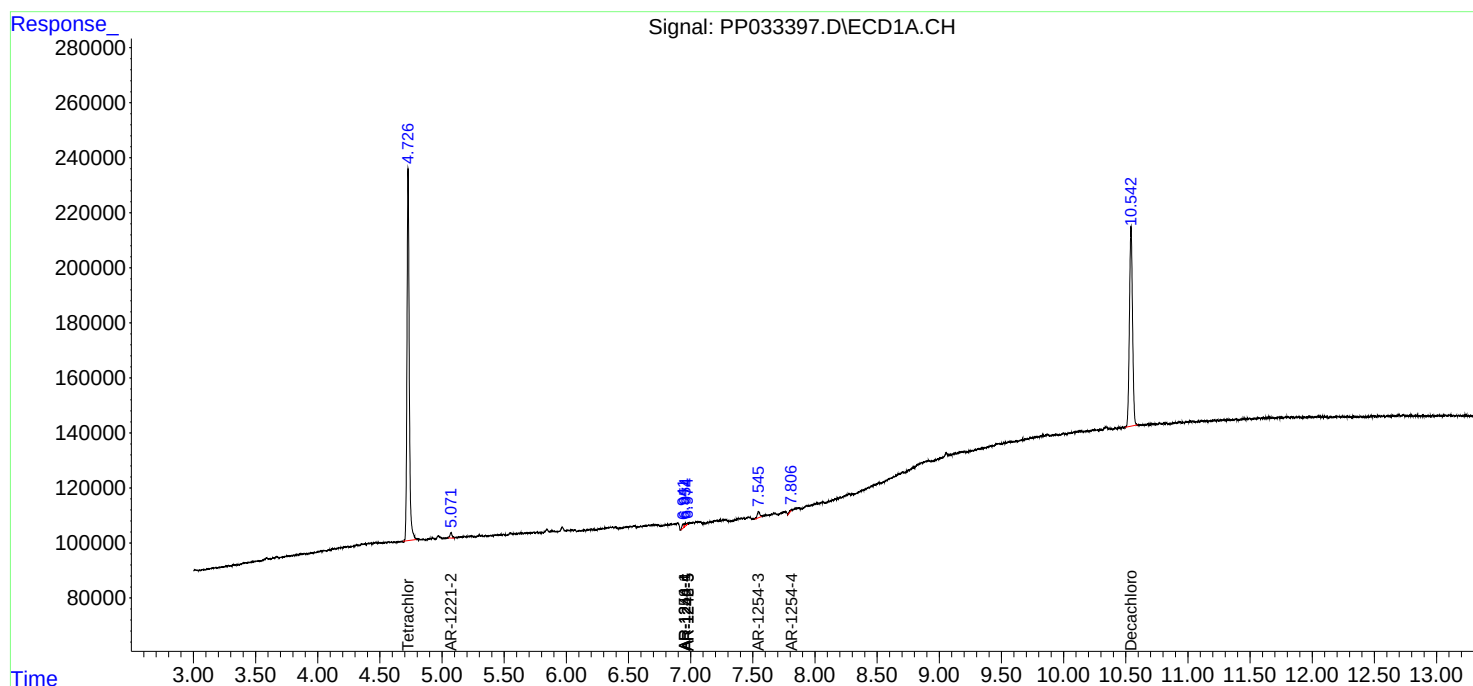


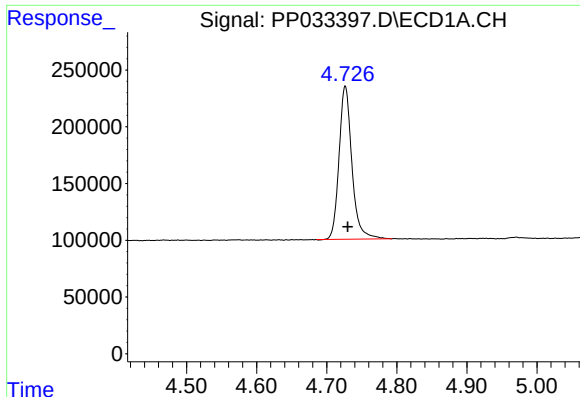

#1 Tetrachloro-m-xylene


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 1721407
Conc: 28.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

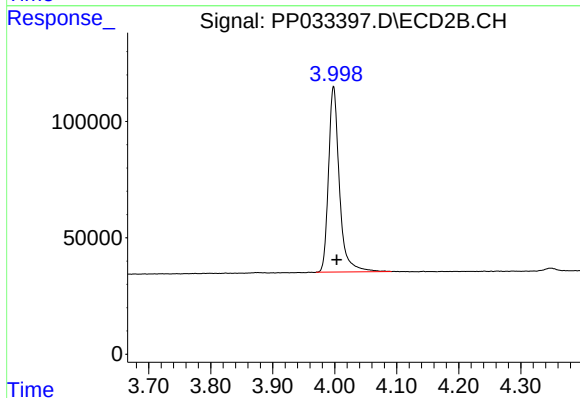


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 971781
Conc: 23.76 ng/ml

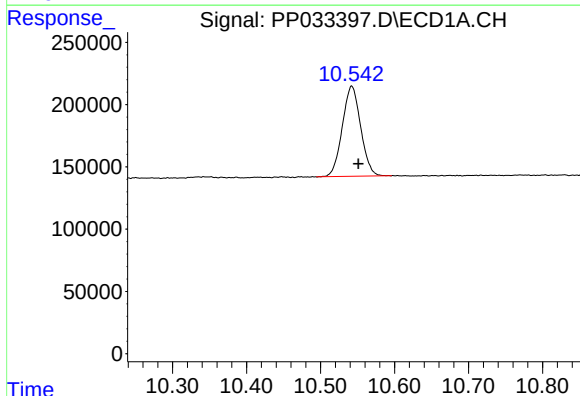


#2 Decachlorobiphenyl

R.T.: 10.542 min
Delta R.T.: -0.009 min
Response: 1247726
Conc: 28.64 ng/ml

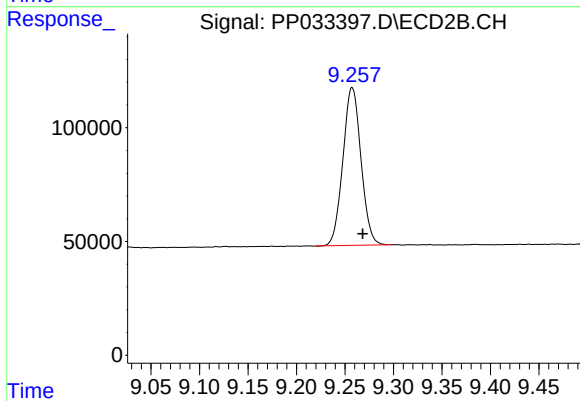

#2 Decachlorobiphenyl


R.T.: 9.257 min
Delta R.T.: -0.011 min
Response: 901093
Conc: 26.90 ng/ml

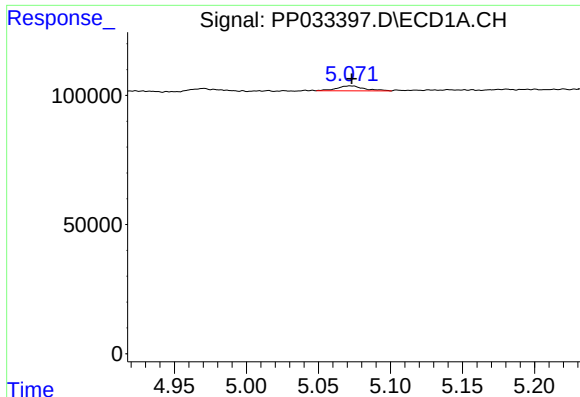

#9 AR-1221-2


R.T.: 5.072 min
Delta R.T.: -0.001 min
Response: 24785
Conc: 53.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

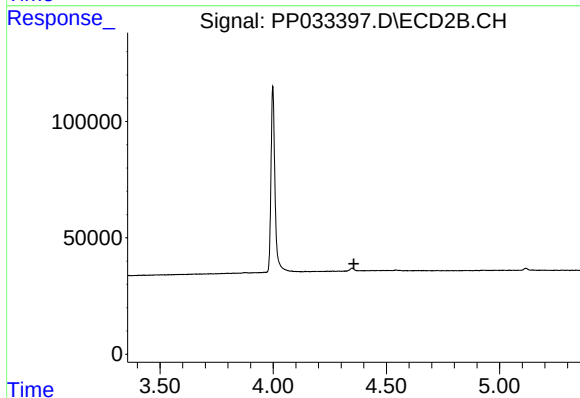


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.356 min
Response: 0
Conc: N.D.

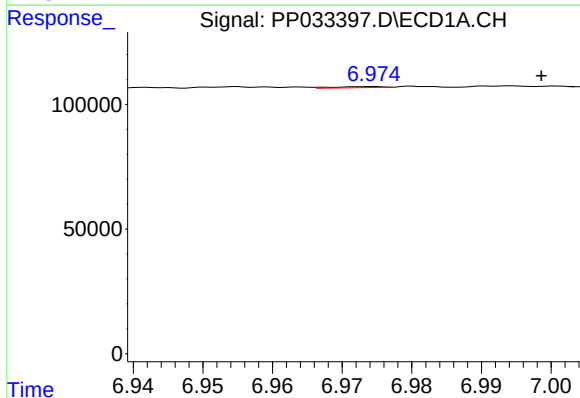


#20 AR-1242-5

R.T.: 6.974 min
Delta R.T.: -0.024 min
Response: 2211
Conc: 2.13 ng/ml

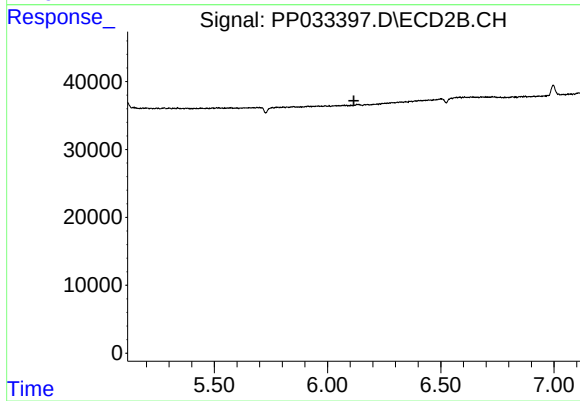

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.116 min
Response: 0
Conc: N.D.

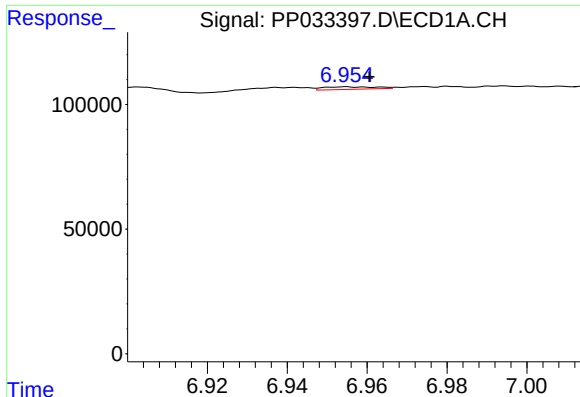

#24 AR-1248-4


R.T.: 6.955 min
Delta R.T.: -0.006 min
Response: 9309
Conc: 5.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

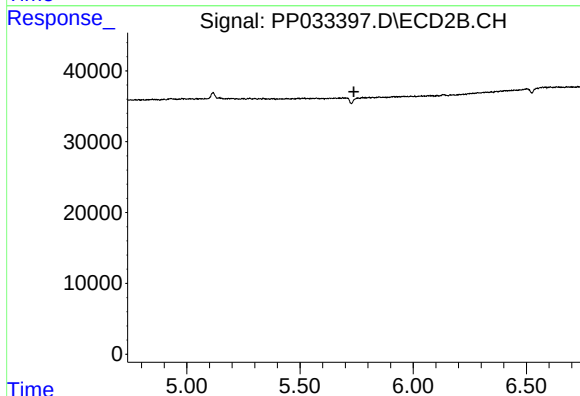


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.738 min
Response: 0
Conc: N.D.

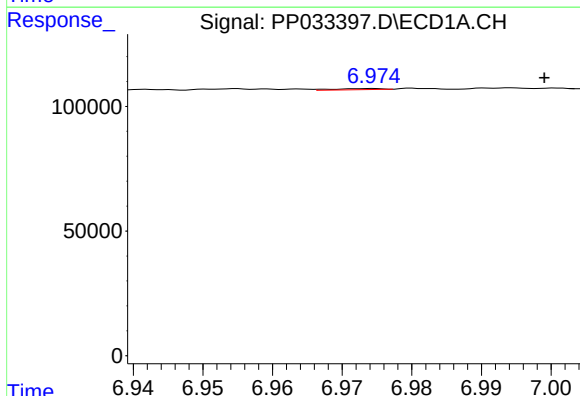


#25 AR-1248-5

R.T.: 6.974 min
Delta R.T.: -0.025 min
Response: 2211
Conc: 1.27 ng/ml

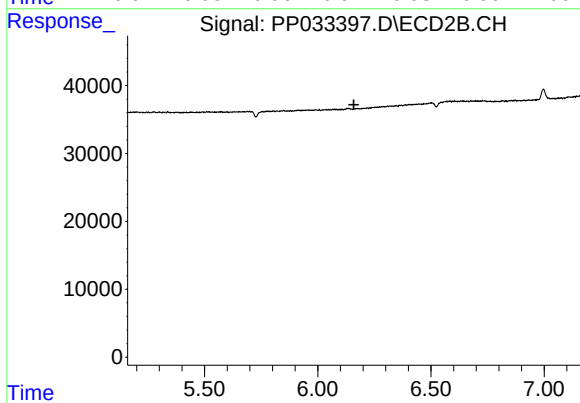

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

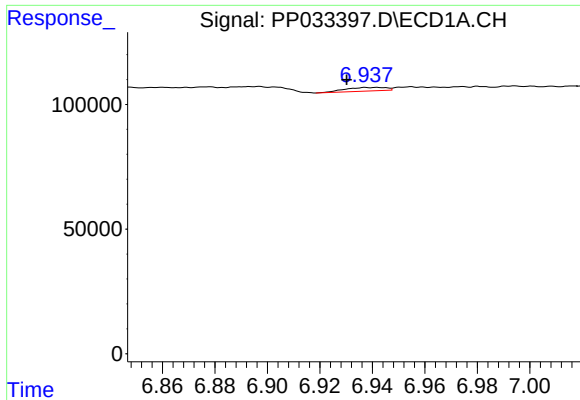

#26 AR-1254-1


R.T.: 6.942 min
Delta R.T.: 0.011 min
Response: 15650
Conc: 8.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

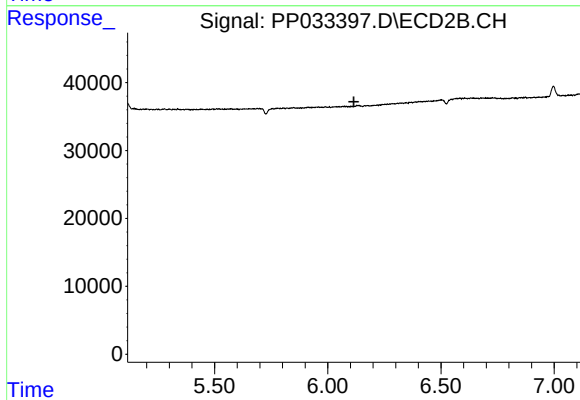


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

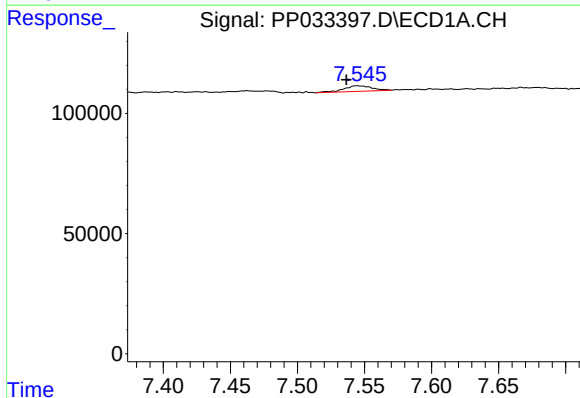


#28 AR-1254-3

R.T.: 7.545 min
Delta R.T.: 0.008 min
Response: 33945
Conc: 11.18 ng/ml

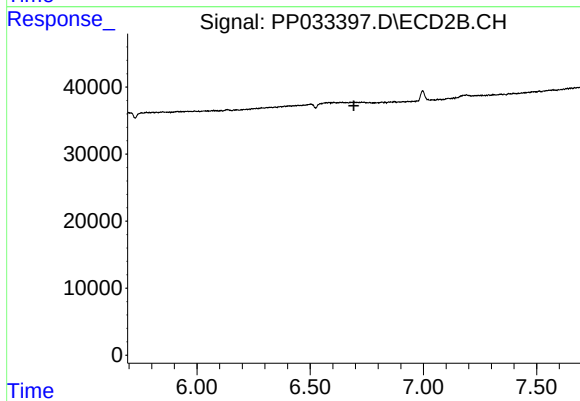

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

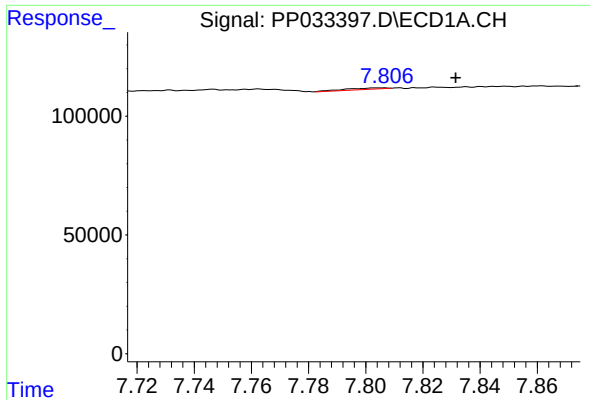

#29 AR-1254-4

R.T.: 7.806 min
Delta R.T.: -0.025 min
Response: 5557
Conc: 2.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

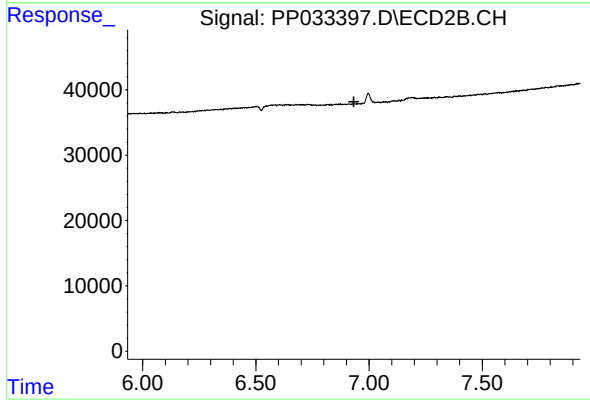

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.