

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
 Data File : PP033390.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2021 9:37
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:33:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 12:56:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.735	3.997	3471461	1995629	56.610m	48.803
2) SA Decachlor...	10.550	9.259	2592596	1811048	59.517	54.061
Target Compounds						
21) L5 AR-1248-1	6.033	5.242	566246	341741	591.403	525.482
22) L5 AR-1248-2	6.326	5.504	736891	472043	556.114	492.041
23) L5 AR-1248-3	6.538	5.547	889695	502194	549.438m	493.918
24) L5 AR-1248-4	6.964	5.732	1001974	548691	582.325	442.751
25) L5 AR-1248-5	7.002	6.153	992295	582536	570.284	515.823

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
Data File : PP033390.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2021 9:37
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 12:56:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

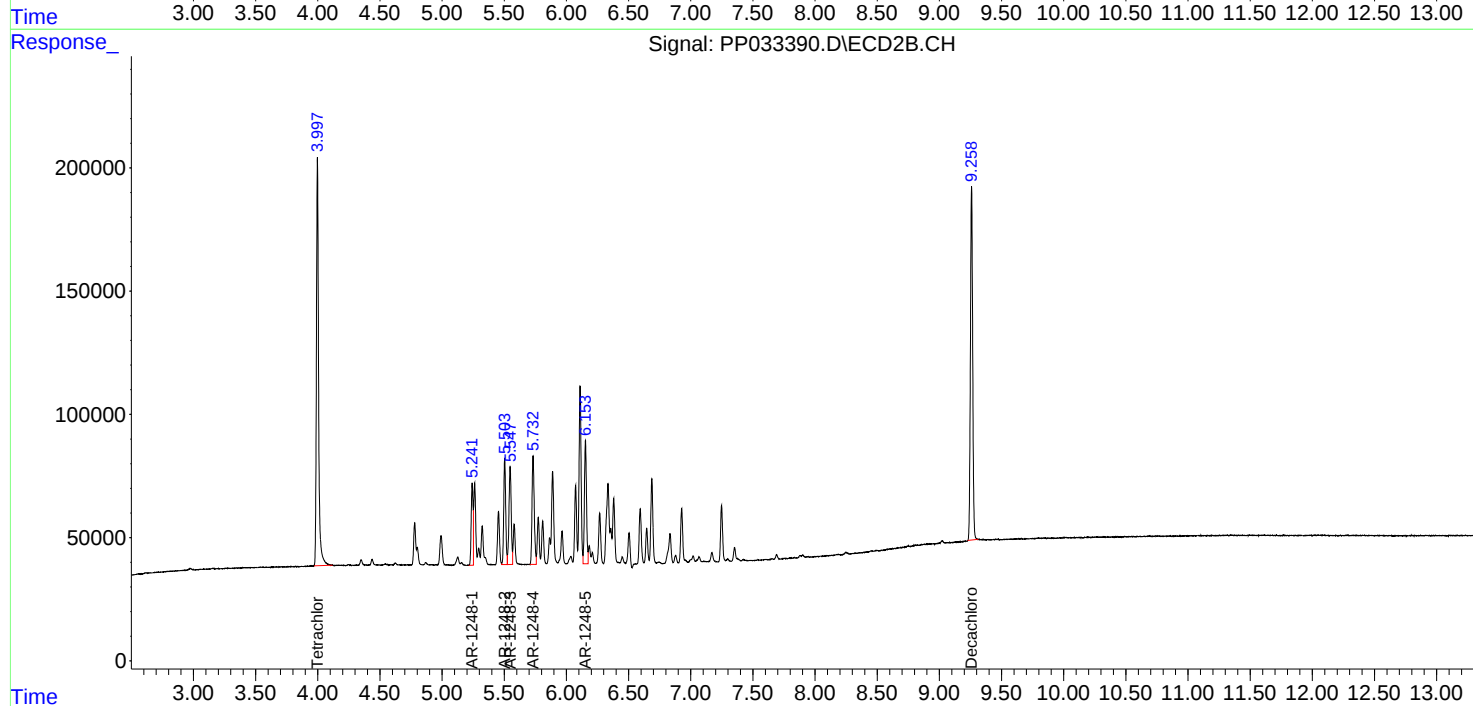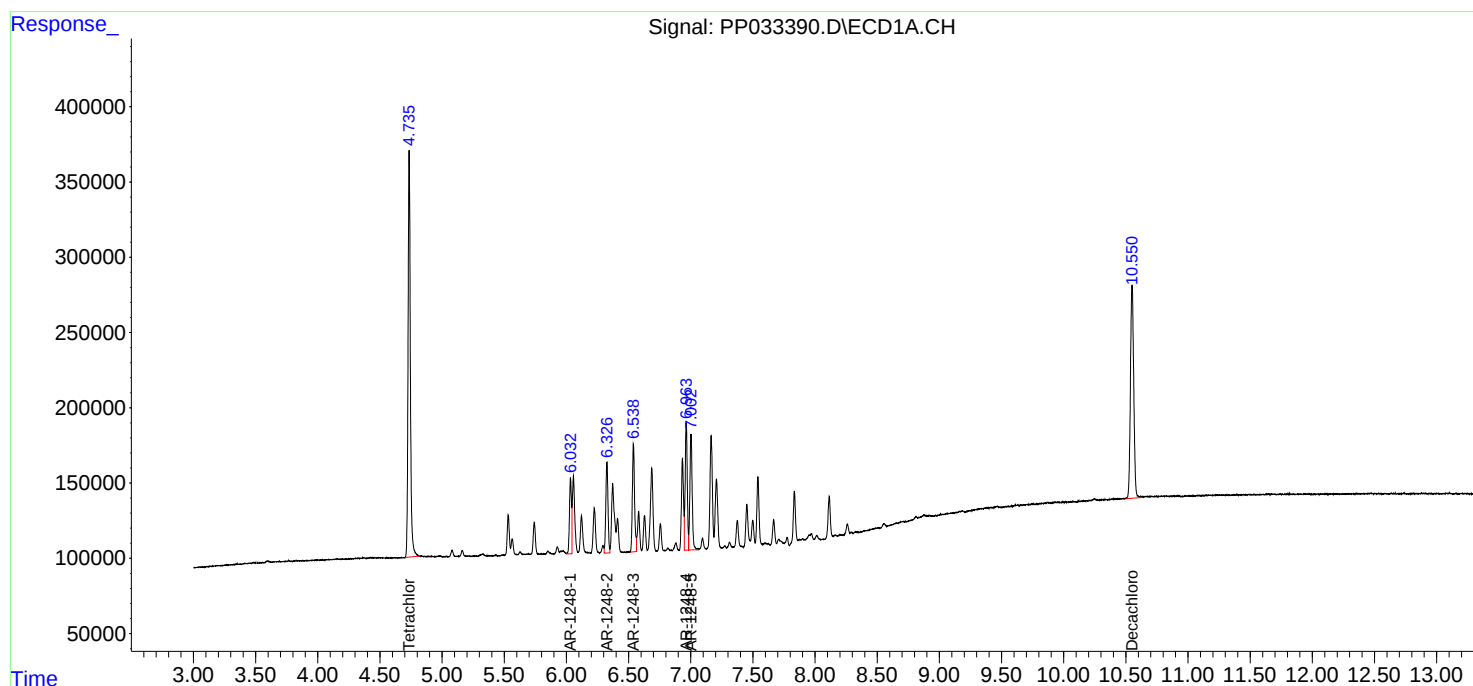

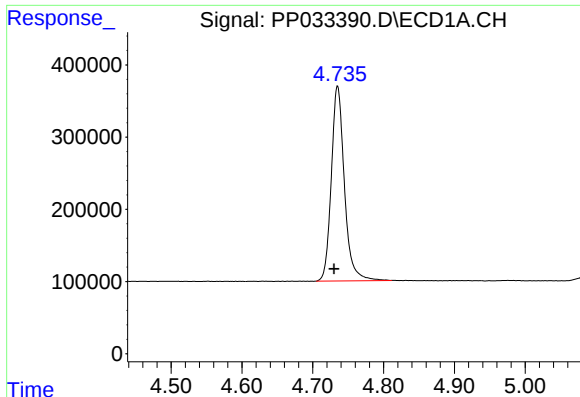


#1 Tetrachloro-m-xylene

R.T.: 4.735 min
Delta R.T.: 0.005 min
Response: 3471461
Conc: 56.61 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:44 AM

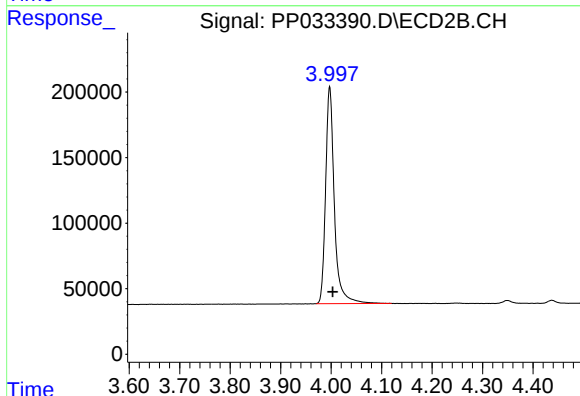


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 1995629
Conc: 48.80 ng/ml

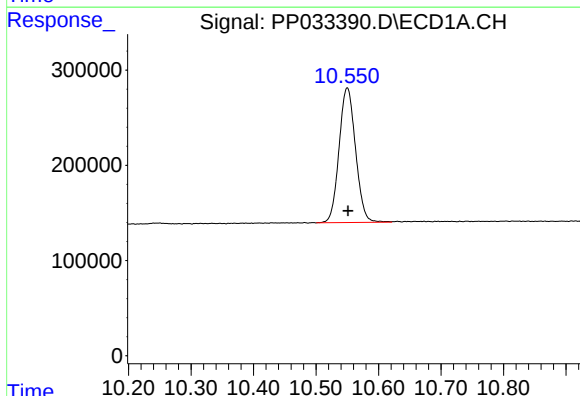


#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: 0.000 min
Response: 2592596
Conc: 59.52 ng/ml

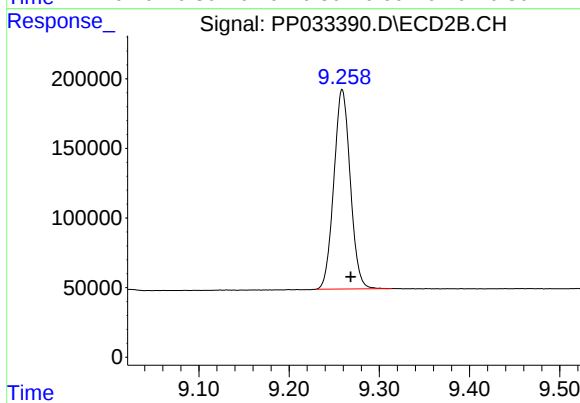

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.010 min
Response: 1811048
Conc: 54.06 ng/ml

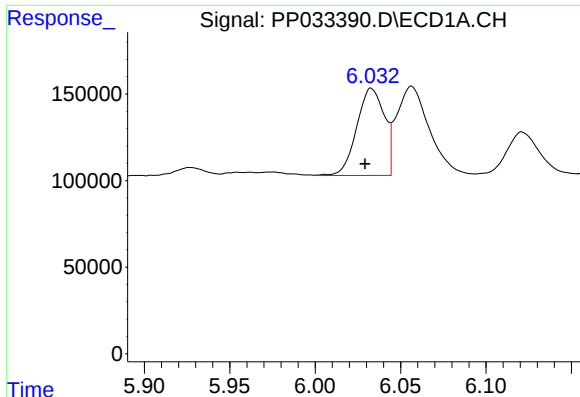


#21 AR-1248-1

R.T.: 6.033 min
Delta R.T.: 0.004 min
Response: 566246
Conc: 591.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:44 AM

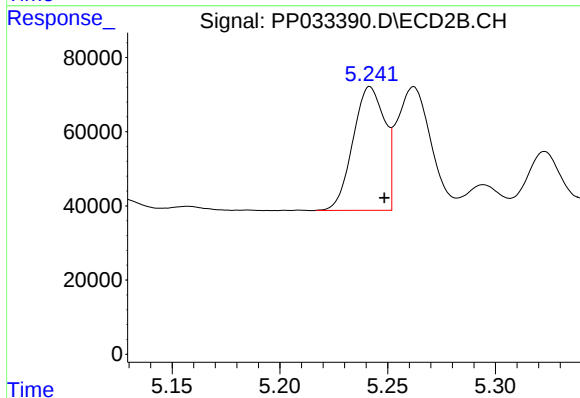


#21 AR-1248-1

R.T.: 5.242 min
Delta R.T.: -0.007 min
Response: 341741
Conc: 525.48 ng/ml

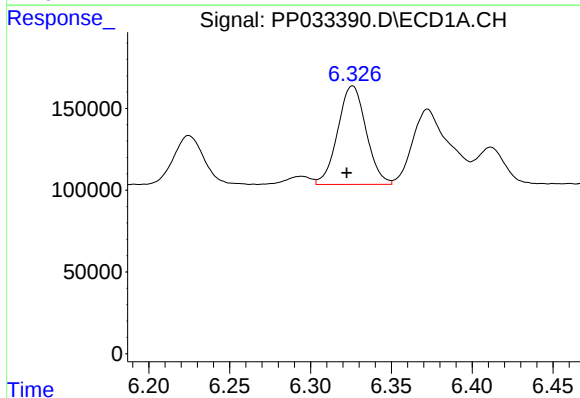


#22 AR-1248-2

R.T.: 6.326 min
Delta R.T.: 0.004 min
Response: 736891
Conc: 556.11 ng/ml

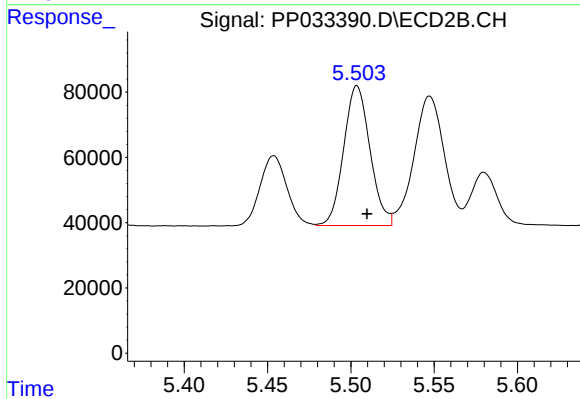

#22 AR-1248-2

R.T.: 5.504 min
Delta R.T.: -0.006 min
Response: 472043
Conc: 492.04 ng/ml

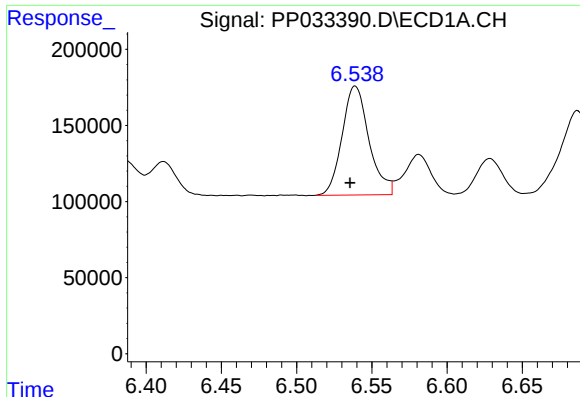


#23 AR-1248-3

R.T.: 6.538 min
Delta R.T.: 0.003 min
Response: 889695
Conc: 549.44 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:44 AM

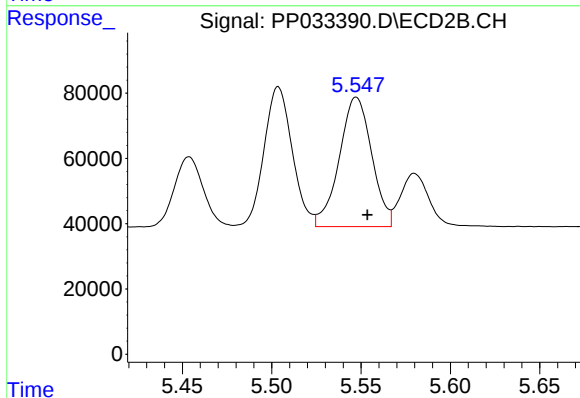


#23 AR-1248-3

R.T.: 5.547 min
Delta R.T.: -0.006 min
Response: 502194
Conc: 493.92 ng/ml

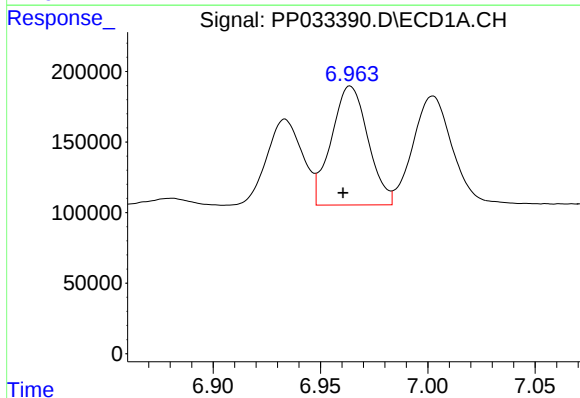


#24 AR-1248-4

R.T.: 6.964 min
Delta R.T.: 0.003 min
Response: 1001974
Conc: 582.32 ng/ml

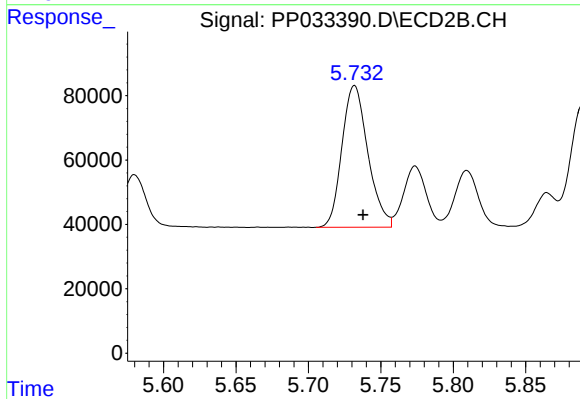

#24 AR-1248-4

R.T.: 5.732 min
Delta R.T.: -0.006 min
Response: 548691
Conc: 442.75 ng/ml

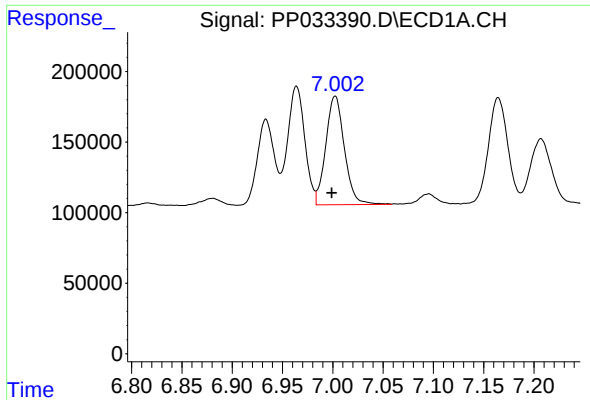


#25 AR-1248-5

R.T.: 7.002 min
Delta R.T.: 0.003 min
Response: 992295
Conc: 570.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:44 AM

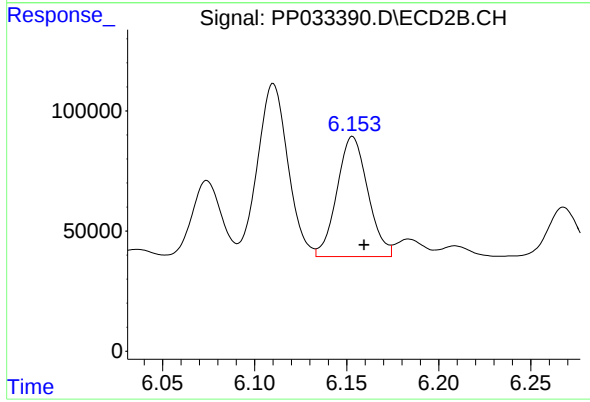

#25 AR-1248-5

R.T.: 6.153 min
Delta R.T.: -0.006 min
Response: 582536
Conc: 515.82 ng/ml