

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
 Data File : PP033394.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2021 10:50
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:33:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 12:57:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.733	3.997	3383549	2005701	55.176	49.049
2)	SA Decachlor...	10.547	9.259	2549212	1813772	58.521	54.142
Target Compounds							
21)	L5 AR-1248-1	6.030	5.241	535811	341872	559.615	525.685
22)	L5 AR-1248-2	6.323	5.503	708055	474991	534.353	495.114
23)	L5 AR-1248-3	6.536	5.547	876352	505720	541.198m	497.385
24)	L5 AR-1248-4	6.961	5.730	971949	546811	564.875	441.234
25)	L5 AR-1248-5	6.999	6.152	956207	580527	549.544	514.045

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
Data File : PP033394.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2021 10:50
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 12:57:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

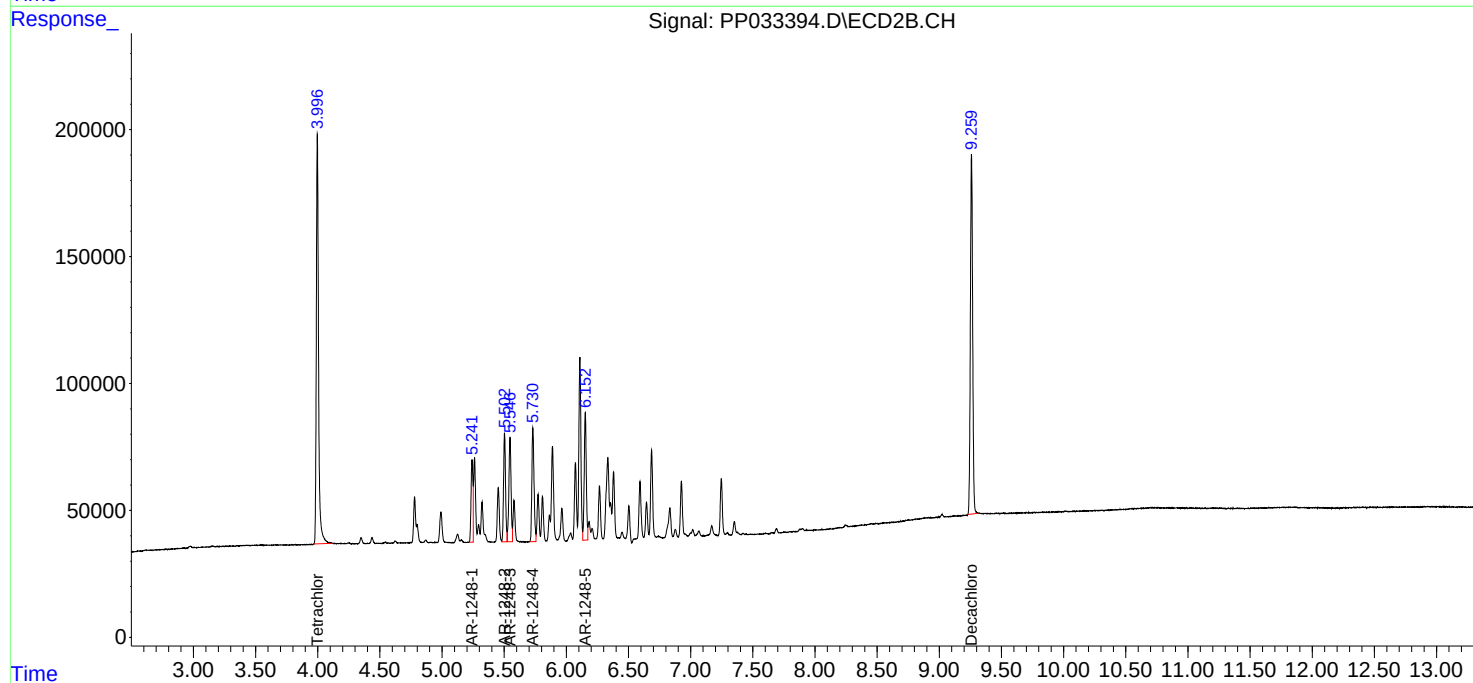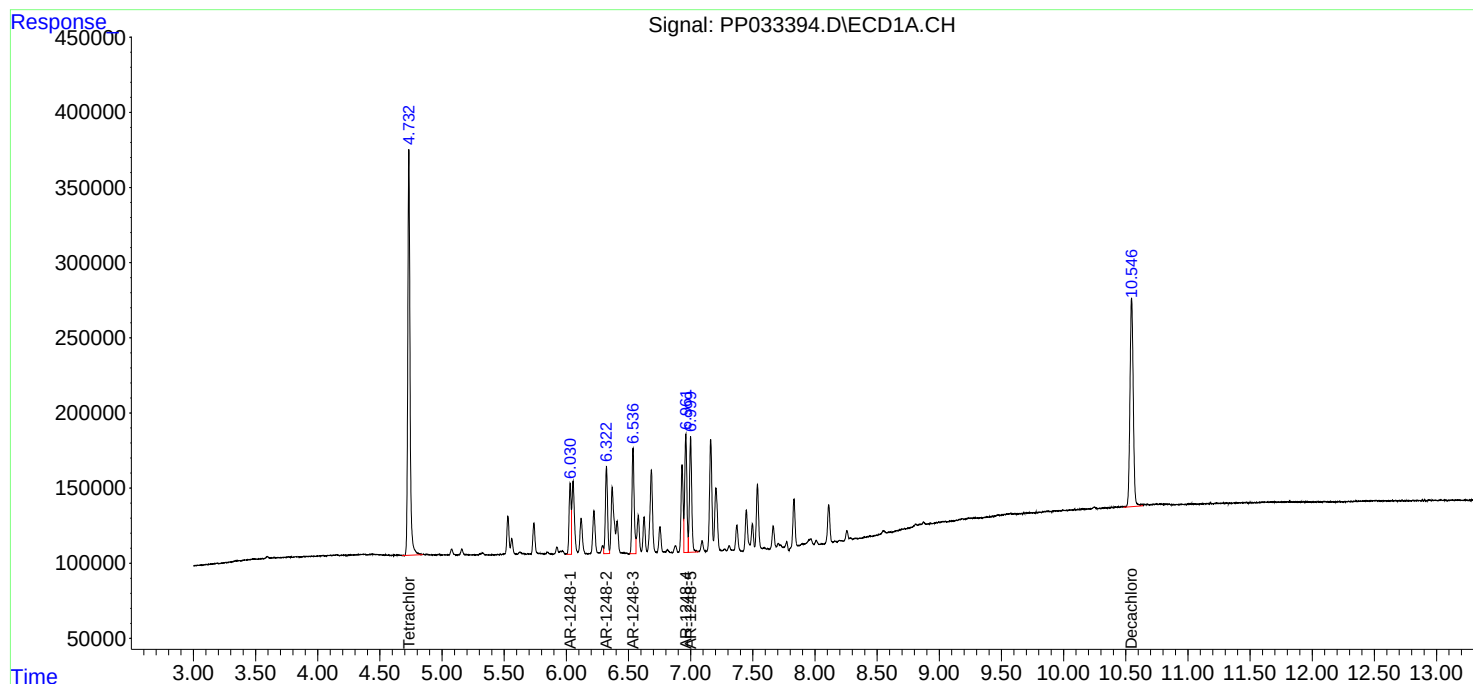

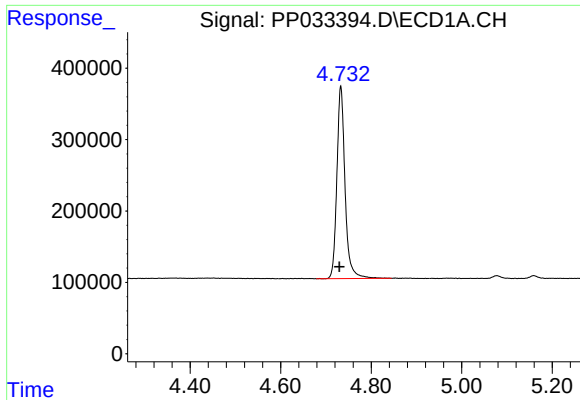


#1 Tetrachloro-m-xylene

R.T.: 4.733 min
Delta R.T.: 0.003 min
Response: 3383549
Conc: 55.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:52 AM

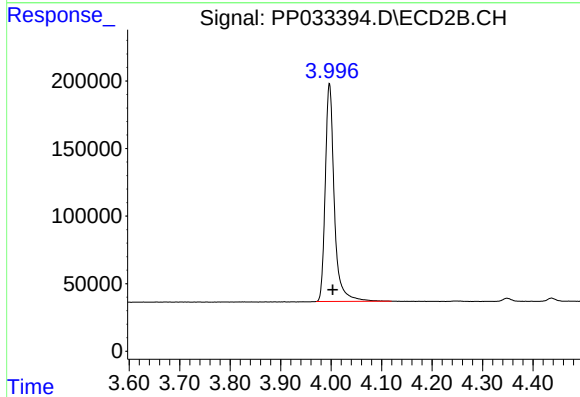


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 2005701
Conc: 49.05 ng/ml

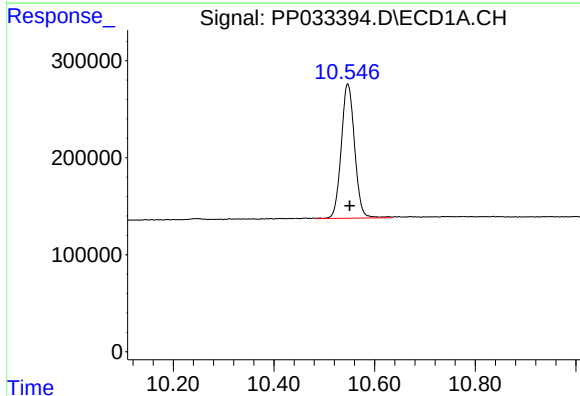


#2 Decachlorobiphenyl

R.T.: 10.547 min
Delta R.T.: -0.004 min
Response: 2549212
Conc: 58.52 ng/ml

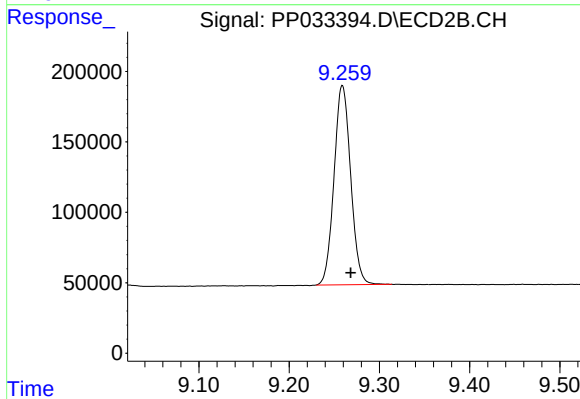

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.009 min
Response: 1813772
Conc: 54.14 ng/ml

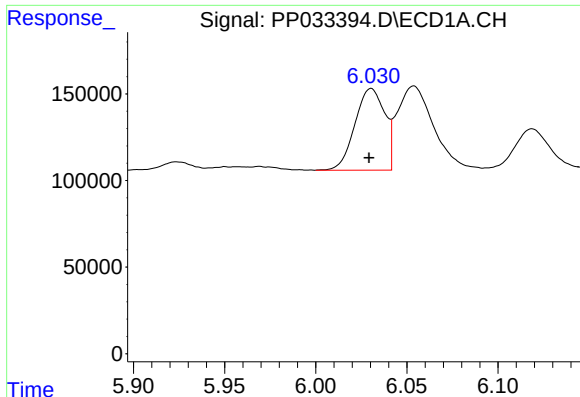


#21 AR-1248-1

R.T.: 6.030 min
Delta R.T.: 0.001 min
Response: 535811
Conc: 559.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:52 AM

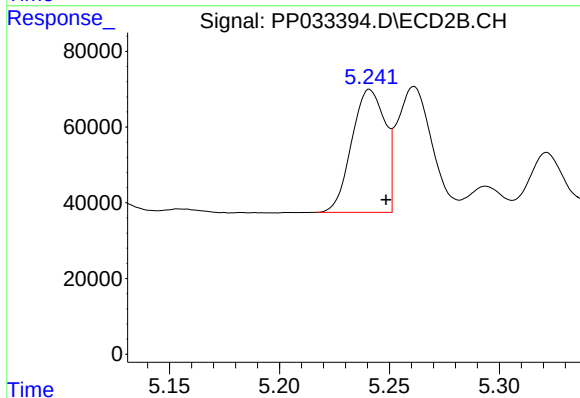


#21 AR-1248-1

R.T.: 5.241 min
Delta R.T.: -0.007 min
Response: 341872
Conc: 525.68 ng/ml

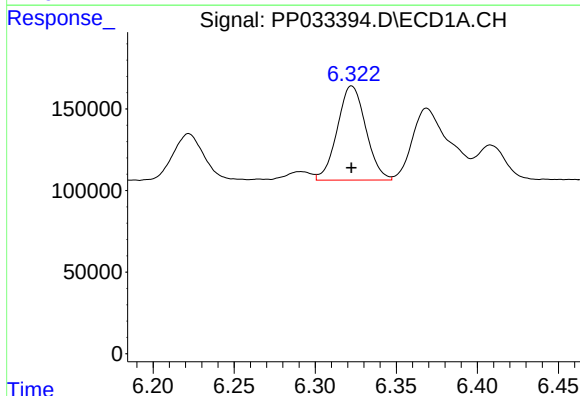


#22 AR-1248-2

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 708055
Conc: 534.35 ng/ml

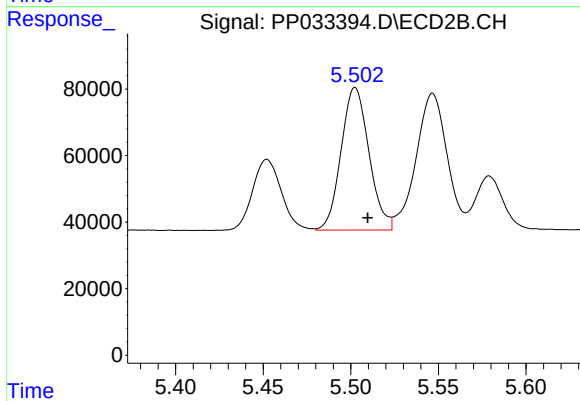

#22 AR-1248-2

R.T.: 5.503 min
Delta R.T.: -0.007 min
Response: 474991
Conc: 495.11 ng/ml

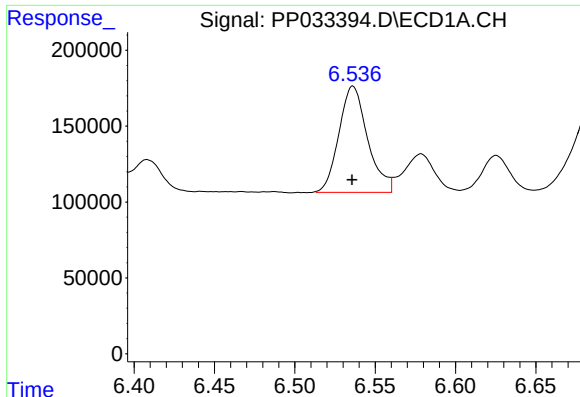


#23 AR-1248-3

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 876352
Conc: 541.20 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:52 AM

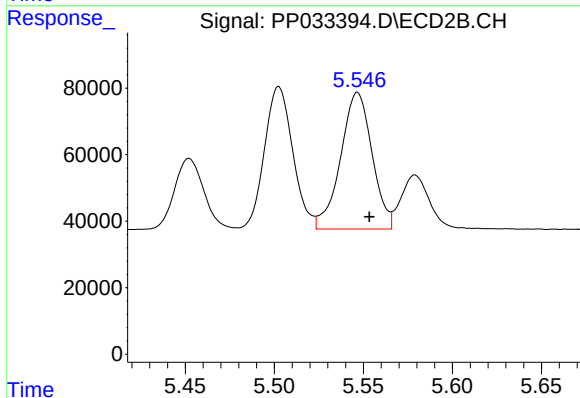


#23 AR-1248-3

R.T.: 5.547 min
Delta R.T.: -0.007 min
Response: 505720
Conc: 497.38 ng/ml

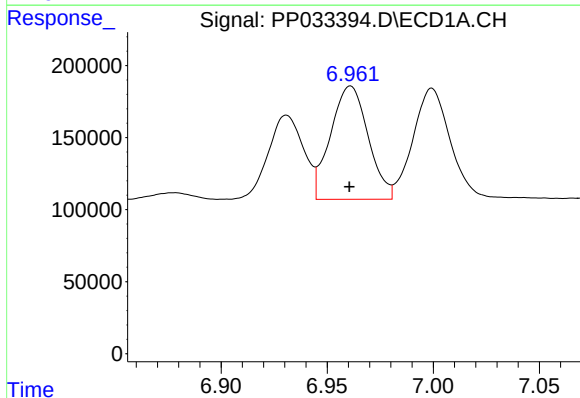


#24 AR-1248-4

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 971949
Conc: 564.88 ng/ml

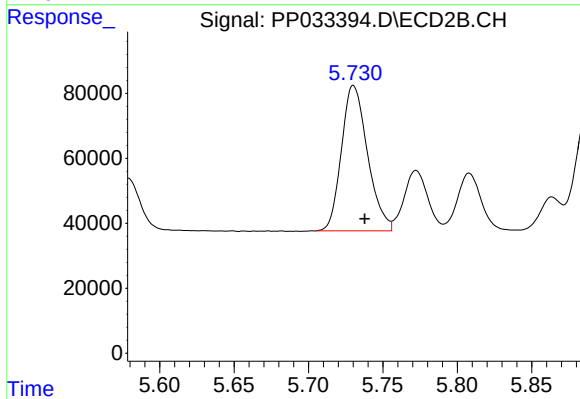

#24 AR-1248-4

R.T.: 5.730 min
Delta R.T.: -0.008 min
Response: 546811
Conc: 441.23 ng/ml

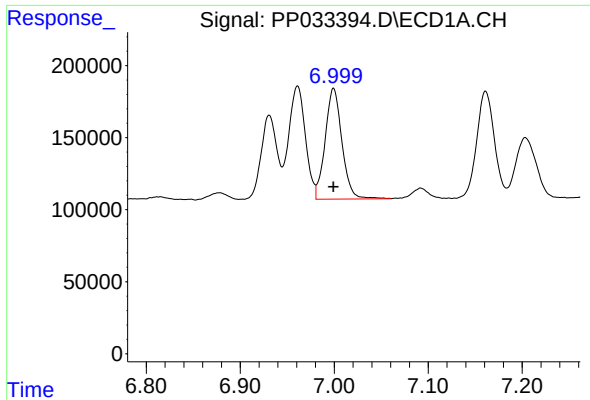


#25 AR-1248-5

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 956207
Conc: 549.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/19/2021 9:33:52 AM

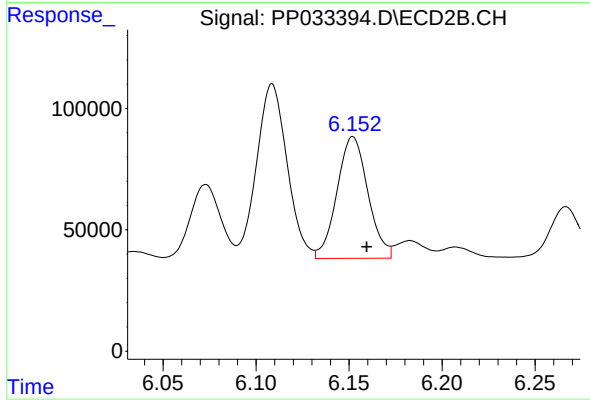

#25 AR-1248-5

R.T.: 6.152 min
Delta R.T.: -0.007 min
Response: 580527
Conc: 514.05 ng/ml