

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
 Data File : PP033428.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Feb 2021 1:35
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/19/2021 9:34:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 03:32:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.724	3.996	3179311	2100084	51.846	51.357
2)	SA Decachlor...	10.538	9.254	2301573	1805691	52.836	53.901
Target Compounds							
21)	L5 AR-1248-1	6.022	5.239	529877	367139	553.418	564.536
22)	L5 AR-1248-2	6.315	5.500	689109	498900	520.054	520.036
23)	L5 AR-1248-3	6.528	5.544	848527	530641	524.015m	521.896
24)	L5 AR-1248-4	6.953	5.728	924579	590221	537.345	476.263
25)	L5 AR-1248-5	6.992	6.149	920100	612598	528.792	542.443

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021821\
Data File : PP033428.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Feb 2021 1:35
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:34:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 03:32:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

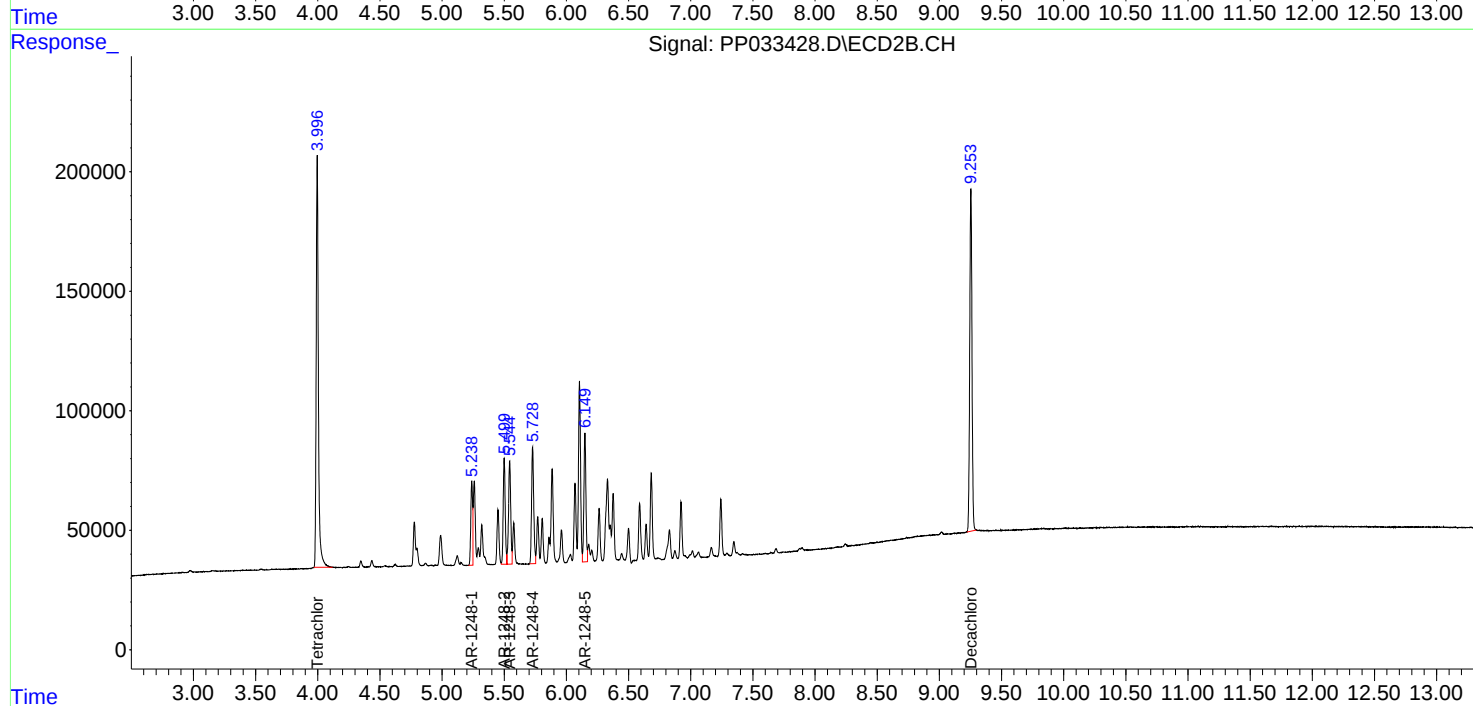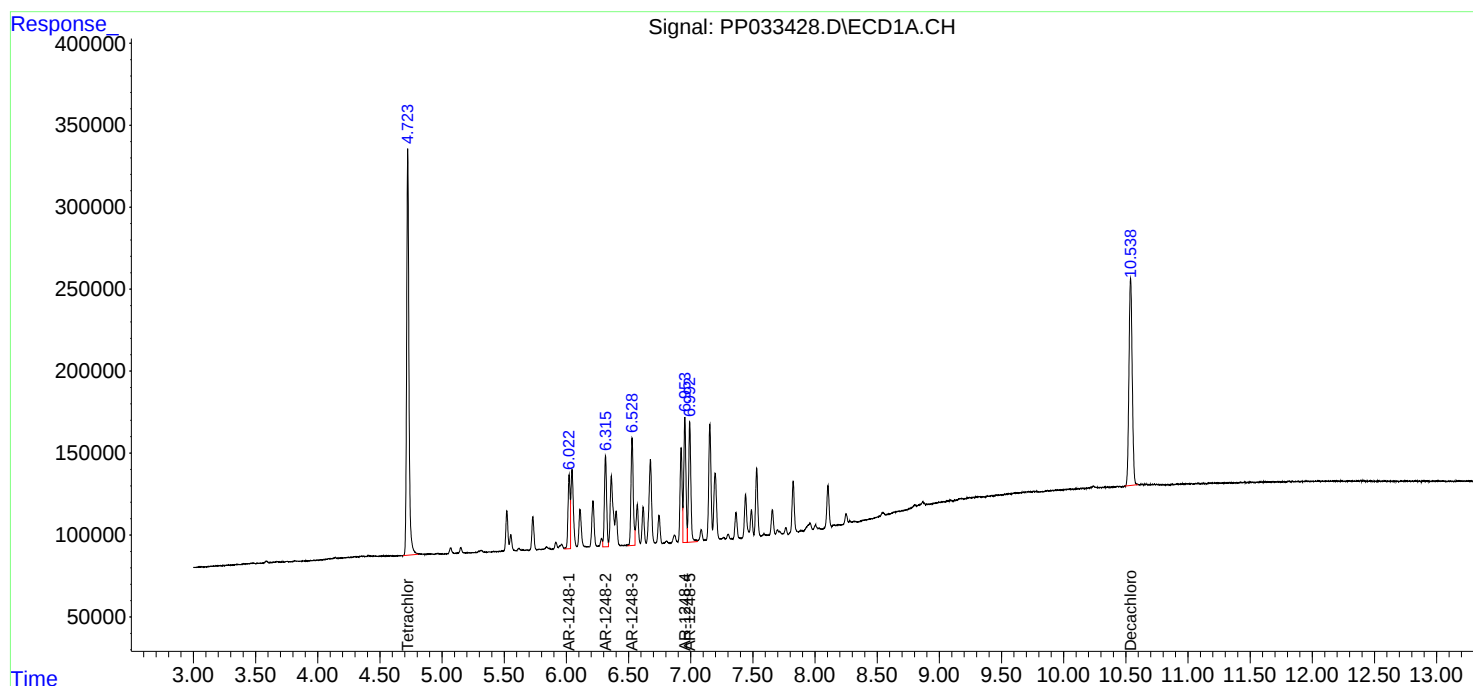

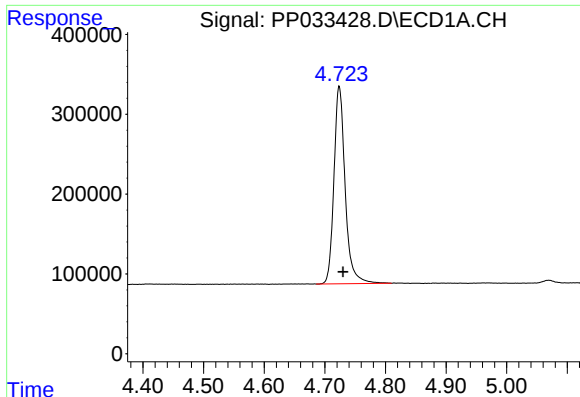


#1 Tetrachloro-m-xylene

R.T.: 4.724 min
Delta R.T.: -0.006 min
Response: 3179311
Conc: 51.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:34:34 AM

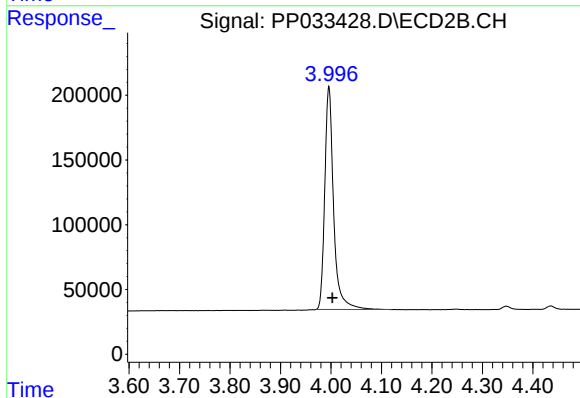


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.007 min
Response: 2100084
Conc: 51.36 ng/ml

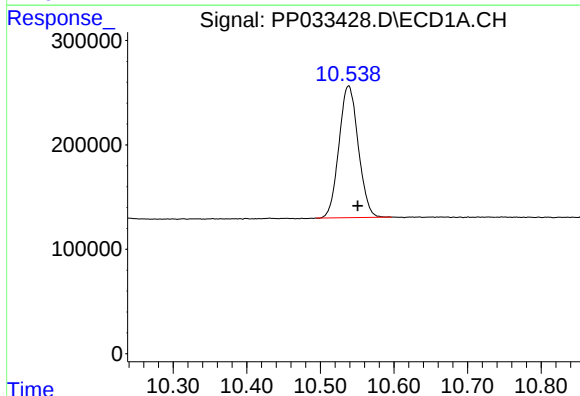


#2 Decachlorobiphenyl

R.T.: 10.538 min
Delta R.T.: -0.013 min
Response: 2301573
Conc: 52.84 ng/ml

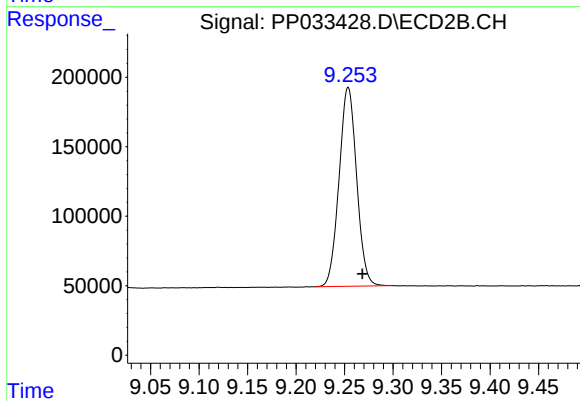

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.015 min
Response: 1805691
Conc: 53.90 ng/ml

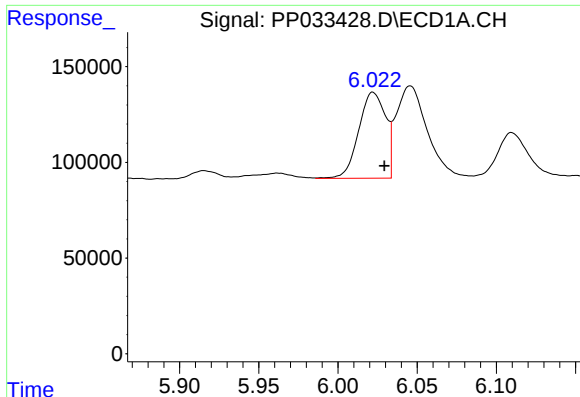


#21 AR-1248-1

R.T.: 6.022 min
Delta R.T.: -0.007 min
Response: 529877
Conc: 553.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:34:34 AM

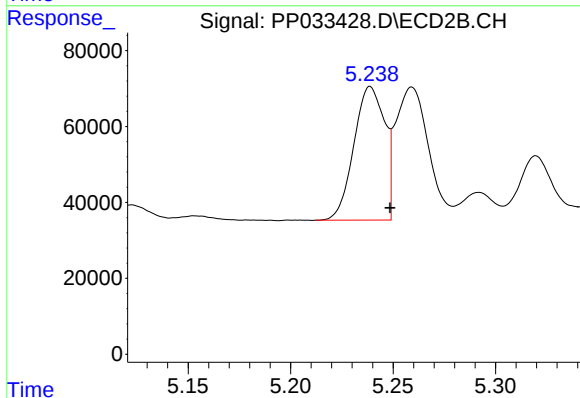


#21 AR-1248-1

R.T.: 5.239 min
Delta R.T.: -0.010 min
Response: 367139
Conc: 564.54 ng/ml

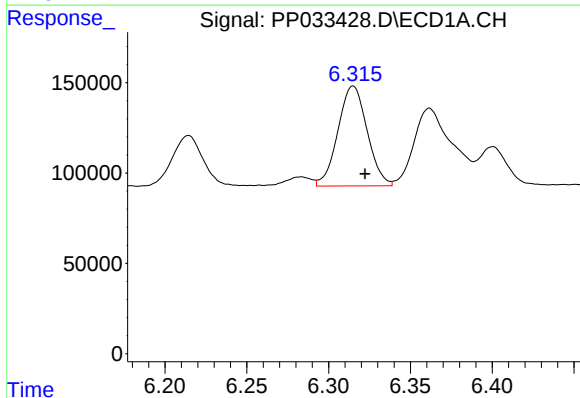


#22 AR-1248-2

R.T.: 6.315 min
Delta R.T.: -0.007 min
Response: 689109
Conc: 520.05 ng/ml

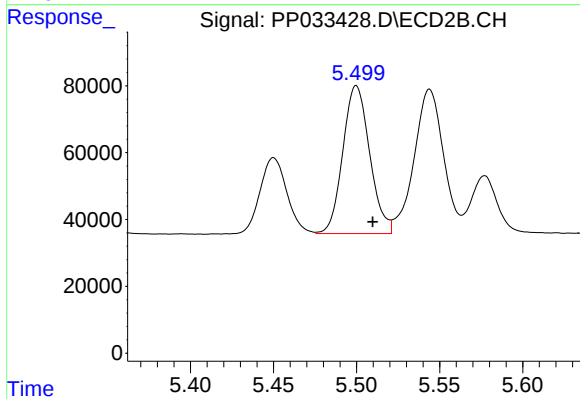

#22 AR-1248-2

R.T.: 5.500 min
Delta R.T.: -0.010 min
Response: 498900
Conc: 520.04 ng/ml

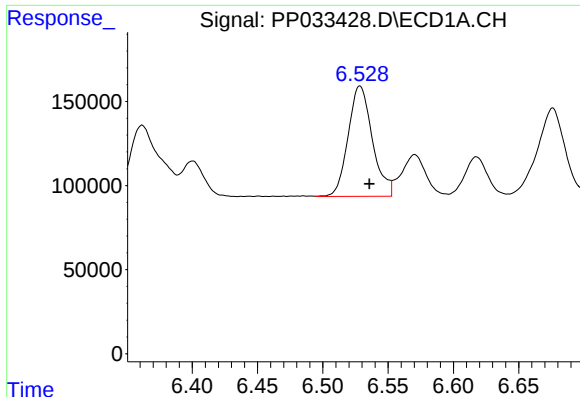


#23 AR-1248-3

R.T.: 6.528 min
Delta R.T.: -0.008 min
Response: 848527
Conc: 524.01 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/19/2021 9:34:34 AM

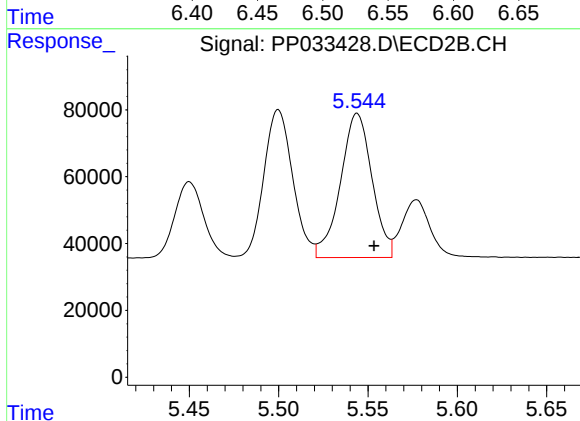


#23 AR-1248-3

R.T.: 5.544 min
Delta R.T.: -0.010 min
Response: 530641
Conc: 521.90 ng/ml

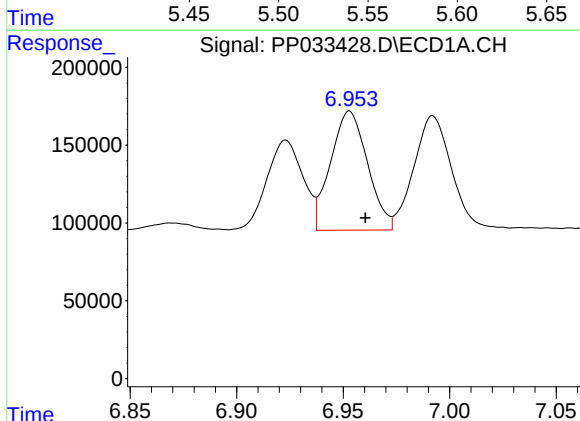


#24 AR-1248-4

R.T.: 6.953 min
Delta R.T.: -0.008 min
Response: 924579
Conc: 537.34 ng/ml

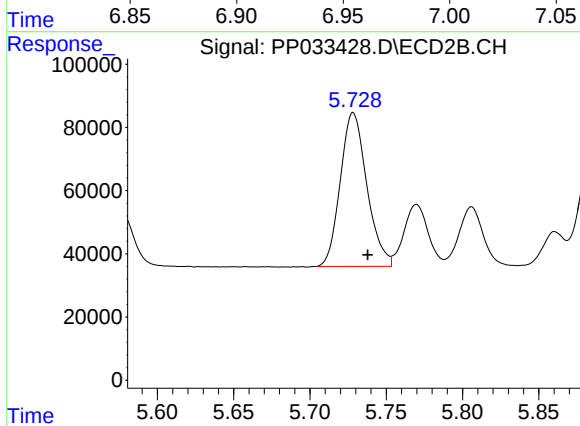

#24 AR-1248-4

R.T.: 5.728 min
Delta R.T.: -0.009 min
Response: 590221
Conc: 476.26 ng/ml

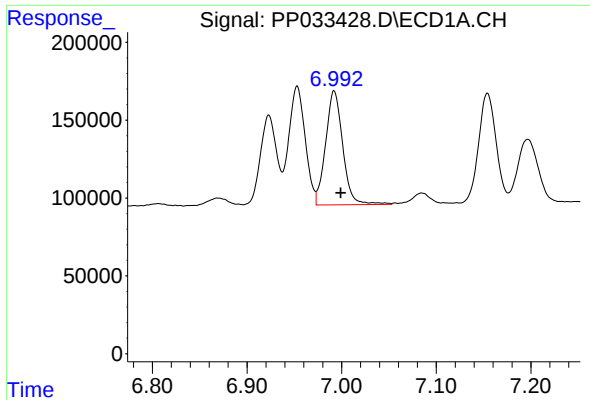


#25 AR-1248-5

R.T.: 6.992 min
Delta R.T.: -0.007 min
Response: 920100
Conc: 528.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/19/2021 9:34:34 AM

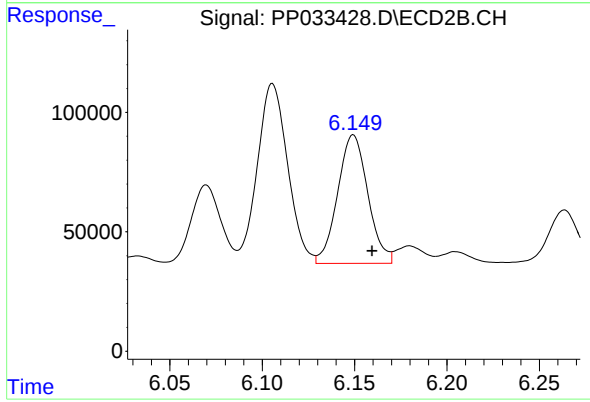

#25 AR-1248-5

R.T.: 6.149 min
Delta R.T.: -0.010 min
Response: 612598
Conc: 542.44 ng/ml