

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021822\
 Data File : PP043821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 12:56
 Operator : YP\AJ
 Sample : N1579-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-6-(3.0-3.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 23:46:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.916	3.173	44826883	40856376	20.274	21.752
2) SA Decachlor...	10.062	8.548	21991995	28976118	18.514	17.860

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021822\
Data File : PP043821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 12:56
Operator : YP\AJ
Sample : N1579-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-6-(3.0-3.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 23:46:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

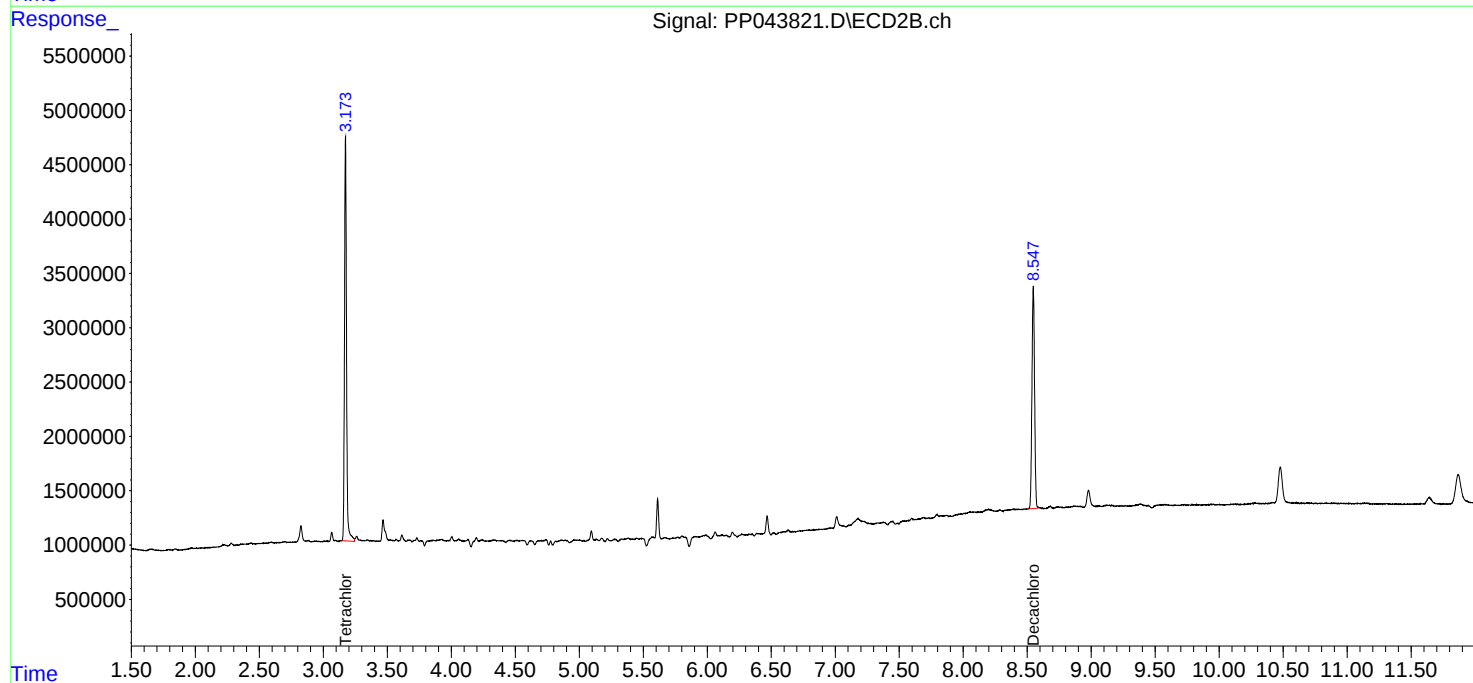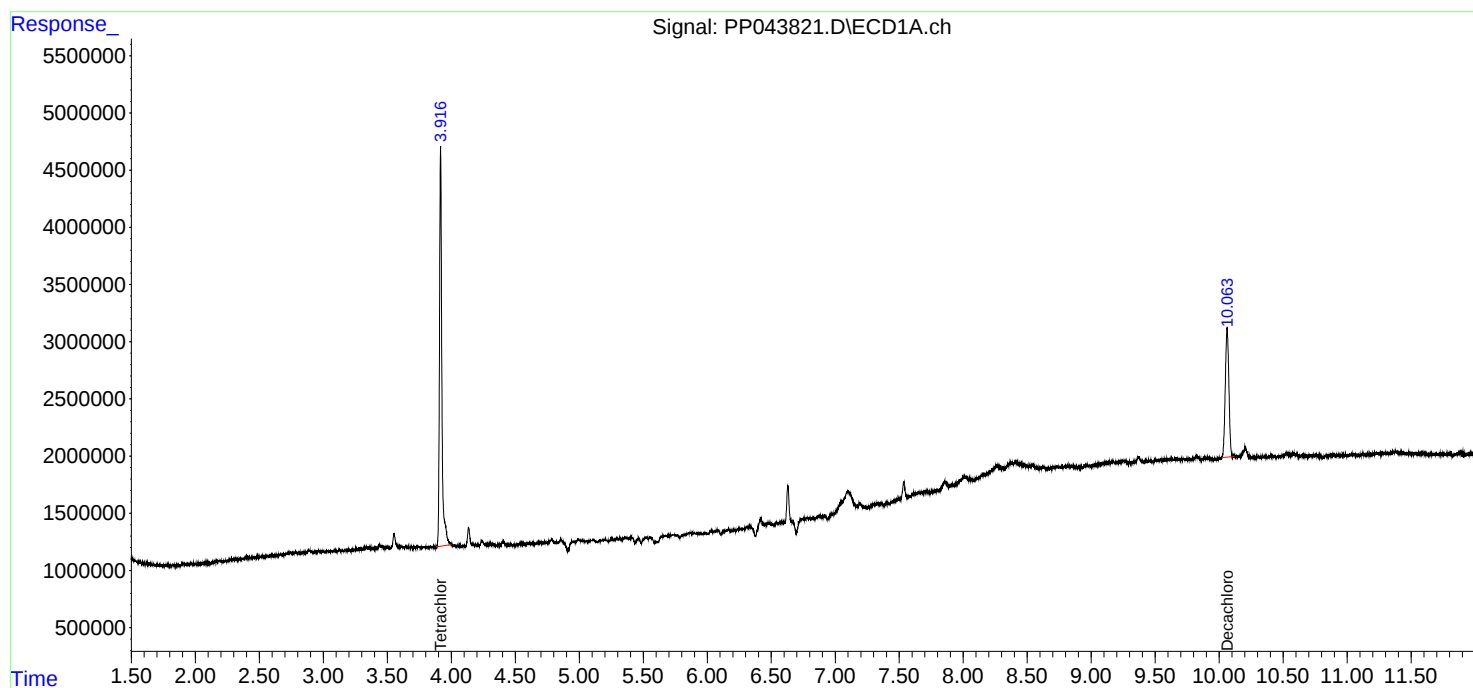


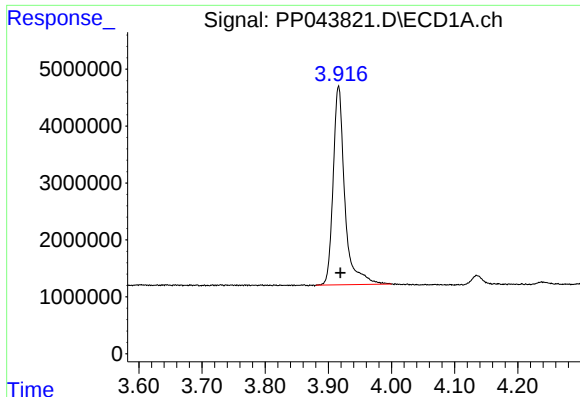

#1 Tetrachloro-m-xylene


R.T.: 3.916 min
Delta R.T.: -0.003 min
Response: 44826883
Conc: 20.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-6-(3.0-3.5)

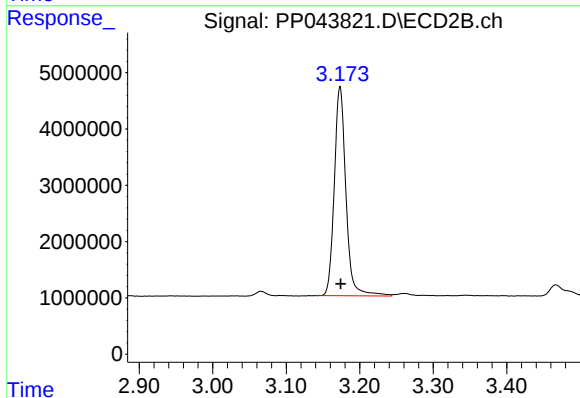


#1 Tetrachloro-m-xylene

R.T.: 3.173 min
Delta R.T.: 0.000 min
Response: 40856376
Conc: 21.75 ng/ml

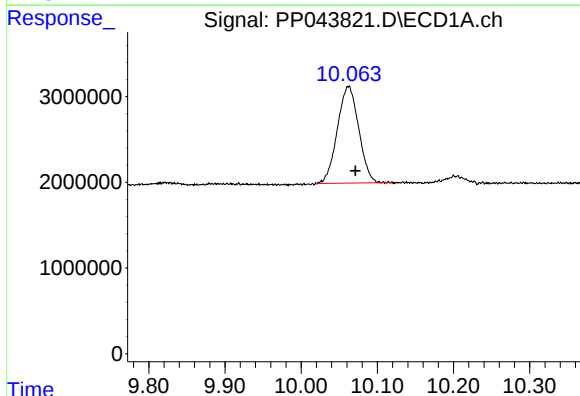

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.009 min
Response: 21991995
Conc: 18.51 ng/ml

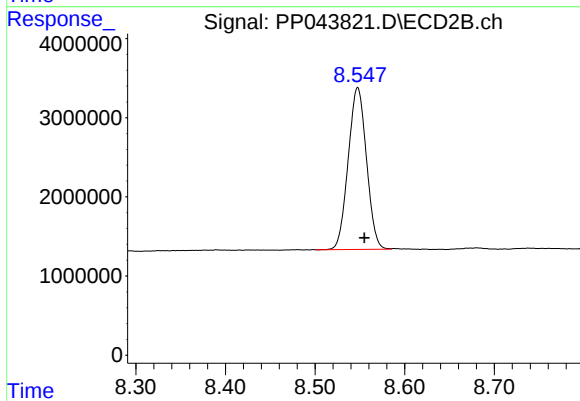

#2 Decachlorobiphenyl

R.T.: 8.548 min
Delta R.T.: -0.007 min
Response: 28976118
Conc: 17.86 ng/ml