

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021822\
 Data File : PP043837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2022 17:04
 Operator : YP\AJ
 Sample : N1595-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 5308

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2022
 Supervised By :Ankita Jodhani 02/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:29:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.927	3.192f	28799559	26330548	13.025	14.019m
2) SA Decachlor...	10.060	8.549	26551088	30701058	22.352	18.923

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021822\
Data File : PP043837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2022 17:04
Operator : YP\AJ
Sample : N1595-05
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
5308


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2022
Supervised By :Ankita Jodhani 02/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:29:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

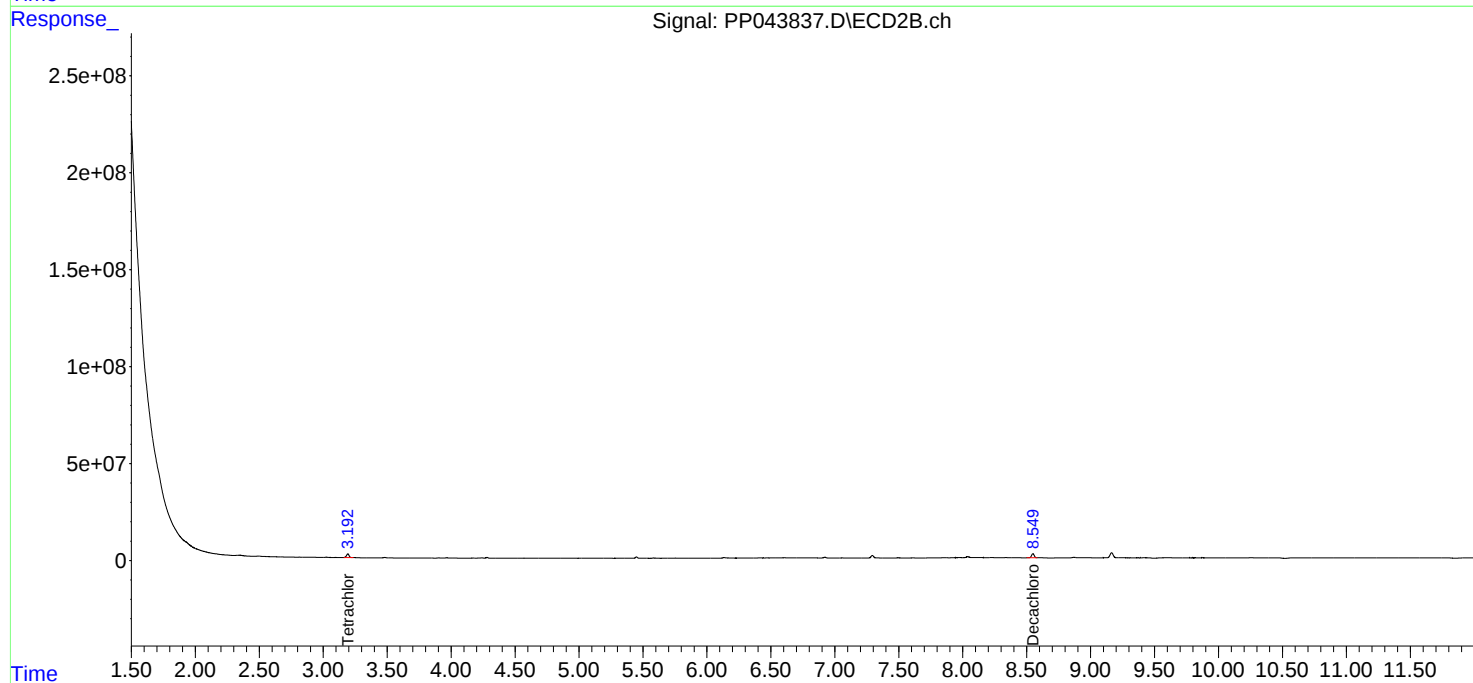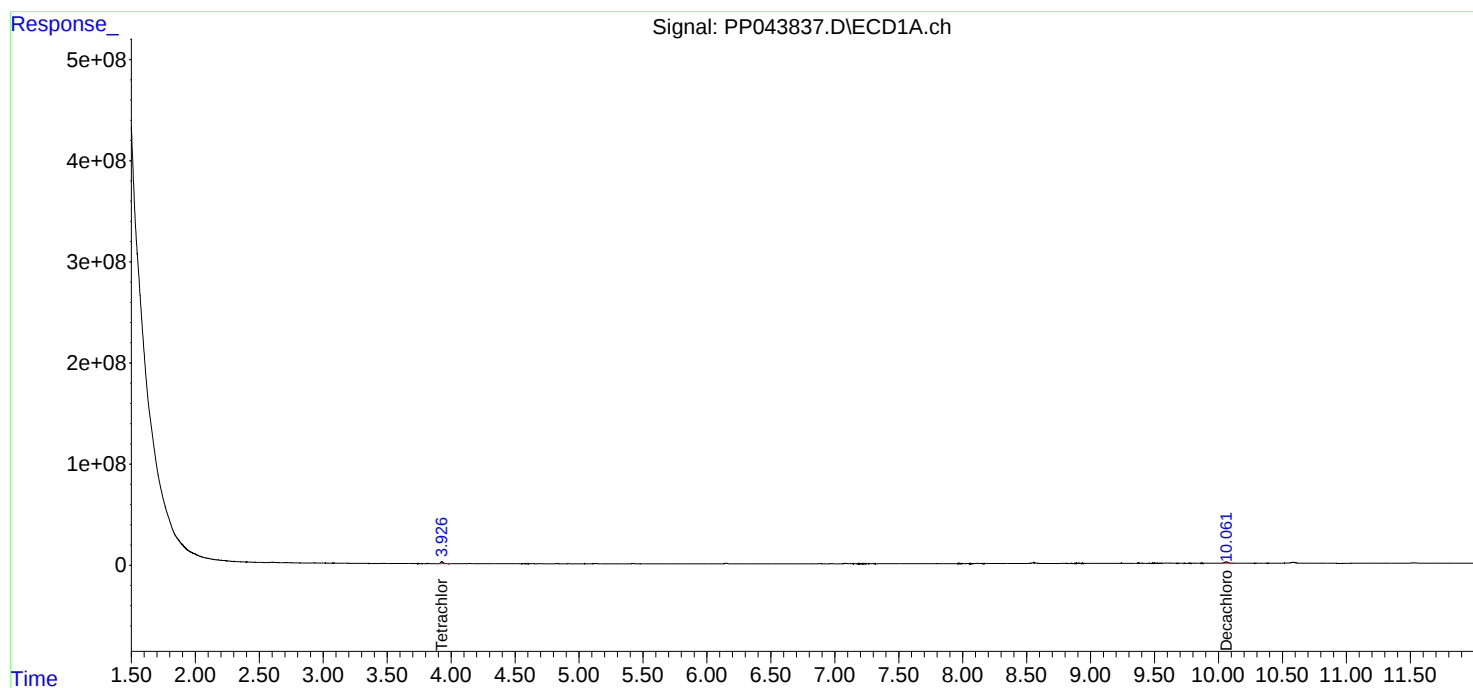

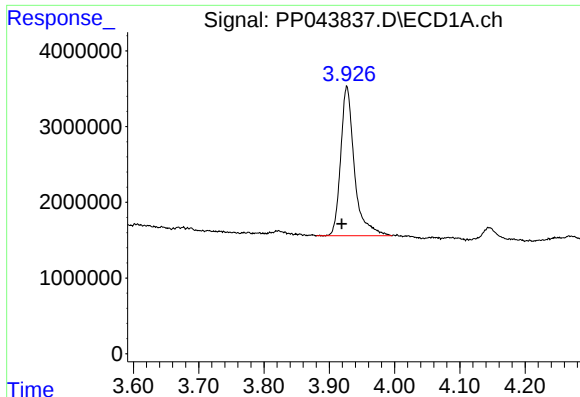


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: 0.008 min
Response: 28799559
Conc: 13.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
5308


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2022
Supervised By :Ankita Jodhani 02/21/2022

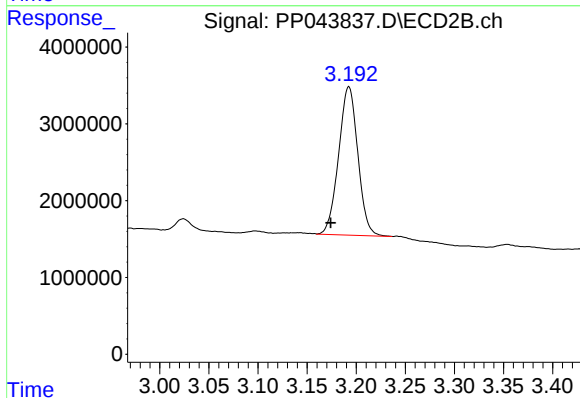


#1 Tetrachloro-m-xylene

R.T.: 3.192 min
Delta R.T.: 0.018 min
Response: 26330548
Conc: 14.02 ng/ml m

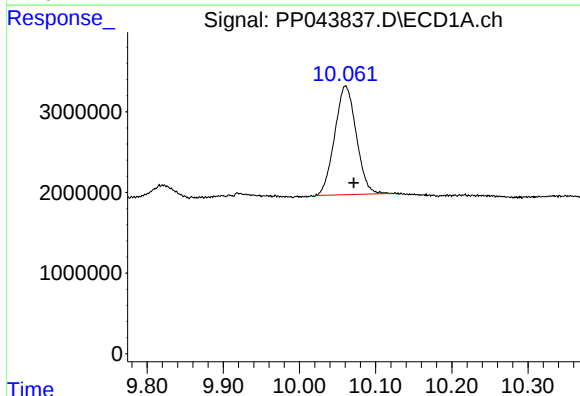

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: -0.011 min
Response: 26551088
Conc: 22.35 ng/ml

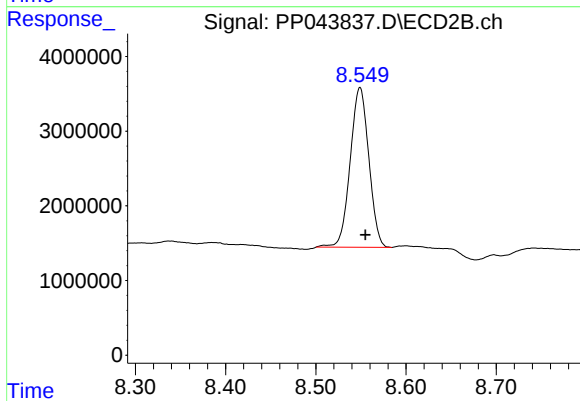

#2 Decachlorobiphenyl

R.T.: 8.549 min
Delta R.T.: -0.006 min
Response: 30701058
Conc: 18.92 ng/ml