

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021825\
 Data File : PP069818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2025 15:20
 Operator : YP\AJ
 Sample : Q1379-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1A-1B-1C-GRAY-CAULK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/19/2025
 Supervised By :Ankita Jodhani 02/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 16:15:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.830	35609253	20179629	24.876	22.609m
2) SA Decachlor...	10.252	8.889	21631350	20243133	19.793m	18.099

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021825\
Data File : PP069818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2025 15:20
Operator : YP\AJ
Sample : Q1379-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1A-1B-1C-GRAY-CAULK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/19/2025
Supervised By :Ankita Jodhani 02/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 16:15:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

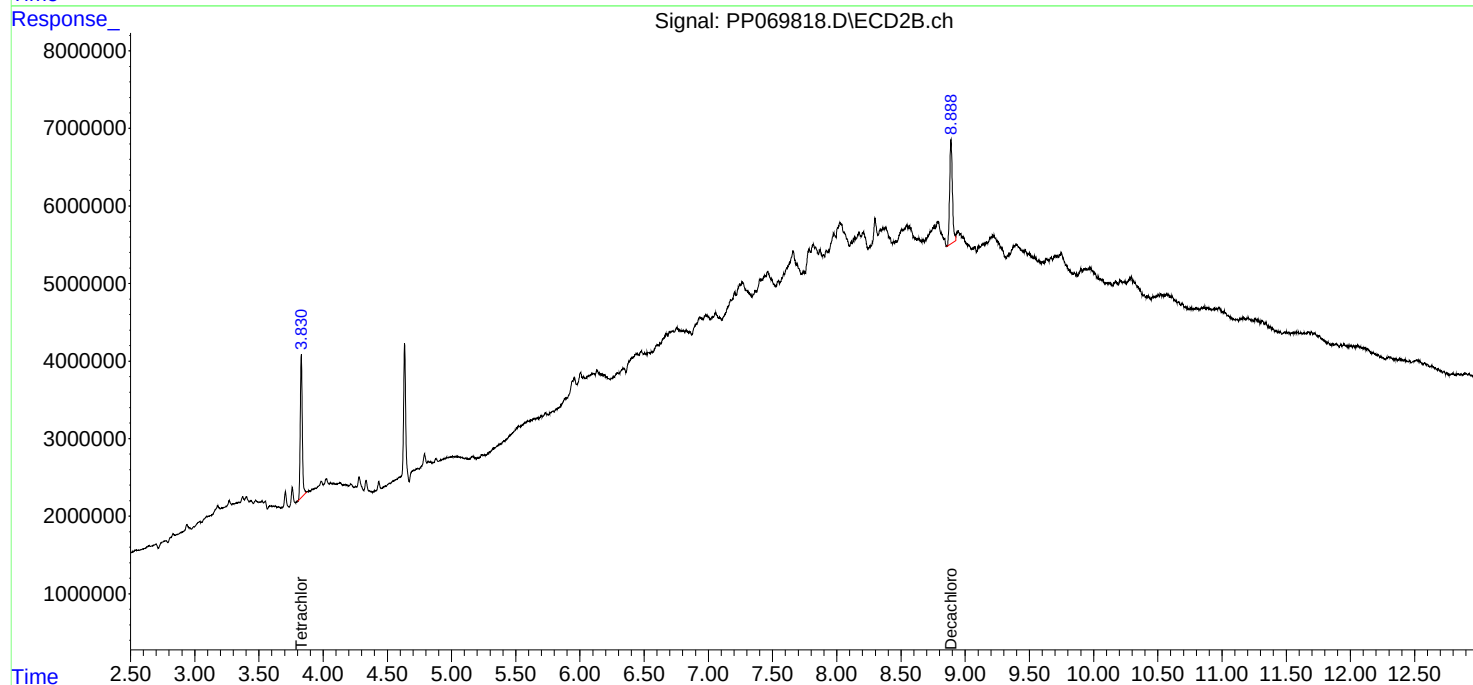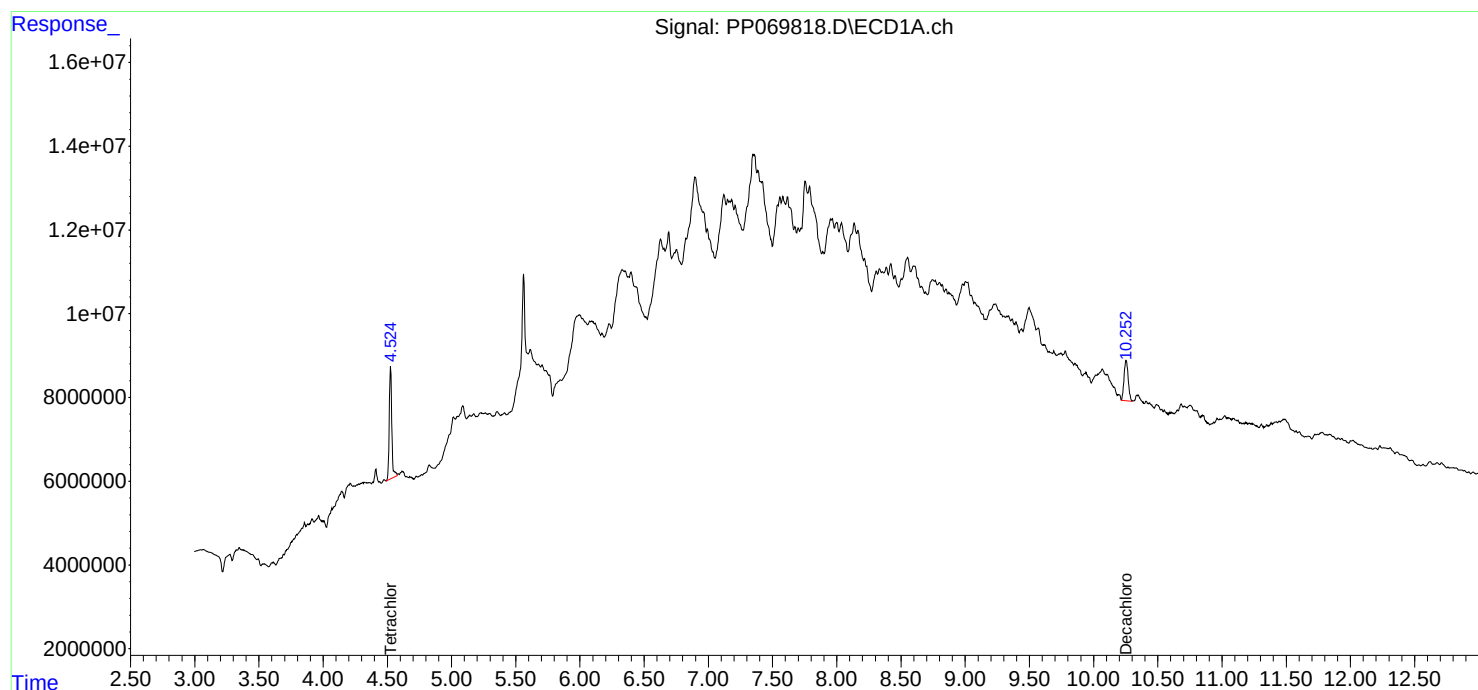

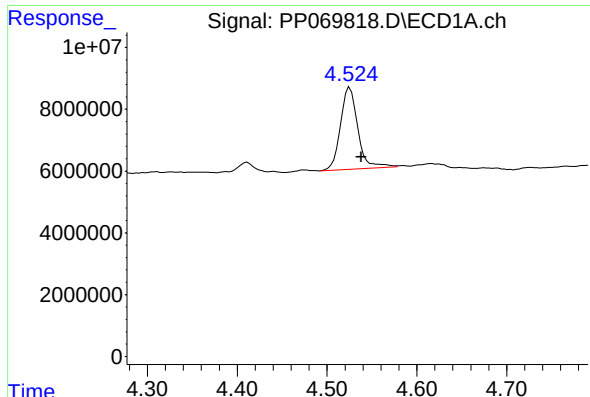


#1 Tetrachloro-m-xylene

R.T.: 4.525 min
Delta R.T.: -0.013 min
Response: 35609253
Conc: 24.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
1A-1B-1C-GRAY-CAULK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/19/2025
Supervised By :Ankita Jodhani 02/20/2025

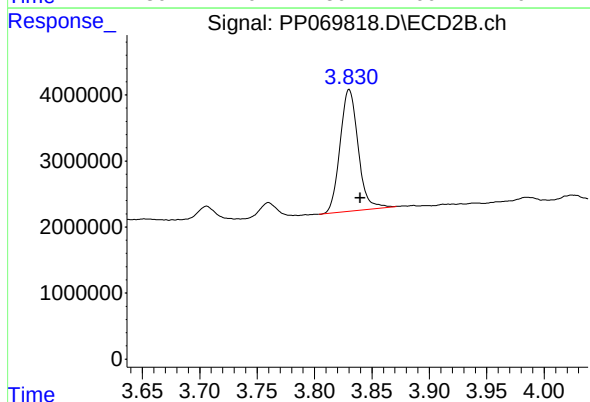


#1 Tetrachloro-m-xylene

R.T.: 3.830 min
Delta R.T.: -0.010 min
Response: 20179629
Conc: 22.61 ng/ml

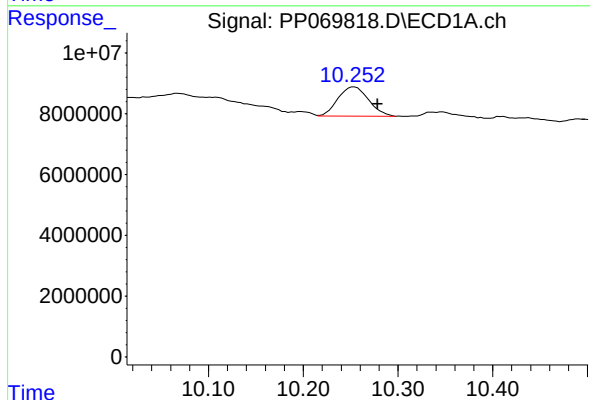

#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: -0.026 min
Response: 21631350
Conc: 19.79 ng/ml

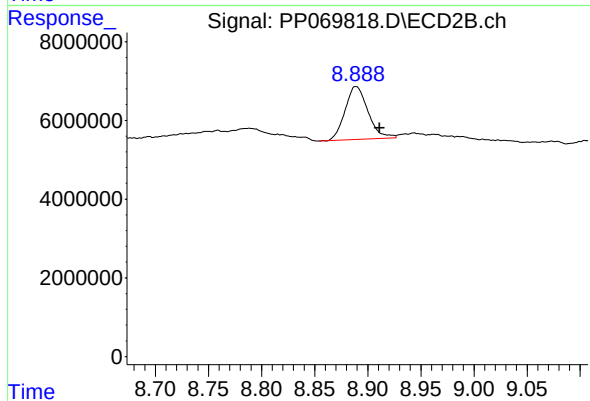

#2 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: -0.022 min
Response: 20243133
Conc: 18.10 ng/ml