

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
 Data File : PP033438.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Feb 2021 10:58
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/22/2021 10:06:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 13:38:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.724	3.997	3466841	2147387	56.535	52.514
2) SA Decachlor...	10.539	9.256	2465272	1837986	56.594	54.865
Target Compounds						
21) L5 AR-1248-1	6.022	5.239	559415	374260	584.269	575.486
22) L5 AR-1248-2	6.314	5.500	736247	507664	555.628	529.171
23) L5 AR-1248-3	6.527	5.544	866346	539894	535.019m	530.996
24) L5 AR-1248-4	6.953	5.729	973499	549089	565.776	443.073
25) L5 AR-1248-5	6.992	6.150	956782	621876	549.874	550.659

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
Data File : PP033438.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Feb 2021 10:58
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 13:38:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

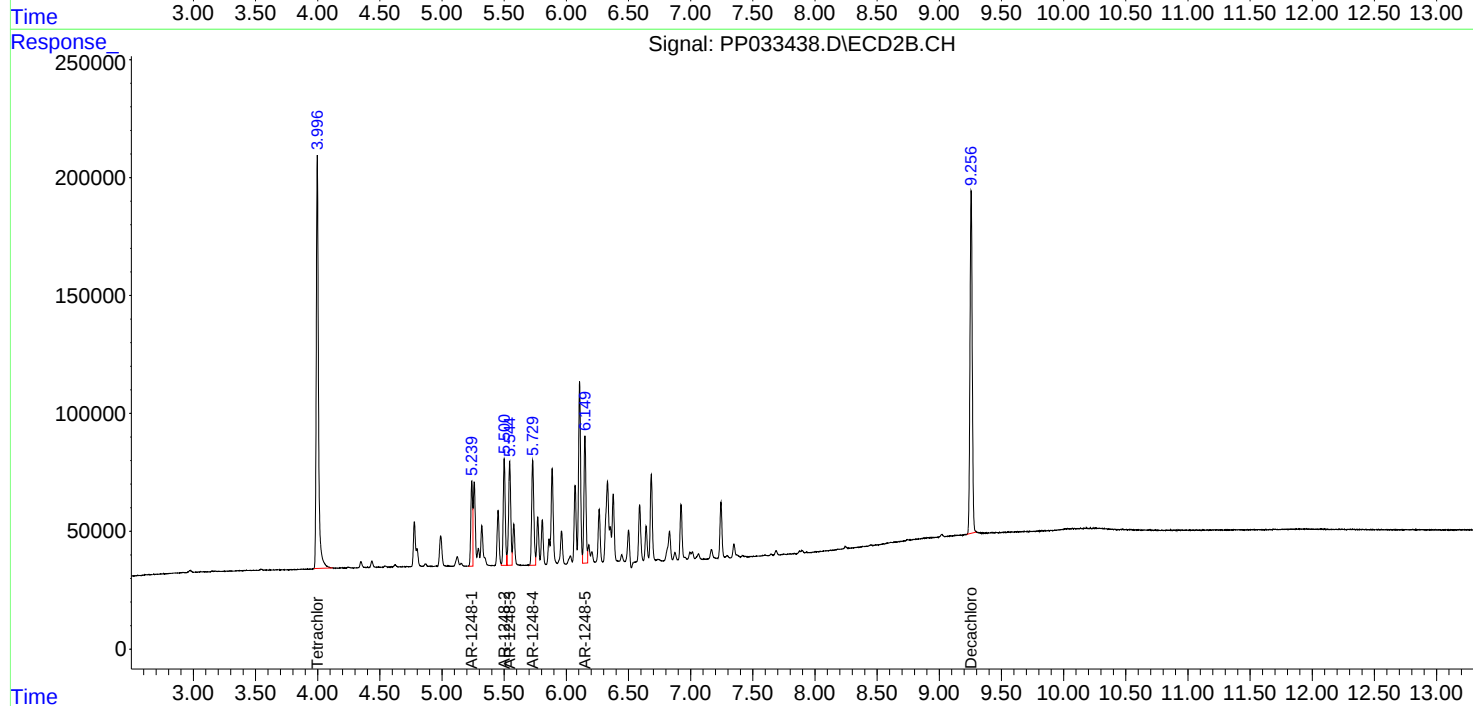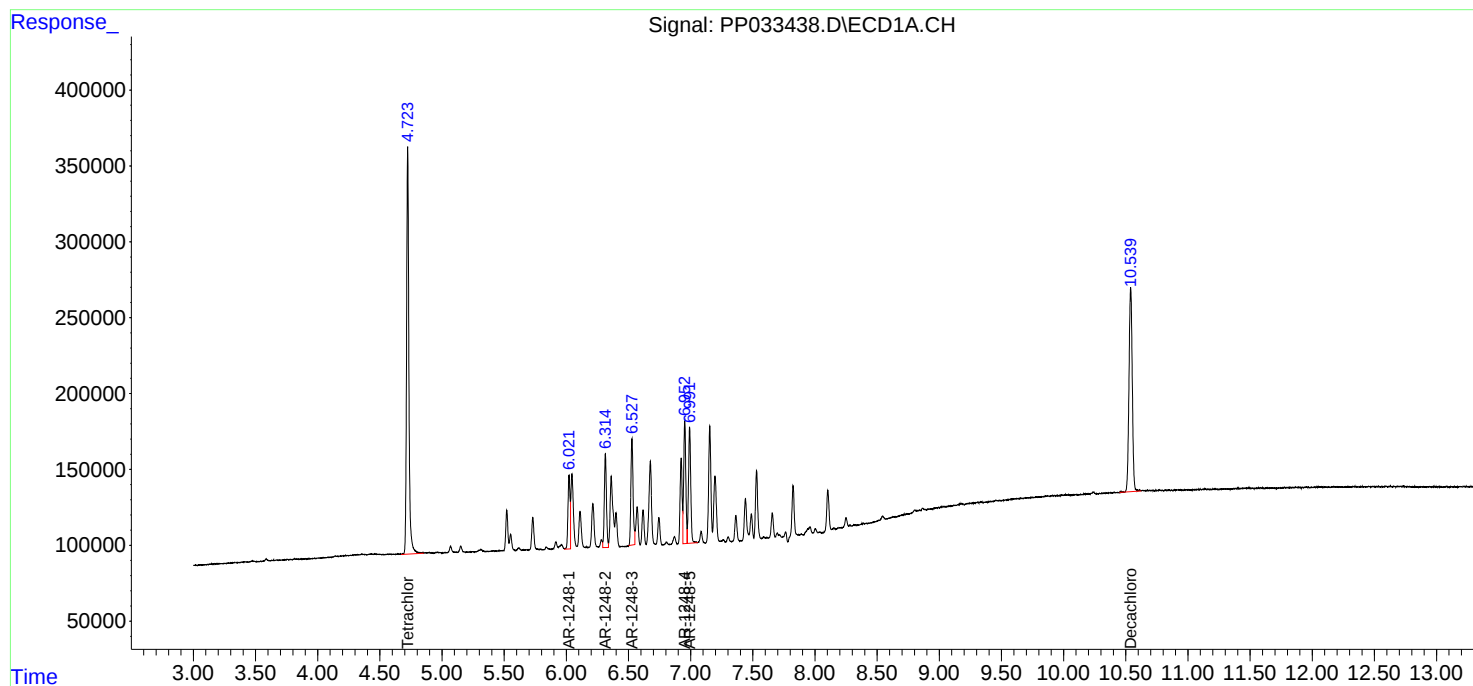

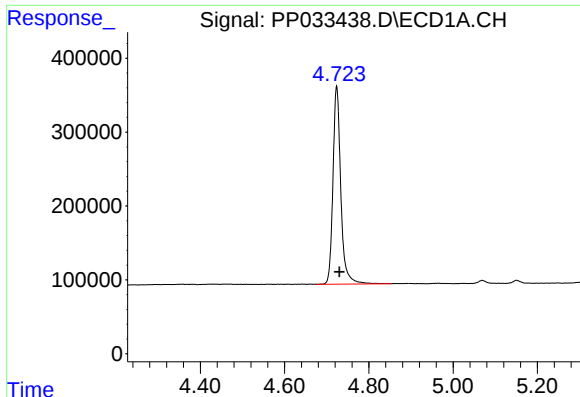


#1 Tetrachloro-m-xylene

R.T.: 4.724 min
Delta R.T.: -0.006 min
Response: 3466841
Conc: 56.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:33 AM

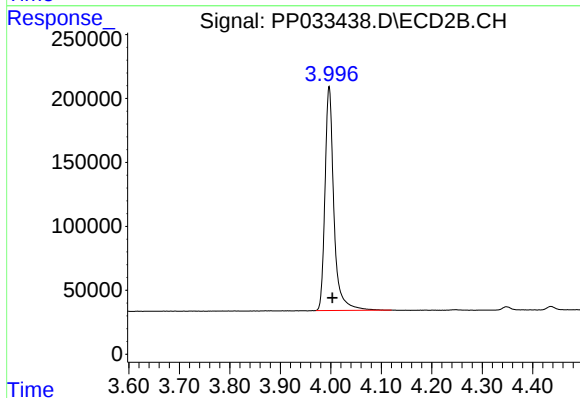


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 2147387
Conc: 52.51 ng/ml

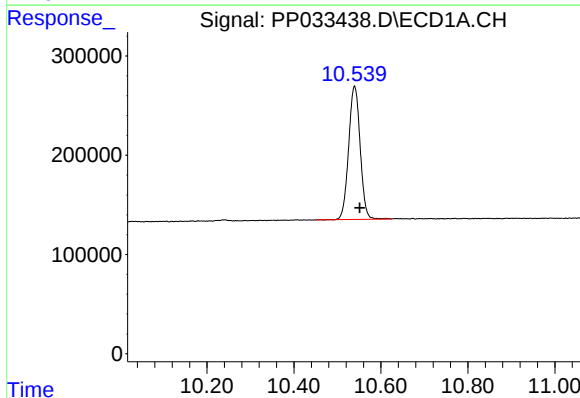


#2 Decachlorobiphenyl

R.T.: 10.539 min
Delta R.T.: -0.012 min
Response: 2465272
Conc: 56.59 ng/ml

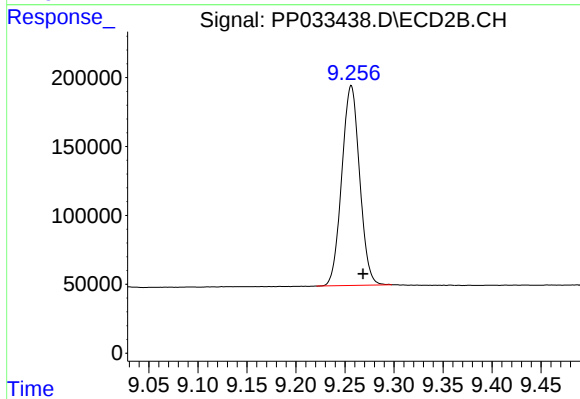

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.012 min
Response: 1837986
Conc: 54.87 ng/ml

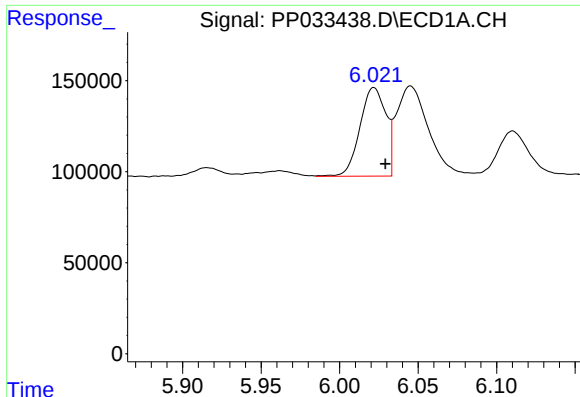


#21 AR-1248-1

R.T.: 6.022 min
Delta R.T.: -0.007 min
Response: 559415
Conc: 584.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:33 AM

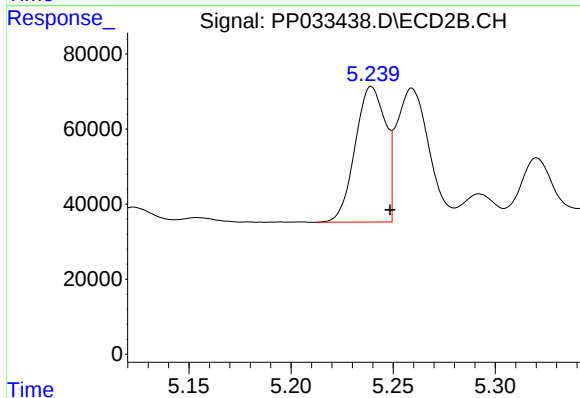


#21 AR-1248-1

R.T.: 5.239 min
Delta R.T.: -0.009 min
Response: 374260
Conc: 575.49 ng/ml

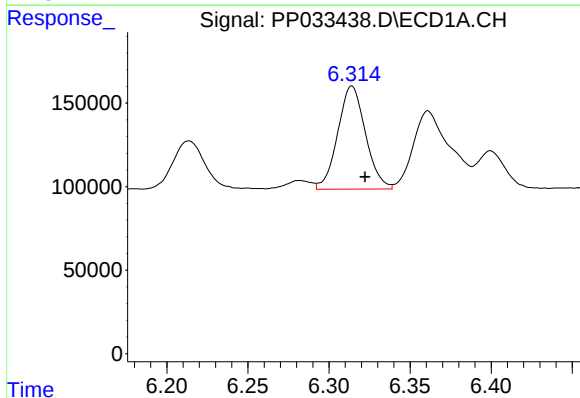


#22 AR-1248-2

R.T.: 6.314 min
Delta R.T.: -0.008 min
Response: 736247
Conc: 555.63 ng/ml

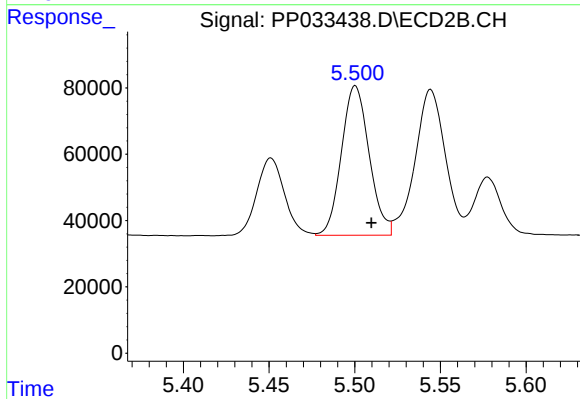

#22 AR-1248-2

R.T.: 5.500 min
Delta R.T.: -0.009 min
Response: 507664
Conc: 529.17 ng/ml

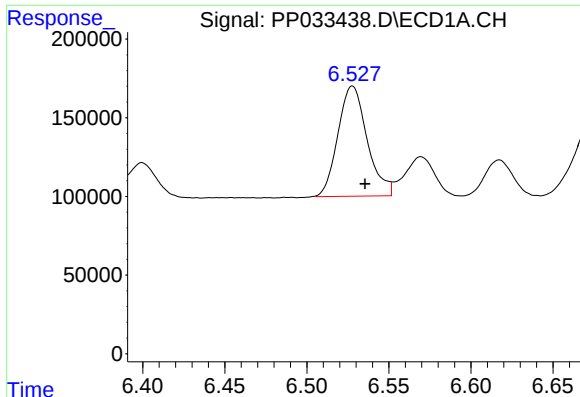


#23 AR-1248-3

R.T.: 6.527 min
Delta R.T.: -0.008 min
Response: 866346
Conc: 535.02 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:33 AM

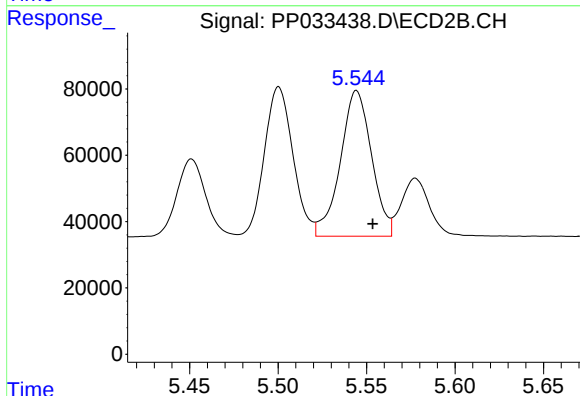


#23 AR-1248-3

R.T.: 5.544 min
Delta R.T.: -0.009 min
Response: 539894
Conc: 531.00 ng/ml

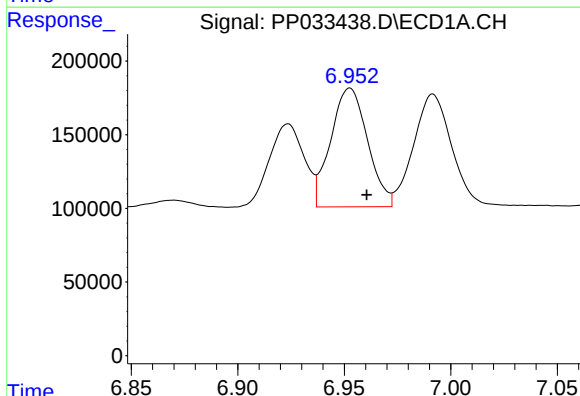


#24 AR-1248-4

R.T.: 6.953 min
Delta R.T.: -0.008 min
Response: 973499
Conc: 565.78 ng/ml

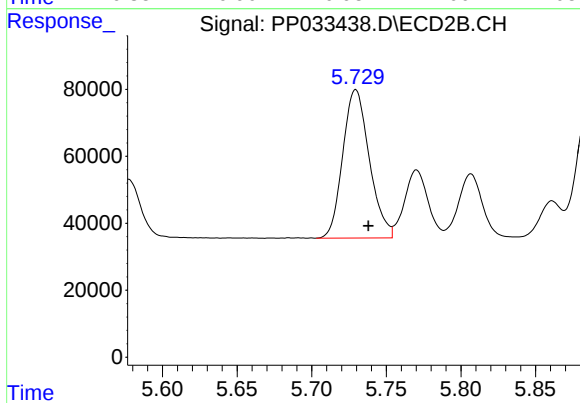

#24 AR-1248-4

R.T.: 5.729 min
Delta R.T.: -0.008 min
Response: 549089
Conc: 443.07 ng/ml

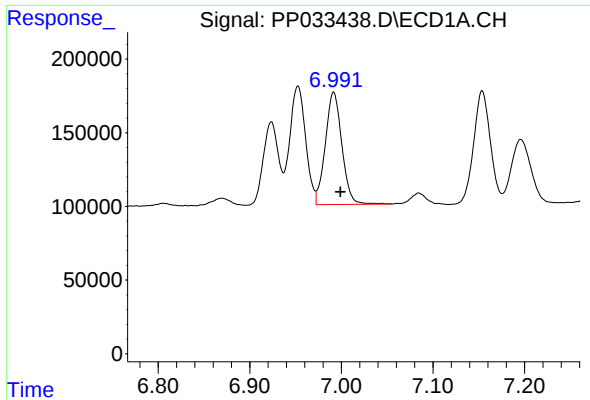


#25 AR-1248-5

R.T.: 6.992 min
Delta R.T.: -0.007 min
Response: 956782
Conc: 549.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:33 AM

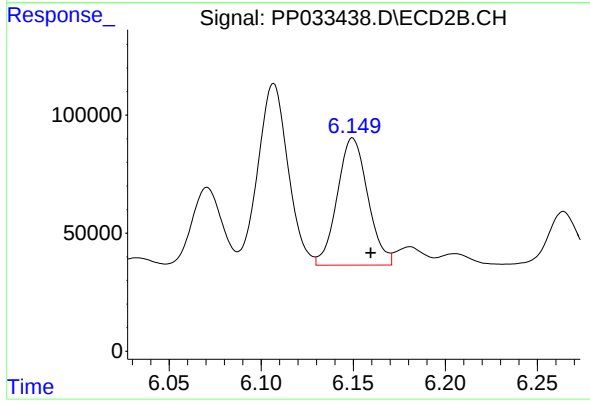

#25 AR-1248-5

R.T.: 6.150 min
Delta R.T.: -0.010 min
Response: 621876
Conc: 550.66 ng/ml