

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
 Data File : PP033459.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Feb 2021 23:27
 Operator : DD\AJ
 Sample : M1449-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RW-2-20210217

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 01:51:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.726	3.998	1236509	775998	20.164	18.977
2)	SA Decachlor...	10.540	9.254	611333	419924	14.034	12.535

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
Data File : PP033459.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Feb 2021 23:27
Operator : DD\AJ
Sample : M1449-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RW-2-20210217

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 01:51:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

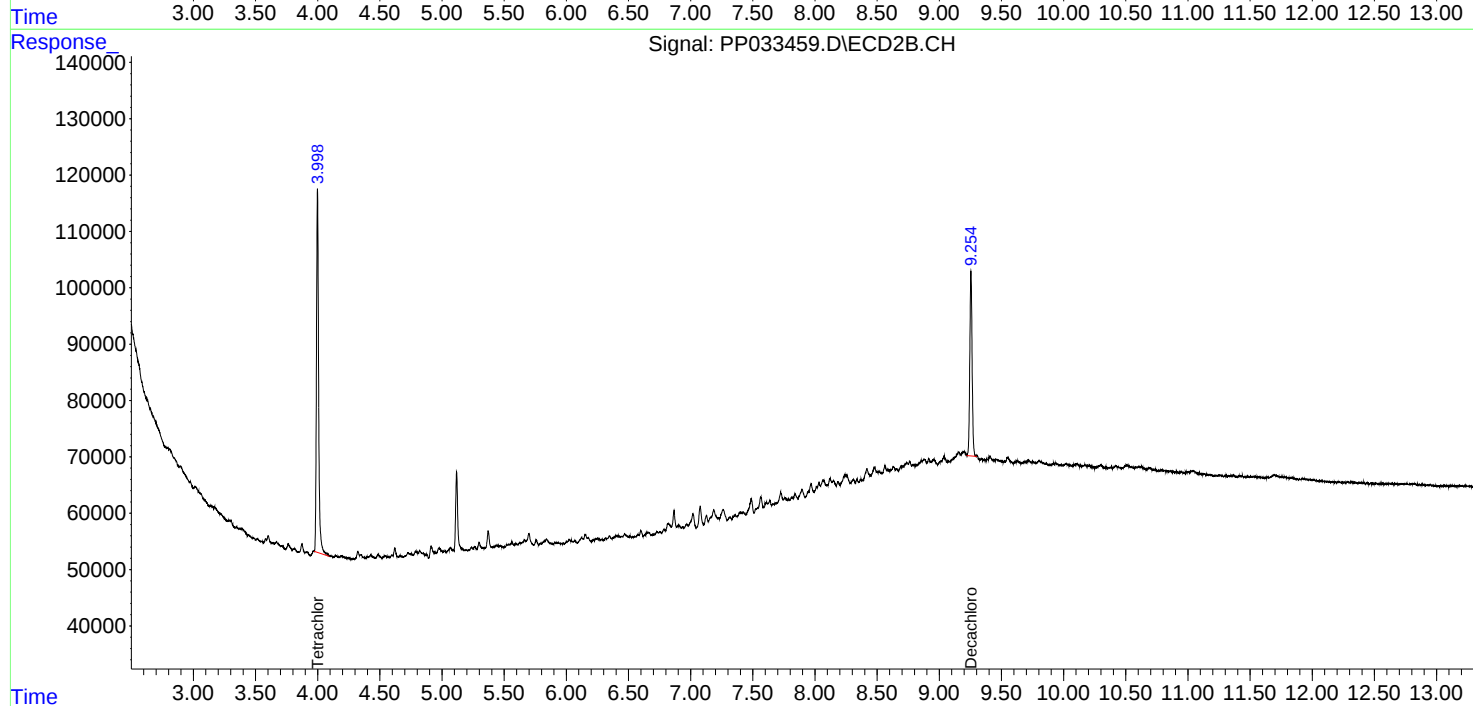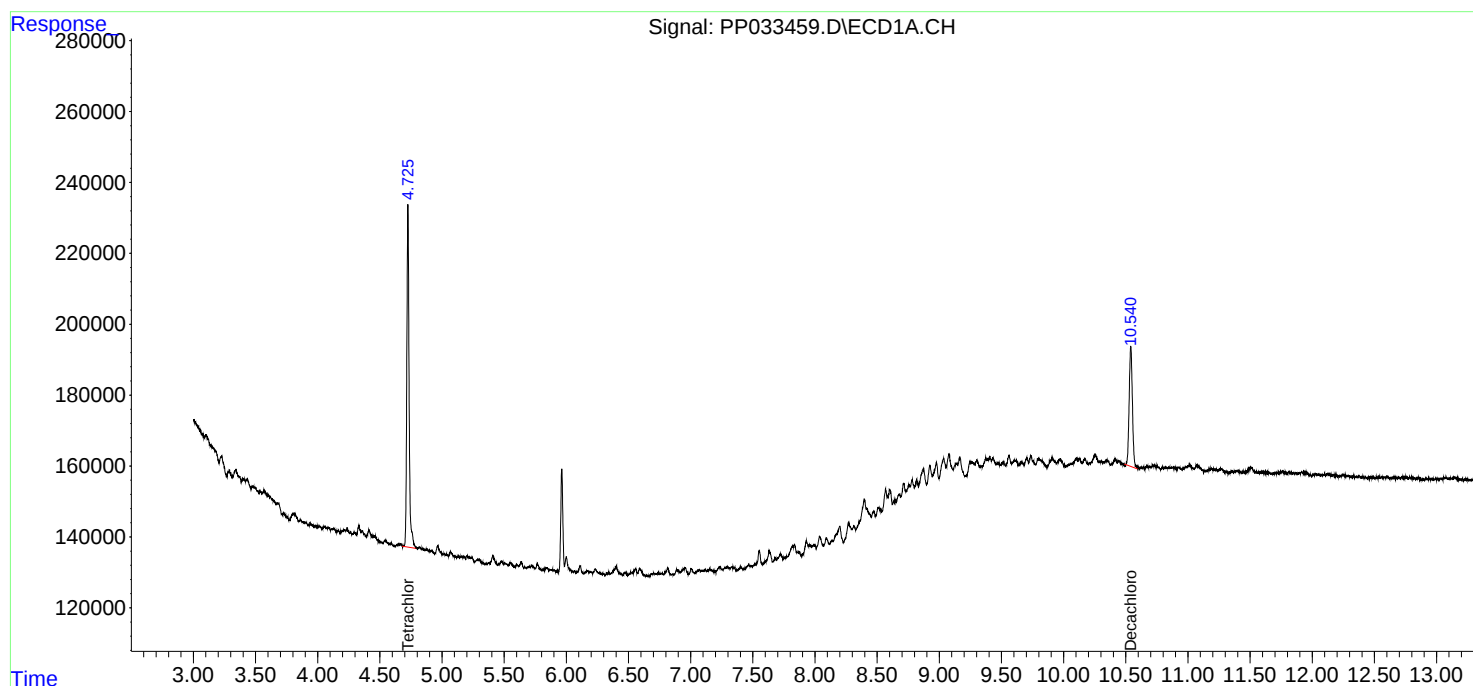


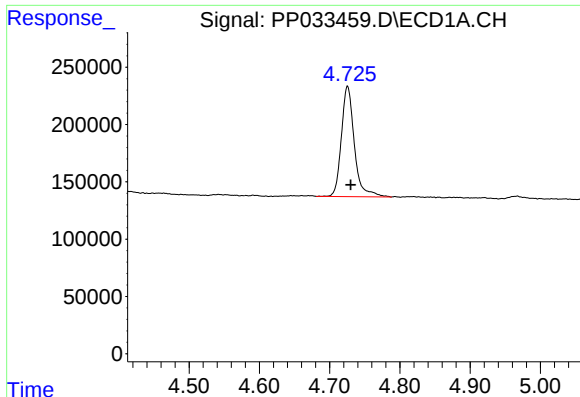

#1 Tetrachloro-m-xylene


R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 1236509
Conc: 20.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
RW-2-20210217

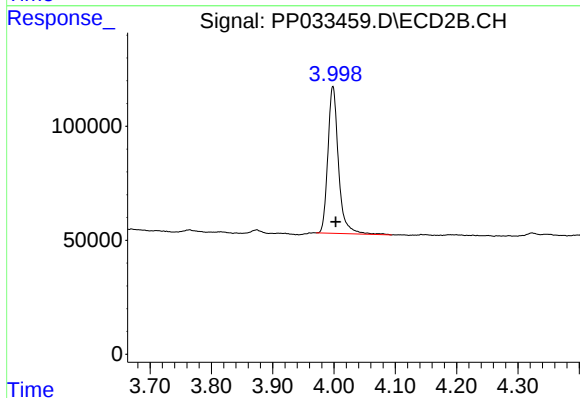


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 775998
Conc: 18.98 ng/ml

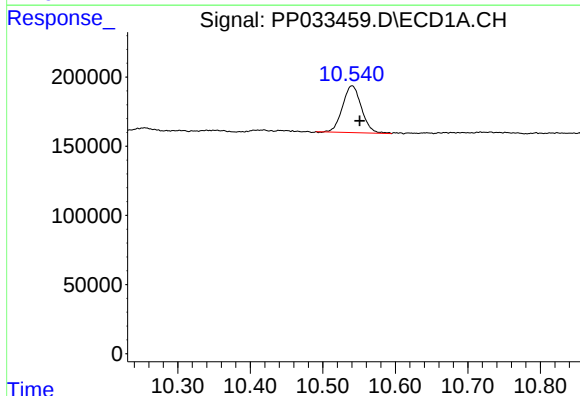

#2 Decachlorobiphenyl

R.T.: 10.540 min
Delta R.T.: -0.011 min
Response: 611333
Conc: 14.03 ng/ml

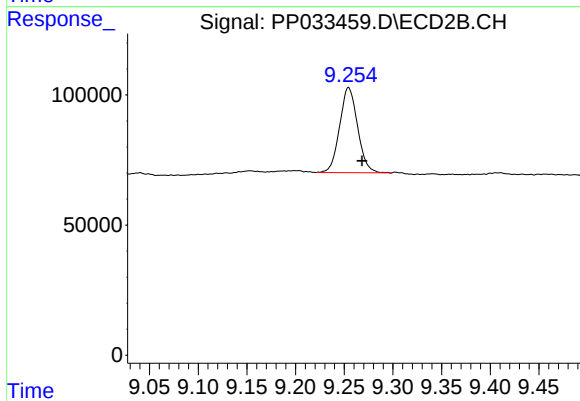

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.014 min
Response: 419924
Conc: 12.54 ng/ml