

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
 Data File : PP033464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Feb 2021 1:08
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/22/2021 10:06:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 01:53:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 04:00:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.724	3.995	3433738	2205125	55.995	53.926
2)	SA Decachlor...	10.541	9.254	2413174	1795453	55.398	53.596
Target Compounds							
21)	L5 AR-1248-1	6.022	5.238	535815	374605	559.620	576.016m
22)	L5 AR-1248-2	6.314	5.499	711347	508693	536.837	530.243
23)	L5 AR-1248-3	6.528	5.543	877911	544181	542.161	535.213
24)	L5 AR-1248-4	6.953	5.728	977356	509345	568.018	411.002 #
25)	L5 AR-1248-5	6.991	6.148	967015	628223	555.755	556.279

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP021921\
Data File : PP033464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Feb 2021 1:08
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 01:53:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 04:00:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

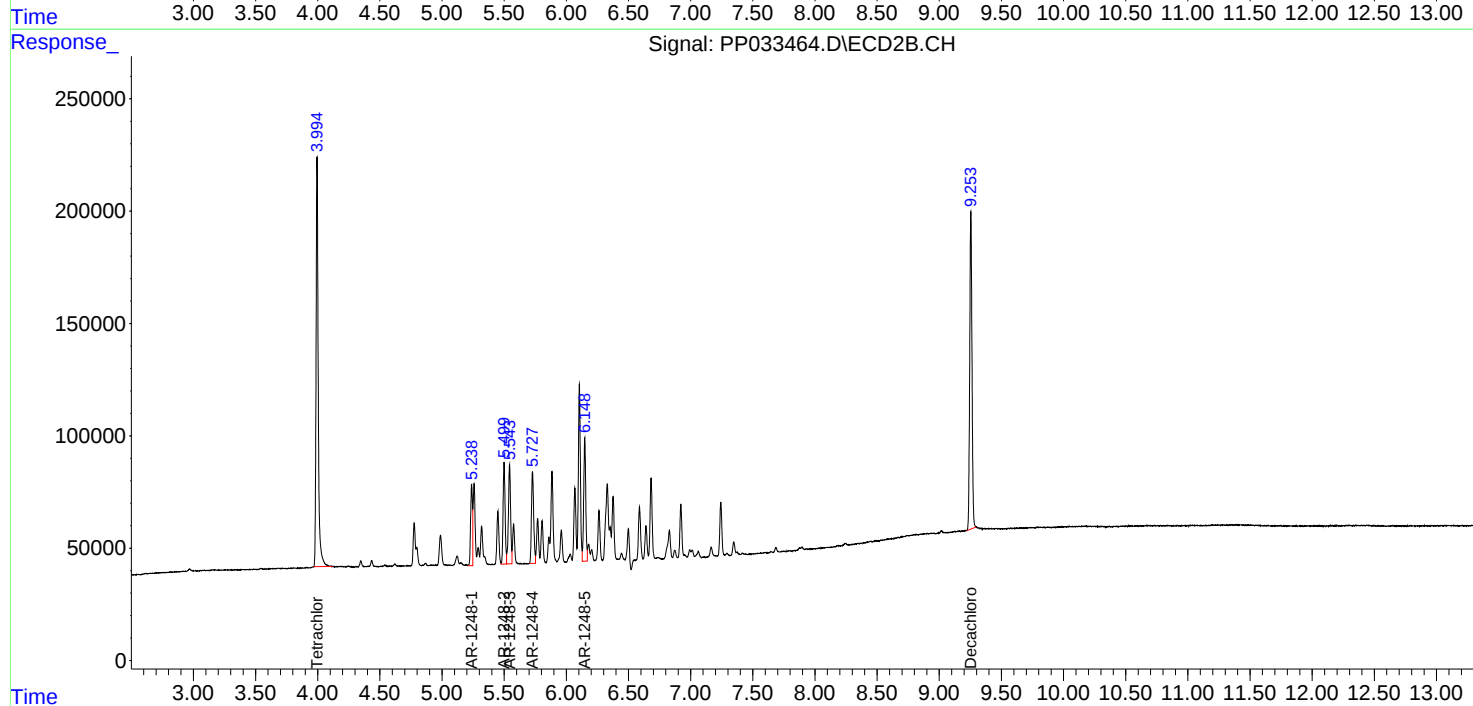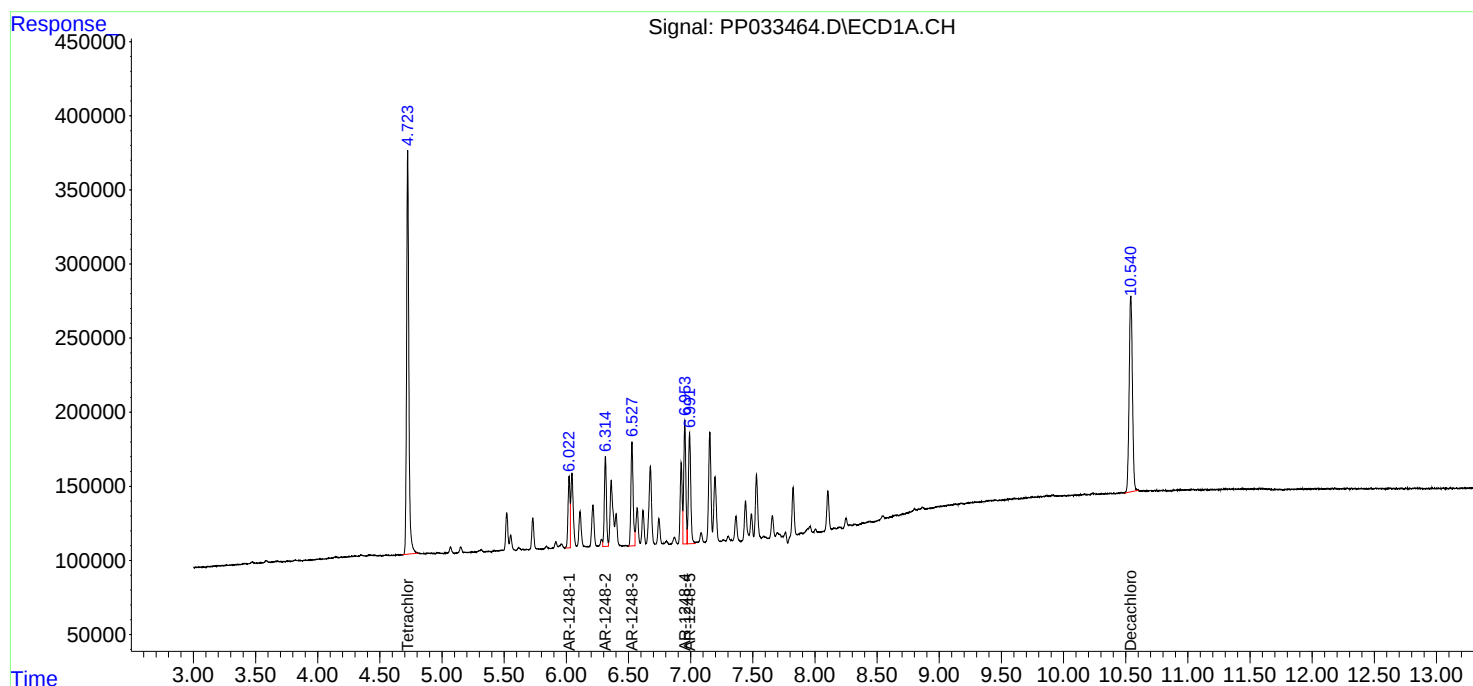

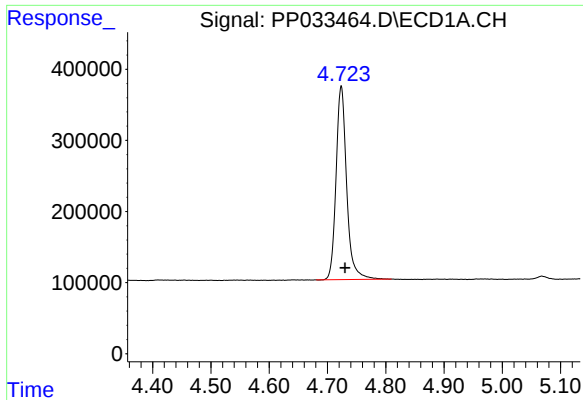


#1 Tetrachloro-m-xylene

R.T.: 4.724 min
Delta R.T.: -0.006 min
Response: 3433738
Conc: 55.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:52 AM

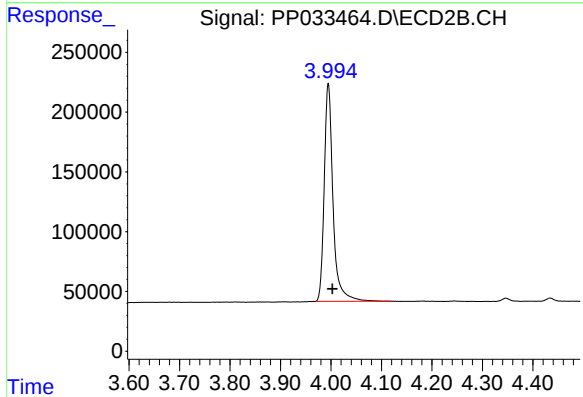


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.008 min
Response: 2205125
Conc: 53.93 ng/ml

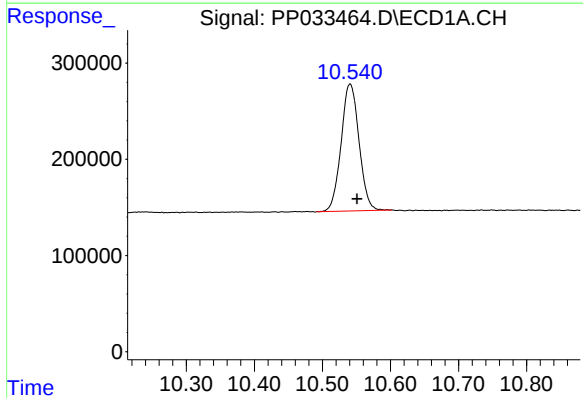


#2 Decachlorobiphenyl

R.T.: 10.541 min
Delta R.T.: -0.010 min
Response: 2413174
Conc: 55.40 ng/ml

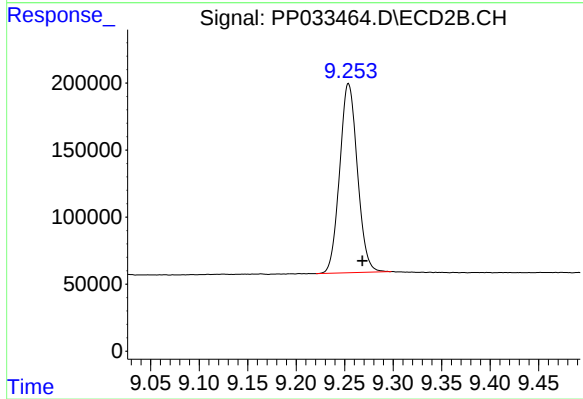

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.014 min
Response: 1795453
Conc: 53.60 ng/ml

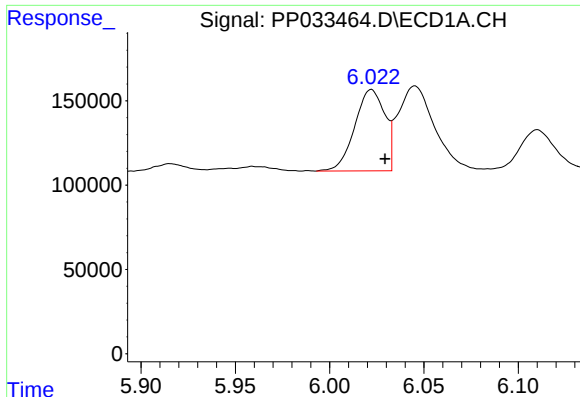


#21 AR-1248-1

R.T.: 6.022 min
Delta R.T.: -0.007 min
Response: 535815
Conc: 559.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:52 AM

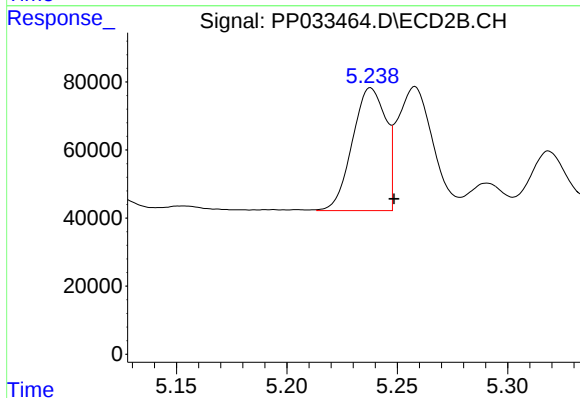


#21 AR-1248-1

R.T.: 5.238 min
Delta R.T.: -0.011 min
Response: 374605
Conc: 576.02 ng/ml m

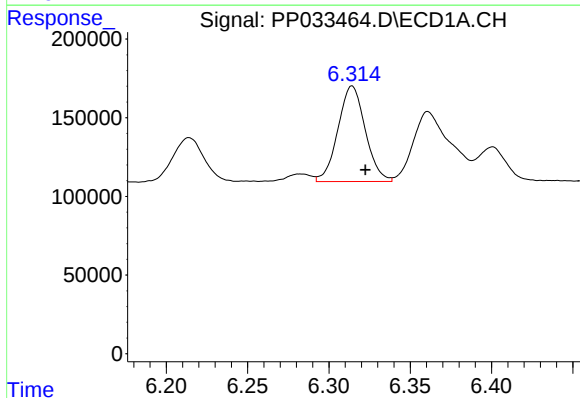


#22 AR-1248-2

R.T.: 6.314 min
Delta R.T.: -0.008 min
Response: 711347
Conc: 536.84 ng/ml

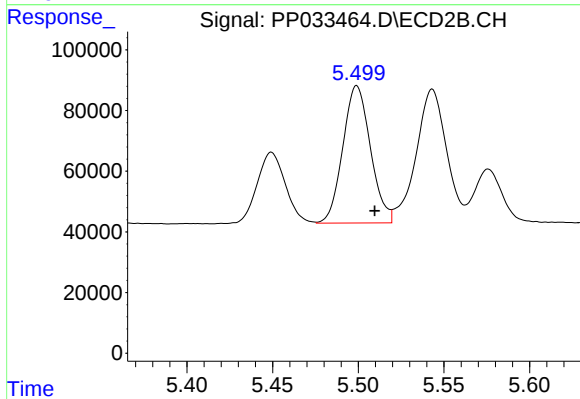

#22 AR-1248-2

R.T.: 5.499 min
Delta R.T.: -0.011 min
Response: 508693
Conc: 530.24 ng/ml

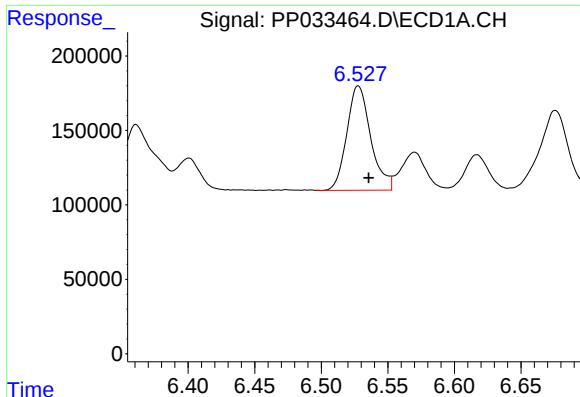


#23 AR-1248-3

R.T.: 6.528 min
Delta R.T.: -0.008 min
Response: 877911
Conc: 542.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:52 AM

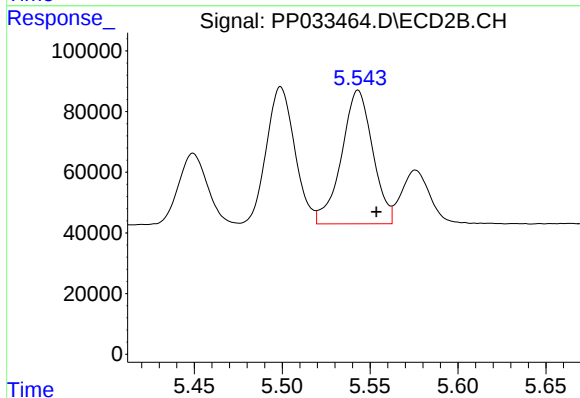


#23 AR-1248-3

R.T.: 5.543 min
Delta R.T.: -0.010 min
Response: 544181
Conc: 535.21 ng/ml

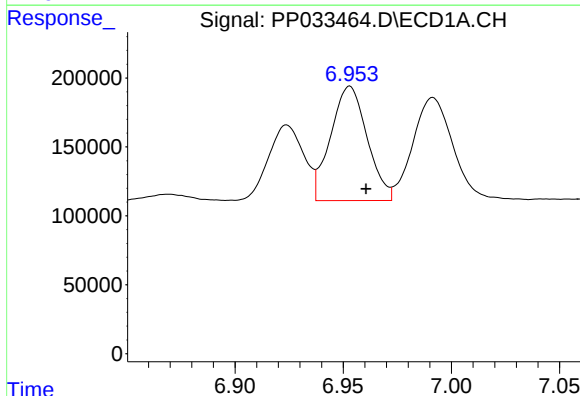


#24 AR-1248-4

R.T.: 6.953 min
Delta R.T.: -0.008 min
Response: 977356
Conc: 568.02 ng/ml

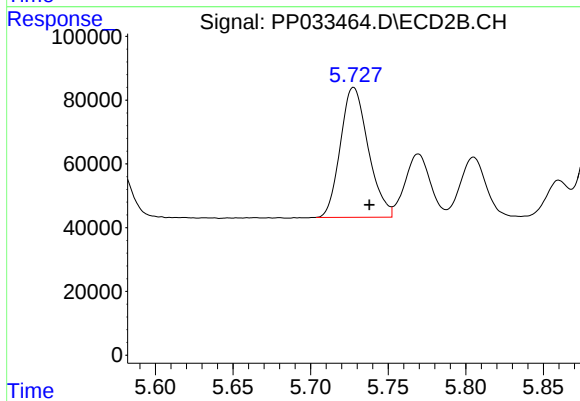

#24 AR-1248-4

R.T.: 5.728 min
Delta R.T.: -0.010 min
Response: 509345
Conc: 411.00 ng/ml

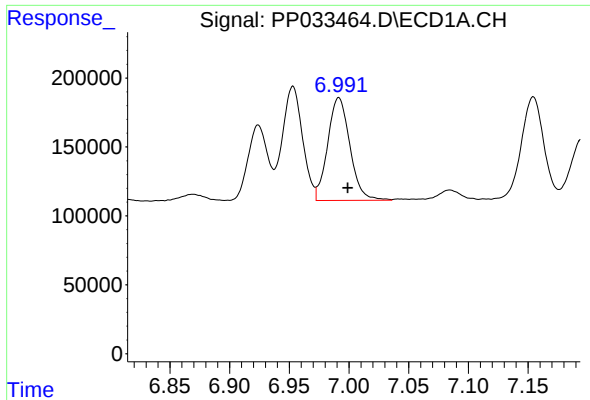


#25 AR-1248-5

R.T.: 6.991 min
Delta R.T.: -0.008 min
Response: 967015
Conc: 555.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/22/2021 10:06:52 AM

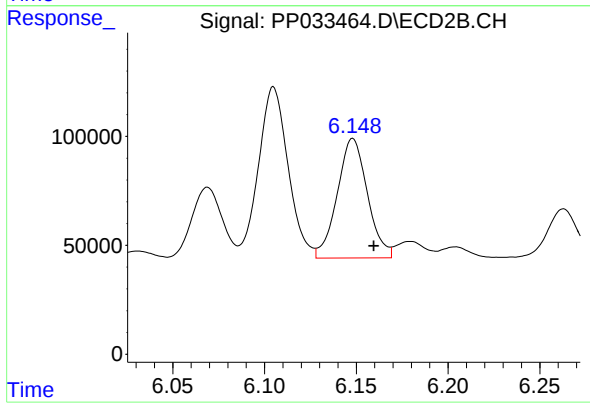

#25 AR-1248-5

R.T.: 6.148 min
Delta R.T.: -0.011 min
Response: 628223
Conc: 556.28 ng/ml