

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022023\
 Data File : PP055817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2023 19:34
 Operator : YP\AJ
 Sample : 01597-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NYE-WATER-0217

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2023
 Supervised By :Ankita Jodhani 02/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:59:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.569	28850550	25458292	17.906	17.435m
2) SA Decachlor...	10.079	8.576	33378619	17856651	16.362	15.740

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022023\
Data File : PP055817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2023 19:34
Operator : YP\AJ
Sample : 01597-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NYE-WATER-0217


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2023
Supervised By :Ankita Jodhani 02/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:59:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

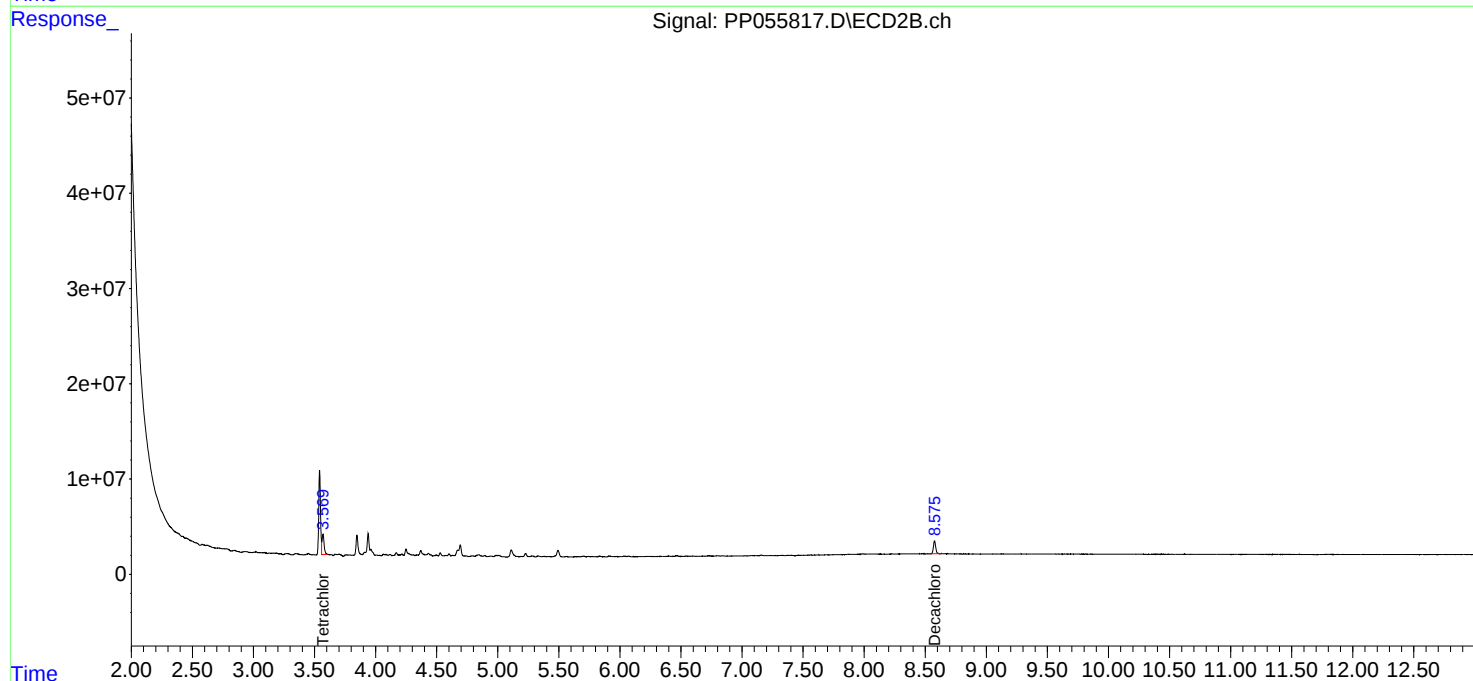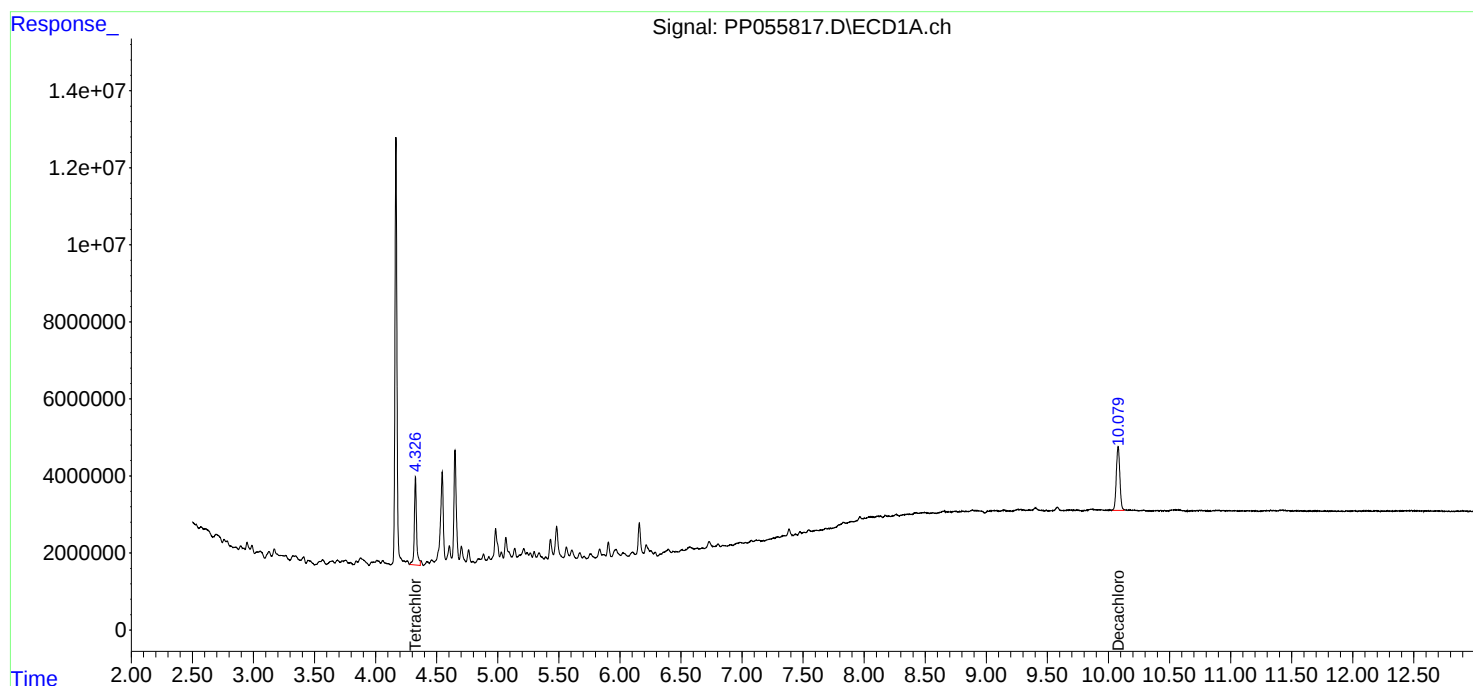

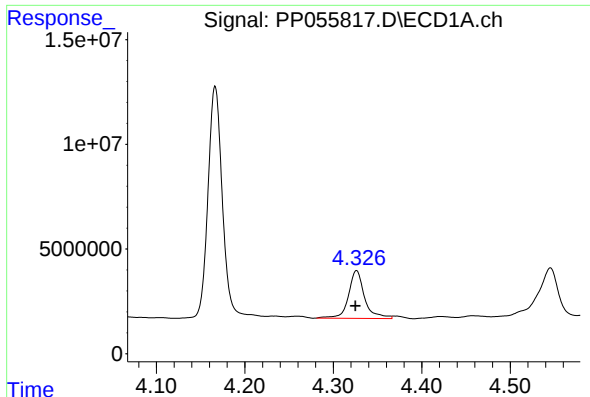


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: 0.001 min
Response: 28850550
Conc: 17.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
NYE-WATER-0217


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2023
Supervised By :Ankita Jodhani 02/21/2023

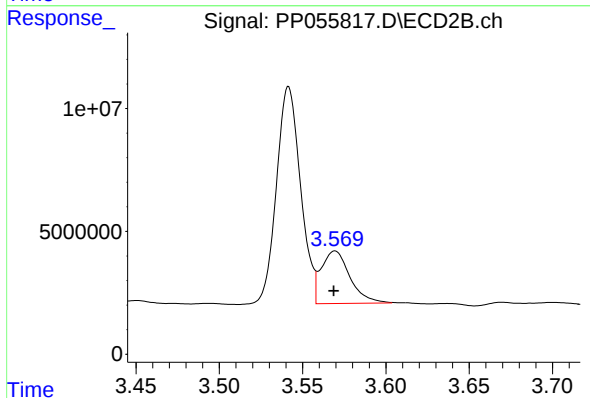


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 25458292
Conc: 17.44 ng/ml m

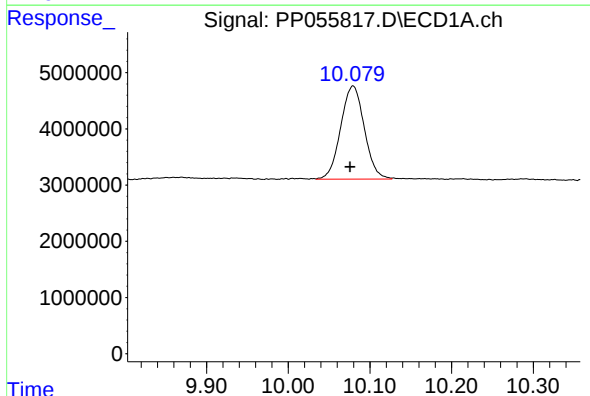

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: 0.003 min
Response: 33378619
Conc: 16.36 ng/ml

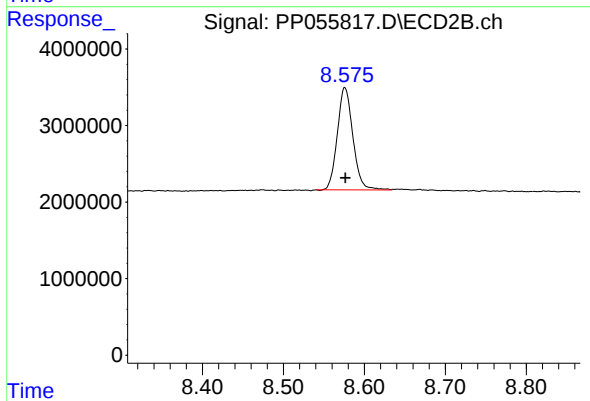

#2 Decachlorobiphenyl

R.T.: 8.576 min
Delta R.T.: 0.000 min
Response: 17856651
Conc: 15.74 ng/ml