

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
 Data File : PP069907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 13:59
 Operator : YP\AJ
 Sample : Q1392-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 435

Manual Integrations APPROVED

Reviewed By :Yogesh
 Patel

02/21/2025

Supervised By :Ankita
 Jodhani
 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 14:49:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.520	3.835	1886492	916267	1.318m	1.027m
2) SA Decachlor...	10.251	8.889	1419203	1241446	1.299m	1.110

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
Data File : PP069907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 13:59
Operator : YP\AJ
Sample : Q1392-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
435



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
02/21/2025

Supervised By :Ankita
Jodhani
02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 14:49:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

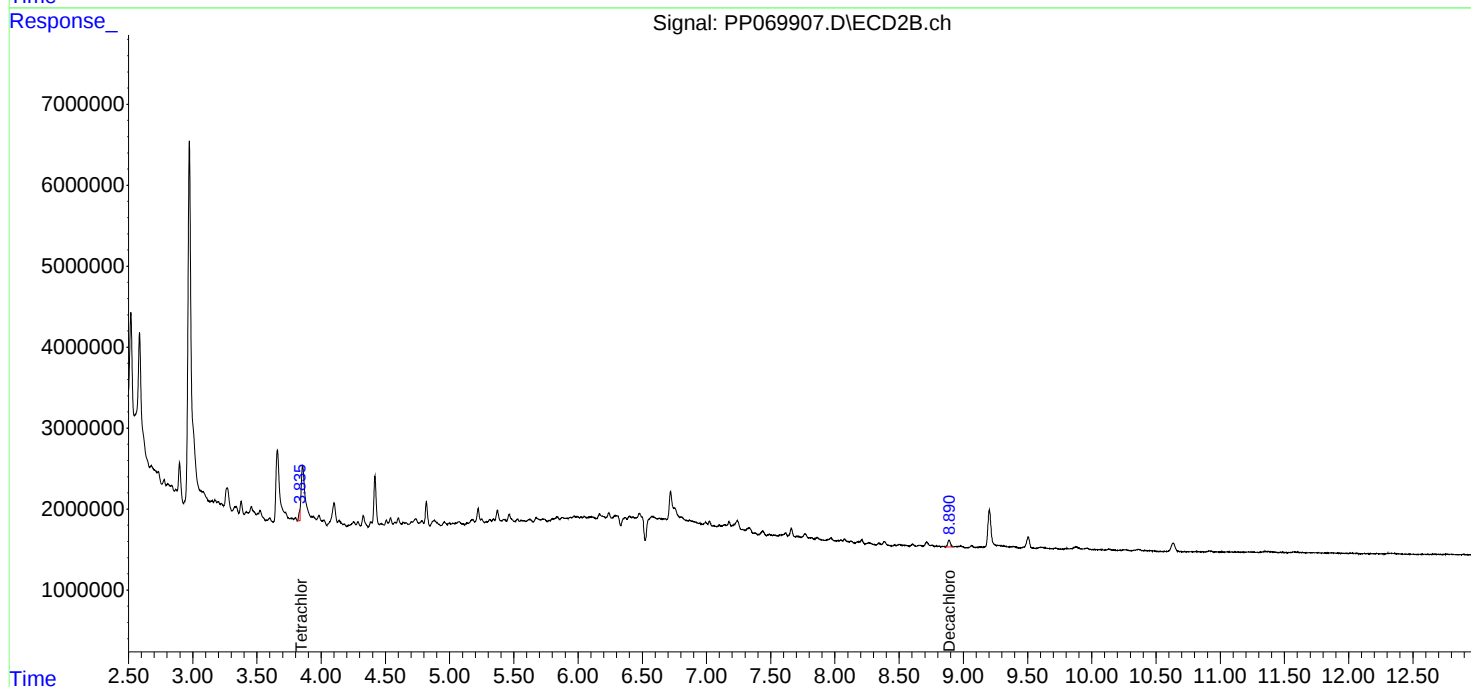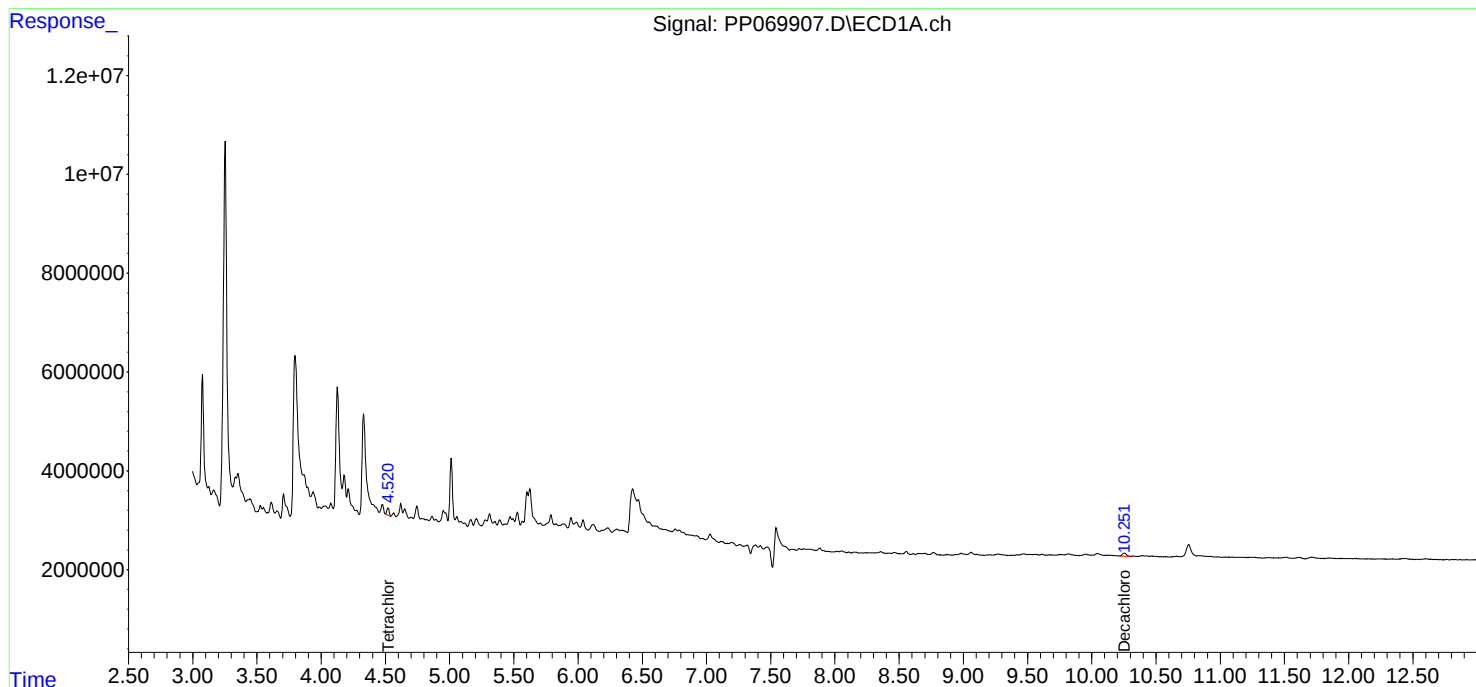

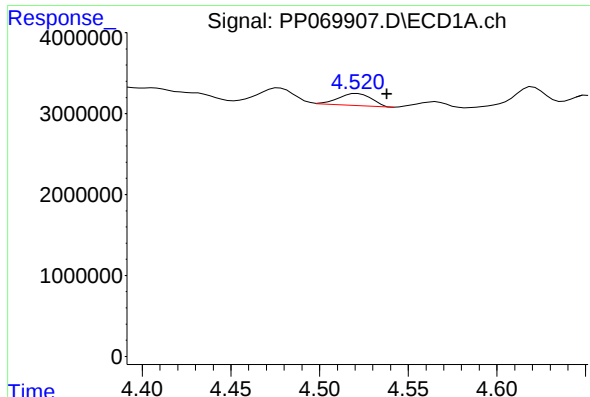

#1 Tetrachloro-m-xylene


R.T.: 4.520 min
Delta R.T.: -0.018 min
Response: 1886492
Conc: 1.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
435

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
02/21/2025

Supervised By :Ankita
Jodhani
02/21/2025

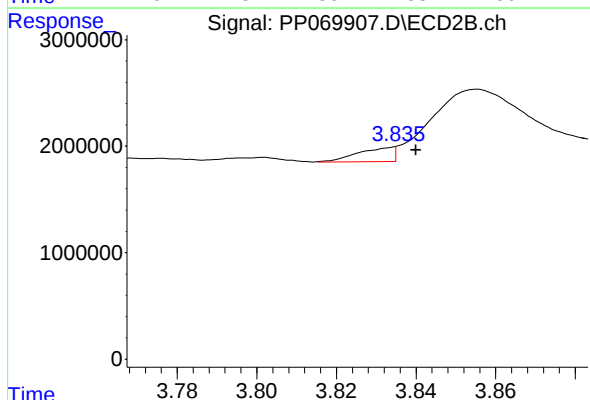


#1 Tetrachloro-m-xylene

R.T.: 3.835 min
Delta R.T.: -0.005 min
Response: 916267
Conc: 1.03 ng/ml

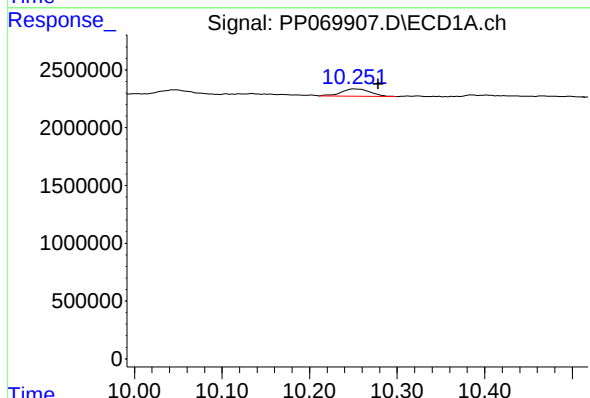

#2 Decachlorobiphenyl

R.T.: 10.251 min
Delta R.T.: -0.027 min
Response: 1419203
Conc: 1.30 ng/ml

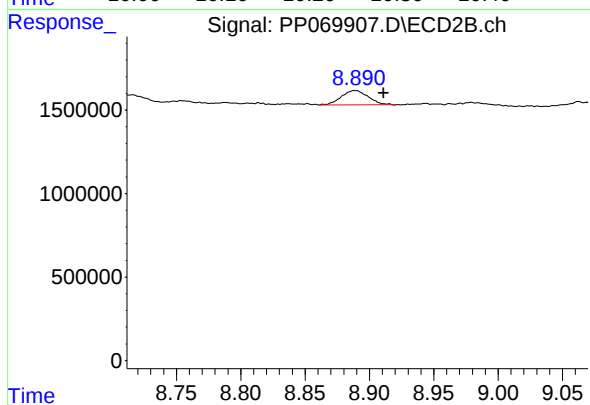

#2 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: -0.022 min
Response: 1241446
Conc: 1.11 ng/ml