

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
 Data File : PP069922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:24
 Operator : YP\AJ
 Sample : Q1390-02 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 3772

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:51:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.830	3346626	1658777	2.338m	1.858
2) SA Decachlor...	10.257	8.893	1788858	2657557	1.637	2.376 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
Data File : PP069922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:24
Operator : YP\AJ
Sample : Q1390-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
3772


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:51:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

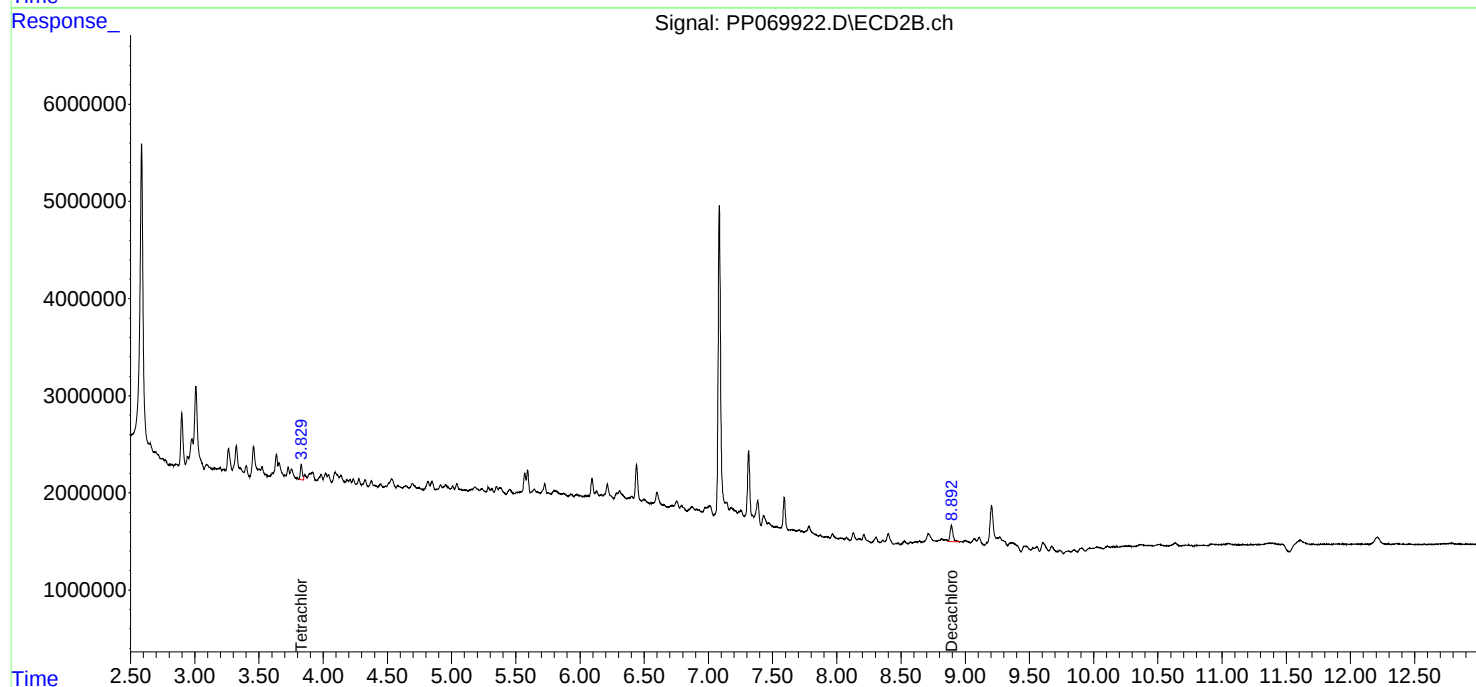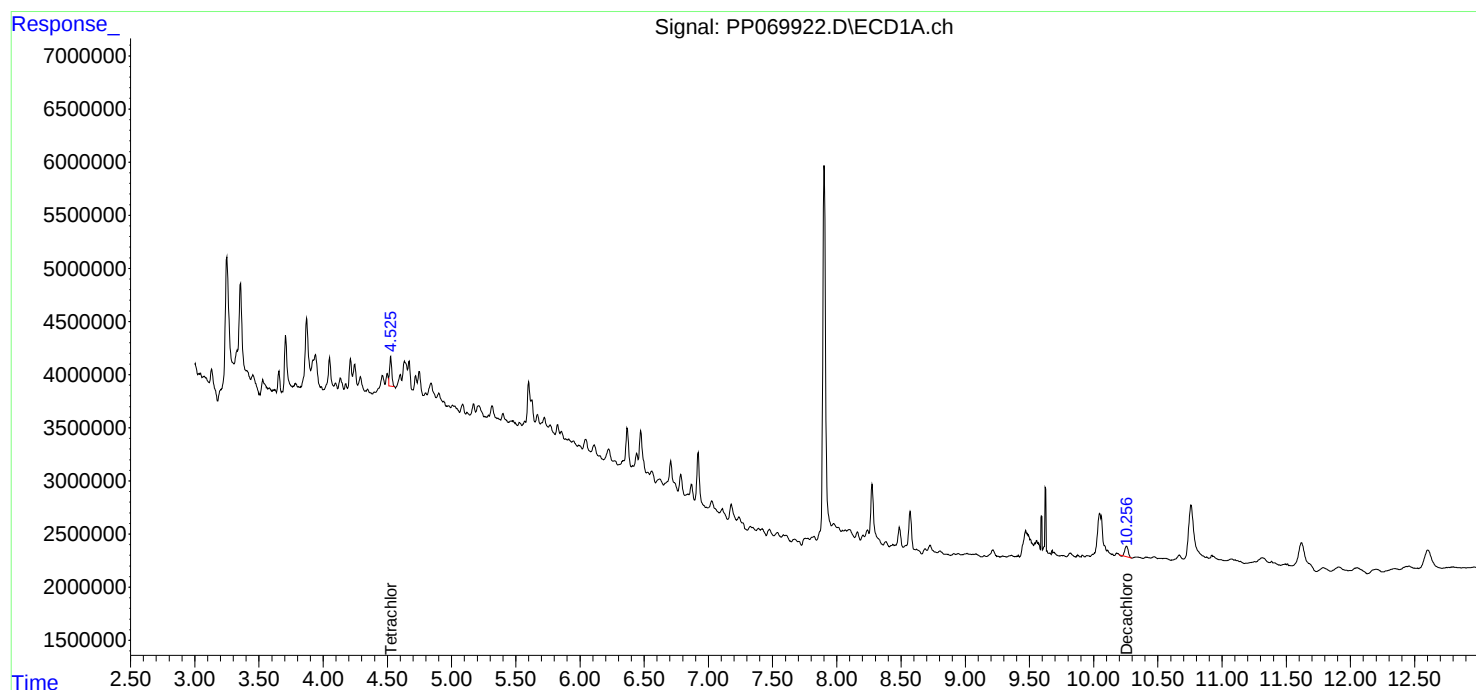

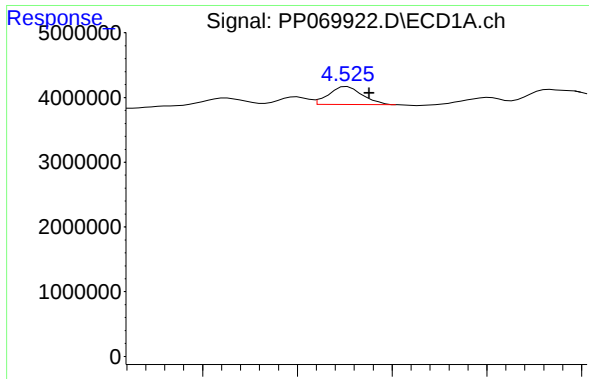


#1 Tetrachloro-m-xylene

R.T.: 4.525 min
Delta R.T.: -0.013 min
Response: 3346626
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
3772


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

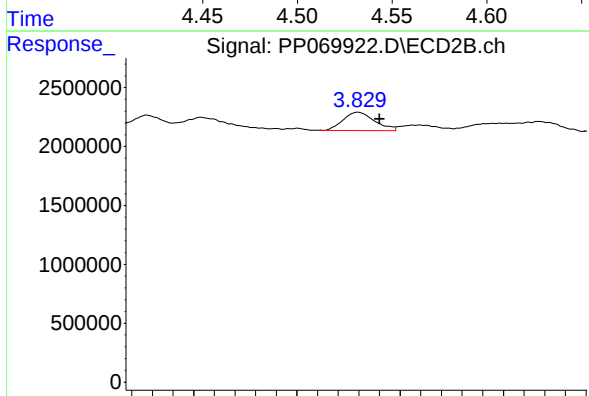


#1 Tetrachloro-m-xylene

R.T.: 3.830 min
Delta R.T.: -0.010 min
Response: 1658777
Conc: 1.86 ng/ml

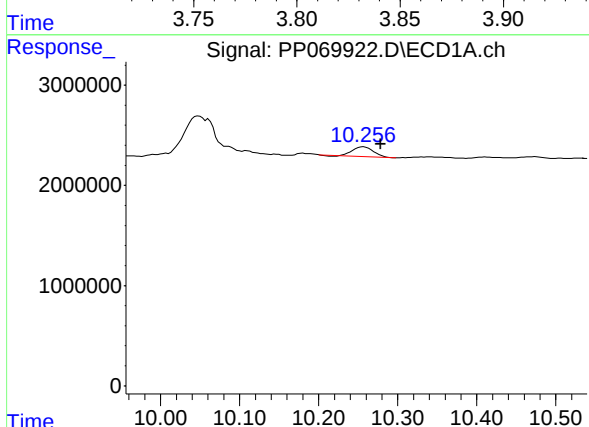

#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: -0.022 min
Response: 1788858
Conc: 1.64 ng/ml

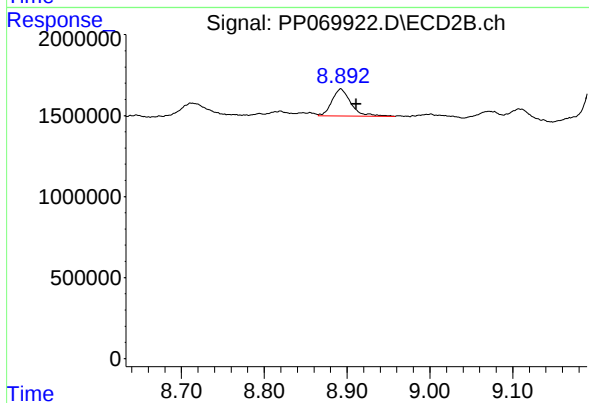

#2 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.019 min
Response: 2657557
Conc: 2.38 ng/ml