

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
 Data File : PP069930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:34
 Operator : YP\AJ
 Sample : Q1382-07RE
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OU4-PCS-TC-04-021725RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:54:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.829	40598309	24795924	28.361	27.781m
2) SA Decachlor...	10.252	8.888	26213438	26681553	23.985	23.855

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022025\
Data File : PP069930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:34
Operator : YP\AJ
Sample : Q1382-07RE
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OU4-PCS-TC-04-021725RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:54:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

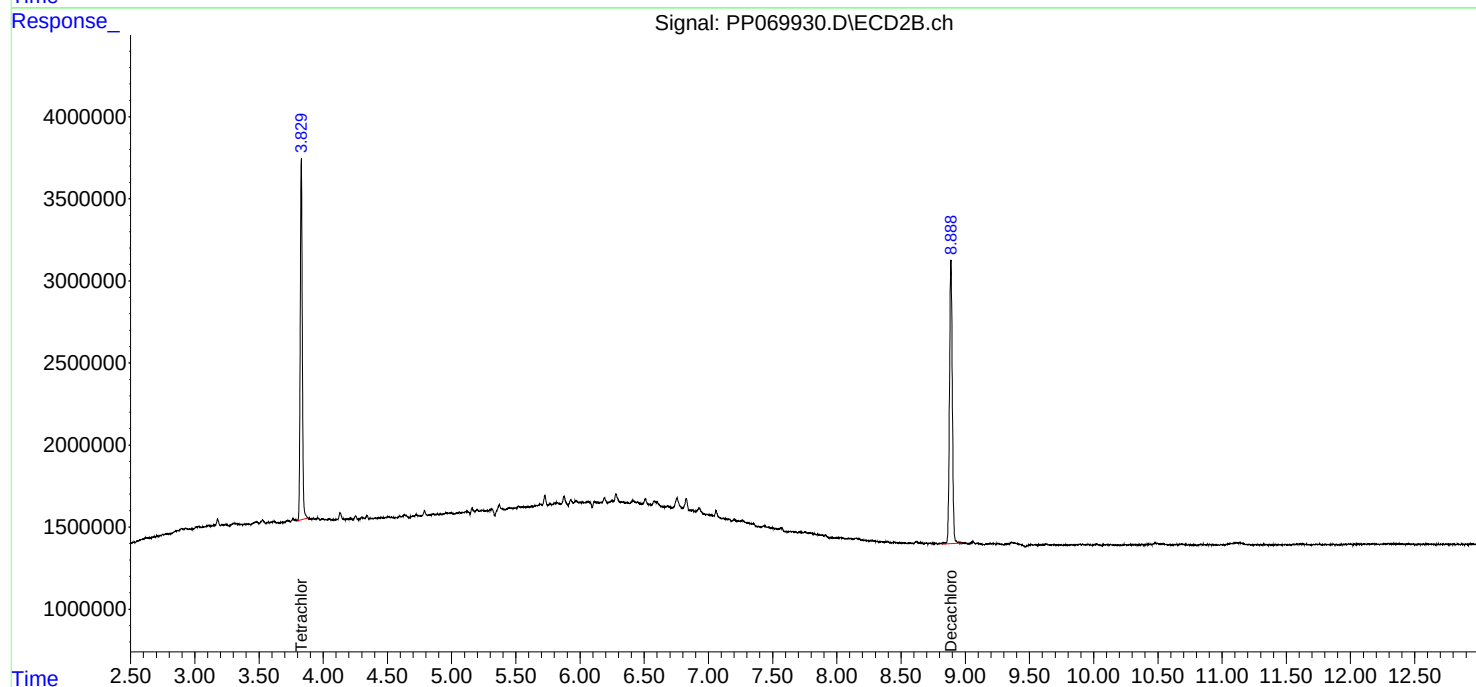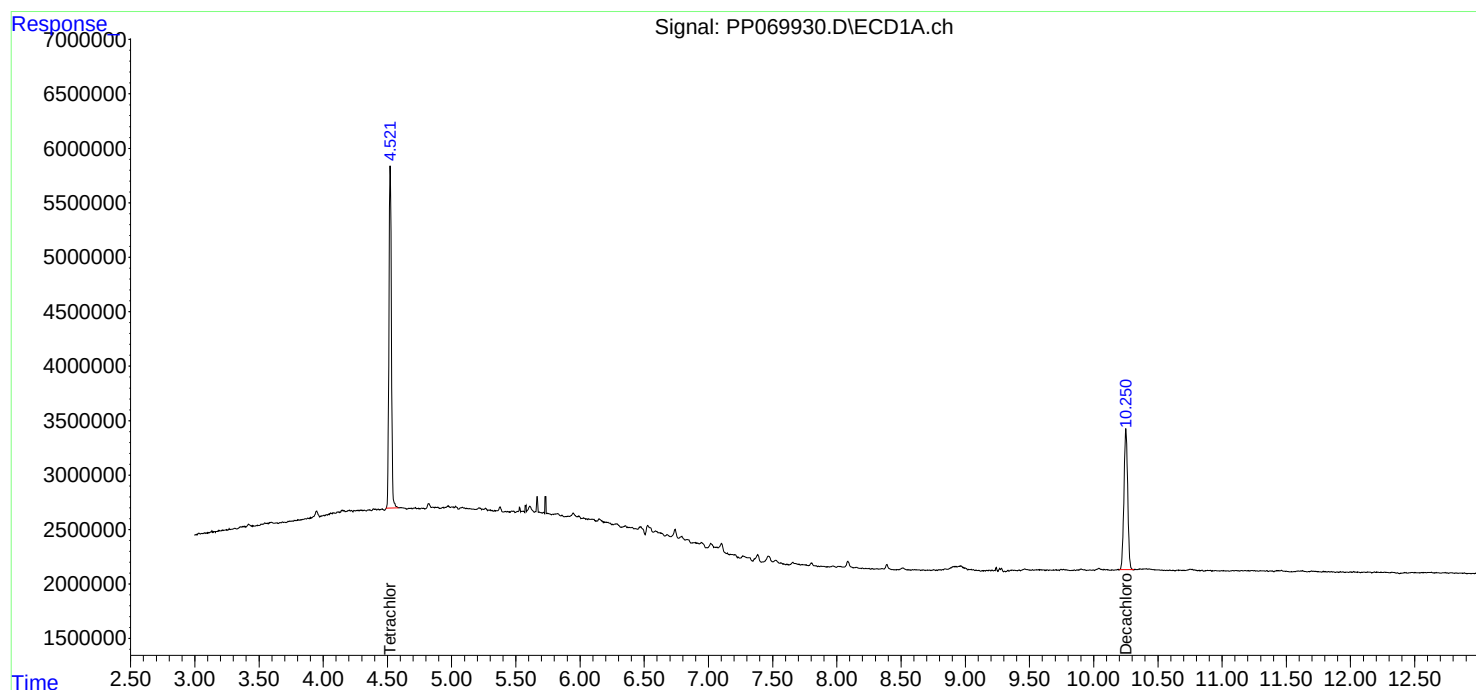

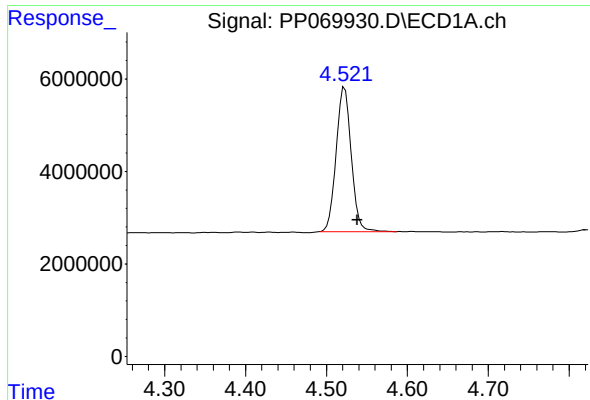


#1 Tetrachloro-m-xylene

R.T.: 4.522 min
Delta R.T.: -0.016 min
Response: 40598309
Conc: 28.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
OU4-PCS-TC-04-021725RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

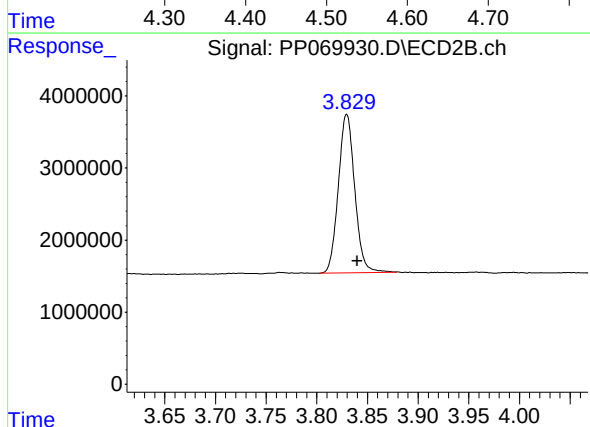


#1 Tetrachloro-m-xylene

R.T.: 3.829 min
Delta R.T.: -0.011 min
Response: 24795924
Conc: 27.78 ng/ml

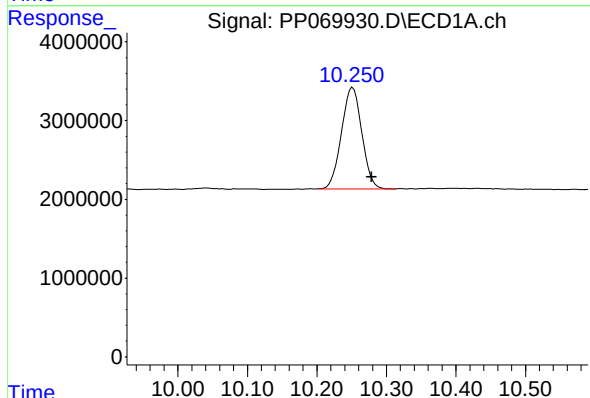

#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: -0.027 min
Response: 26213438
Conc: 23.99 ng/ml

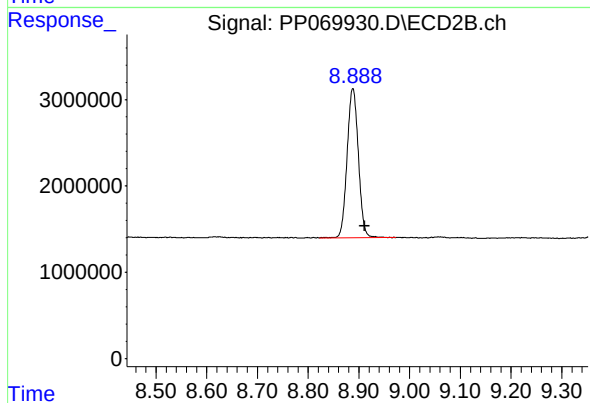

#2 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: -0.023 min
Response: 26681553
Conc: 23.86 ng/ml