

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022119\
 Data File : PP029165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Feb 2019 13:51
 Operator : EI\MA
 Sample : HEXANE
 Misc : hexane
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 02:26:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	12.094	0	4041183	N.D.	106.480 #
Target Compounds							
2) T	3,5-DICHL...	0.000	10.202	0	766824	N.D.	15.130 #
3) T	4-Nitroph...	0.000	11.316	0	9368087	N.D.	391.187 #
5) T	DICAMBA	0.000	12.452	0	216831	N.D.	1.694 #
9) T	2,4-D	0.000	14.078	0	2727274	N.D.	60.147 #
10) T	Pentachlo...	0.000	14.674	0	3457411	N.D.	6.718 #
12) T	2,4,5-T	0.000	15.852	0	20795447	N.D.	125.597 #
13) T	2,4-DB	0.000	16.451	0	25348477	N.D.	1125.269 #
14) T	DINOSEB	0.000	16.793	0	43700524	N.D.	333.408 #
15) T	Picloram	0.000	18.209	0	498.6E6	N.D.	2215.601 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022119\
Data File : PP029165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2019 13:51
Operator : EI\MA
Sample : HEXANE
Misc : hexane
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 02:26:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

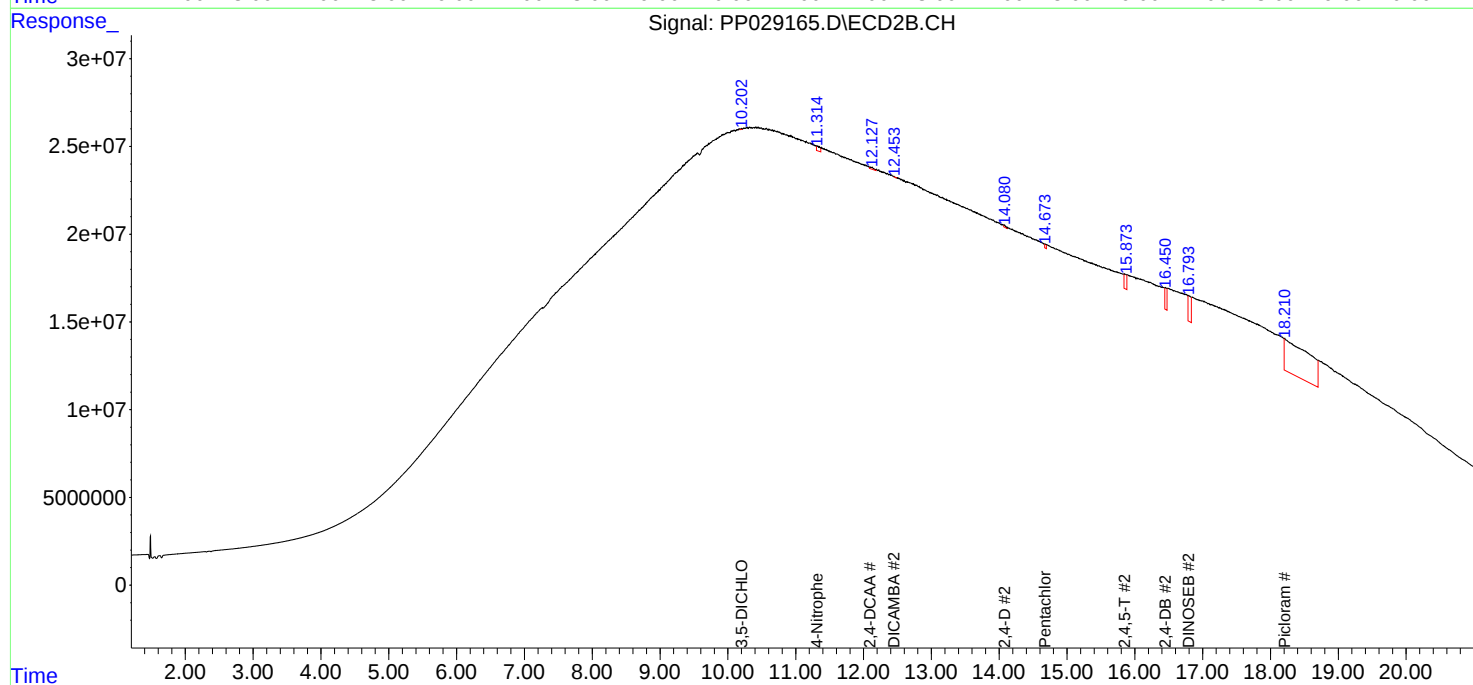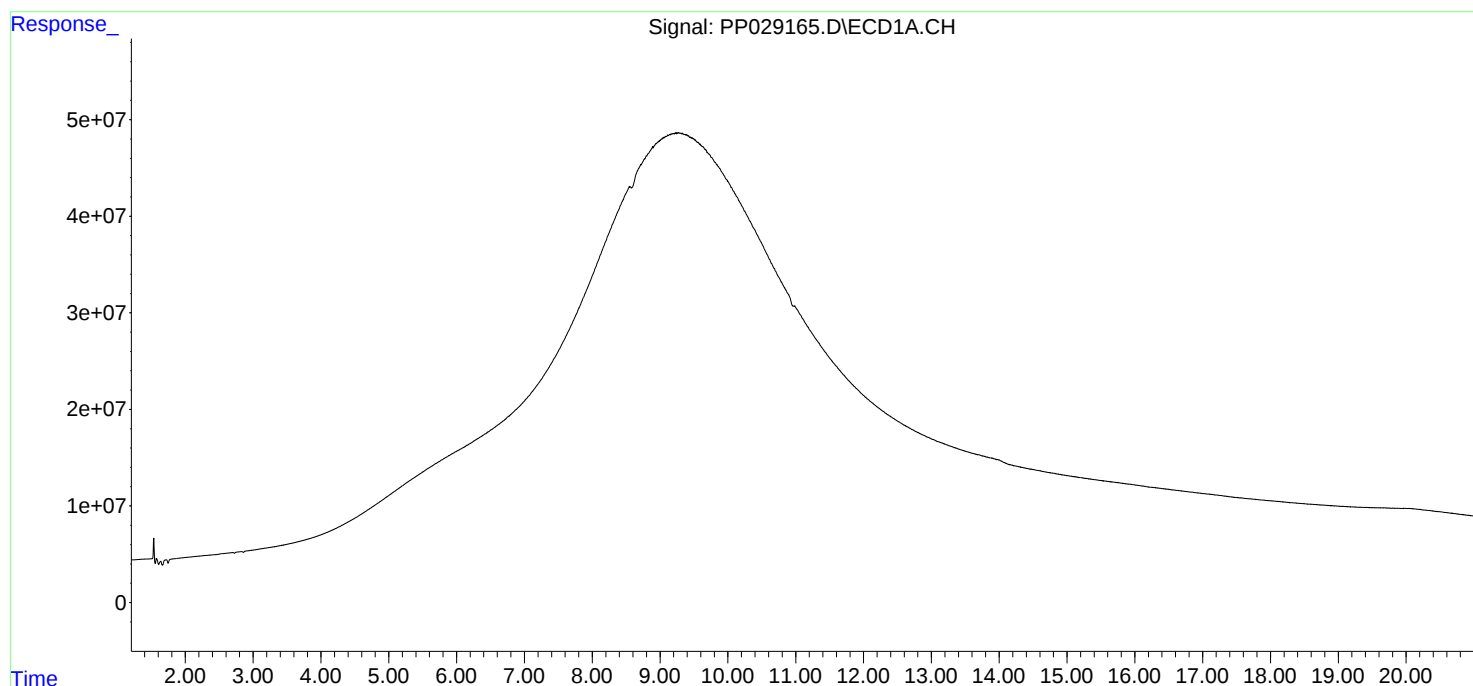


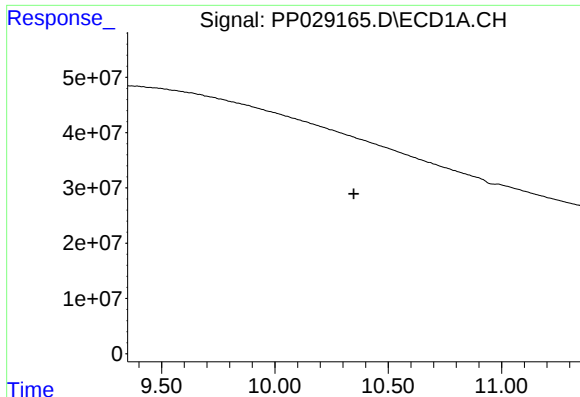

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.348 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

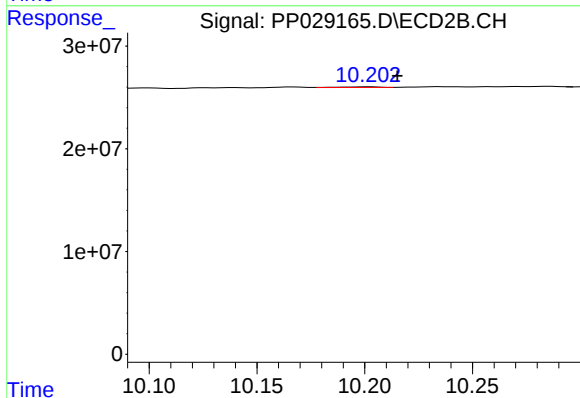


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.202 min
Delta R.T.: -0.013 min
Response: 766824
Conc: 15.13 ng/ml

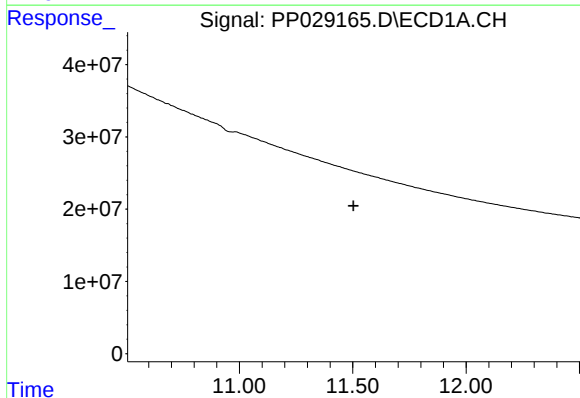


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

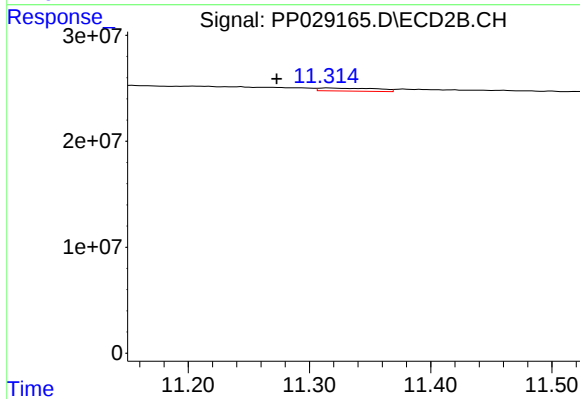

#3 4-Nitrophenol


R.T.: 11.316 min
Delta R.T.: 0.043 min
Response: 9368087
Conc: 391.19 ng/ml

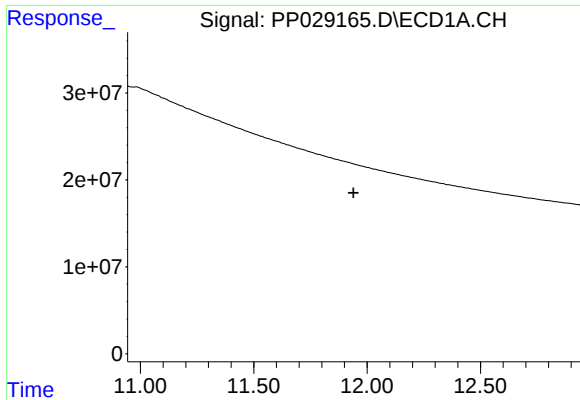

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

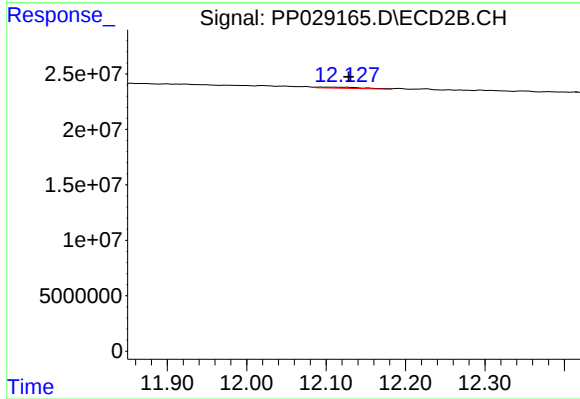


#4 2,4-DCAA

R.T.: 12.094 min
Delta R.T.: -0.034 min
Response: 4041183
Conc: 106.48 ng/ml

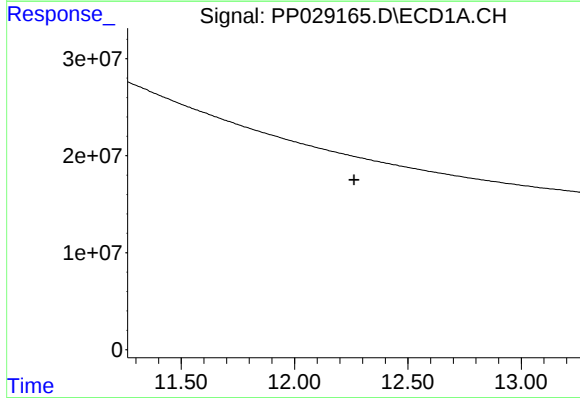


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 12.262 min
Response: 0
Conc: N.D.

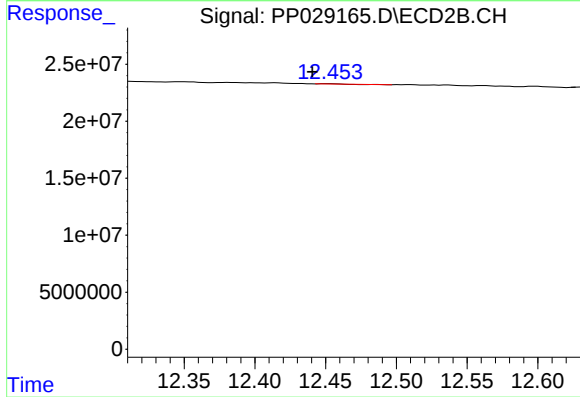

#5 DICAMBA


R.T.: 12.452 min
Delta R.T.: 0.011 min
Response: 216831
Conc: 1.69 ng/ml

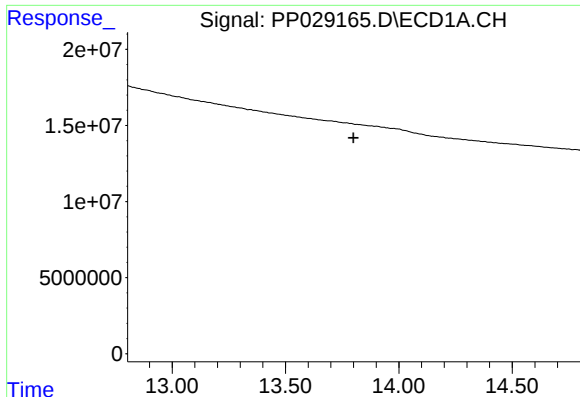

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

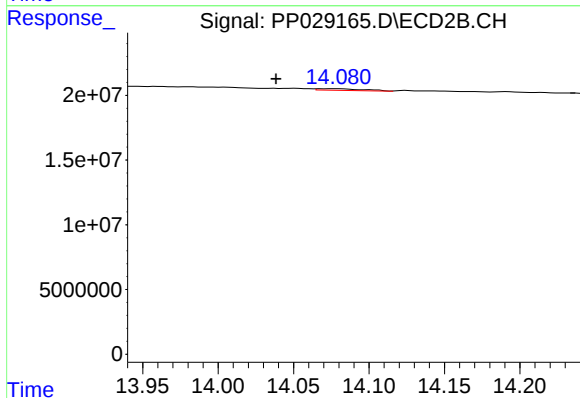


#9 2,4-D

R.T.: 14.078 min
Delta R.T.: 0.040 min
Response: 2727274
Conc: 60.15 ng/ml

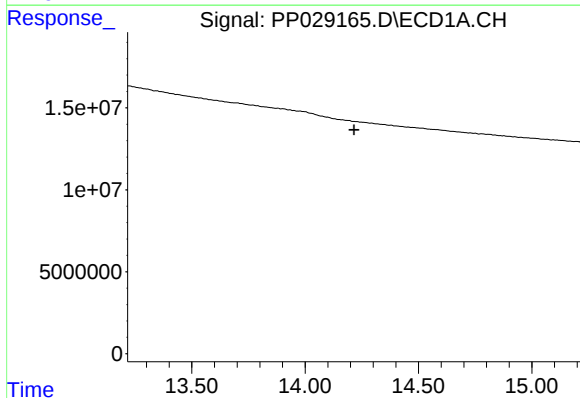


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 14.216 min
Response: 0
Conc: N.D.

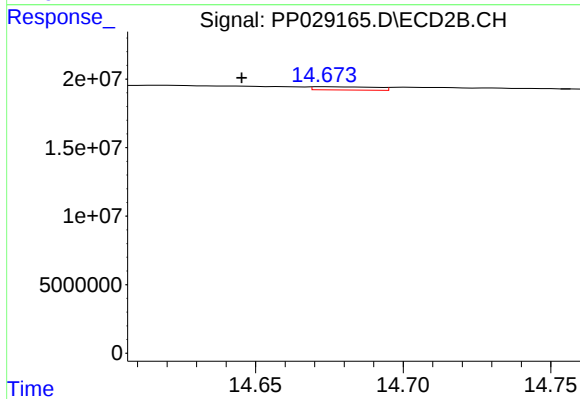

#10 Pentachlorophenol


R.T.: 14.674 min
Delta R.T.: 0.029 min
Response: 3457411
Conc: 6.72 ng/ml

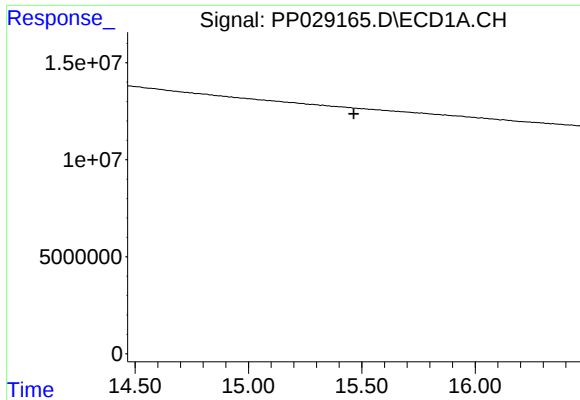

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

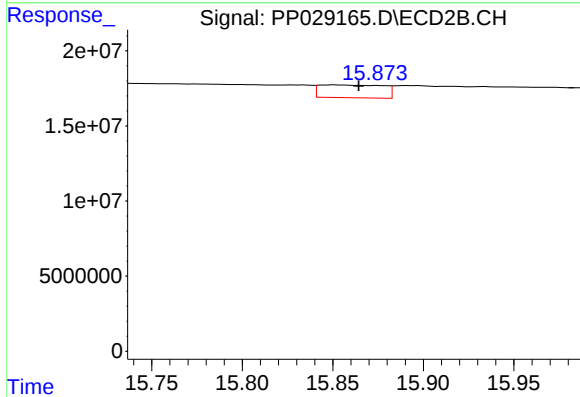


#12 2,4,5-T

R.T.: 15.852 min
Delta R.T.: -0.013 min
Response: 20795447
Conc: 125.60 ng/ml

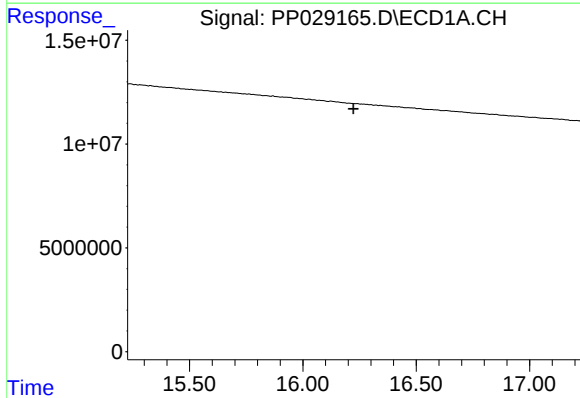


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.223 min
Response: 0
Conc: N.D.

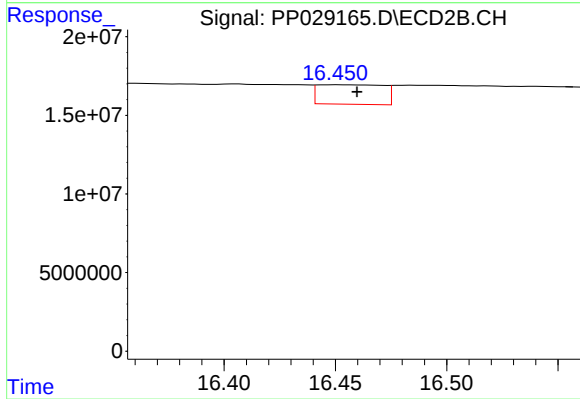

#13 2,4-DB


R.T.: 16.451 min
Delta R.T.: -0.009 min
Response: 25348477
Conc: 1125.27 ng/ml

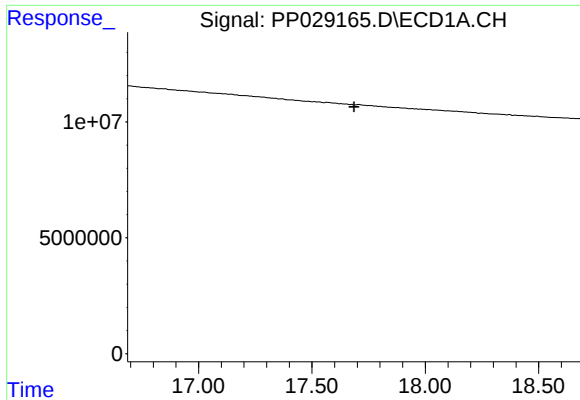

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

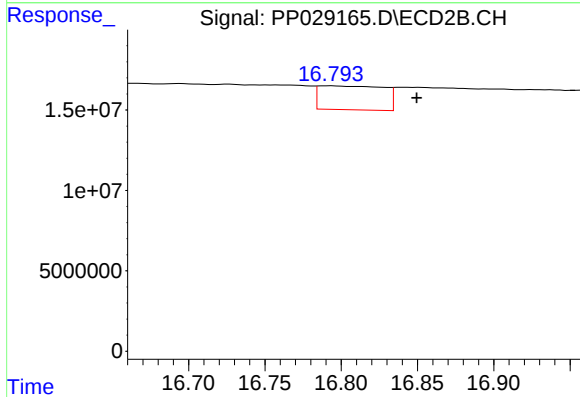


#14 DINOSEB

R.T.: 16.793 min
Delta R.T.: -0.056 min
Response: 43700524
Conc: 333.41 ng/ml

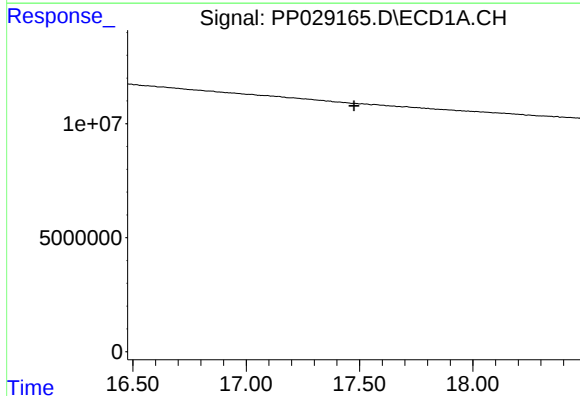

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.475 min
Response: 0
Conc: N.D.

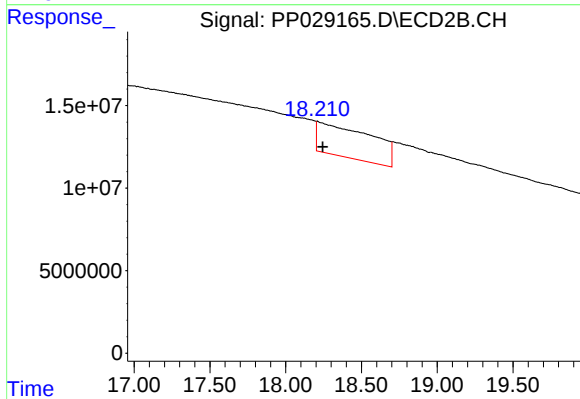

#15 Picloram

R.T.: 18.209 min
Delta R.T.: -0.036 min
Response: 498560678
Conc: 2215.60 ng/ml