

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022121\
 Data File : PP033492.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Feb 2021 8:30
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 2/23/2021 8:51:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 08:31:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 08:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.720	3.990	345717	220199	4.689	4.943
2)	SA Decachlor...	10.536	9.249	224895	162327	5.178m	5.257
Target Compounds							
26)	L6 AR-1254-1	6.921	6.101	93429	92117	47.348	50.444
27)	L6 AR-1254-2	7.148	6.260	165921	82432	54.070	53.549
28)	L6 AR-1254-3	7.528	6.679	154448	123980	50.461	49.795
29)	L6 AR-1254-4	7.822	6.918	120641	63260	54.047	49.492m
30)	L6 AR-1254-5	8.249	7.344	115943	110353	49.415	52.558

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022121\
Data File : PP033492.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Feb 2021 8:30
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
2/23/2021 8:51:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 08:31:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 08:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

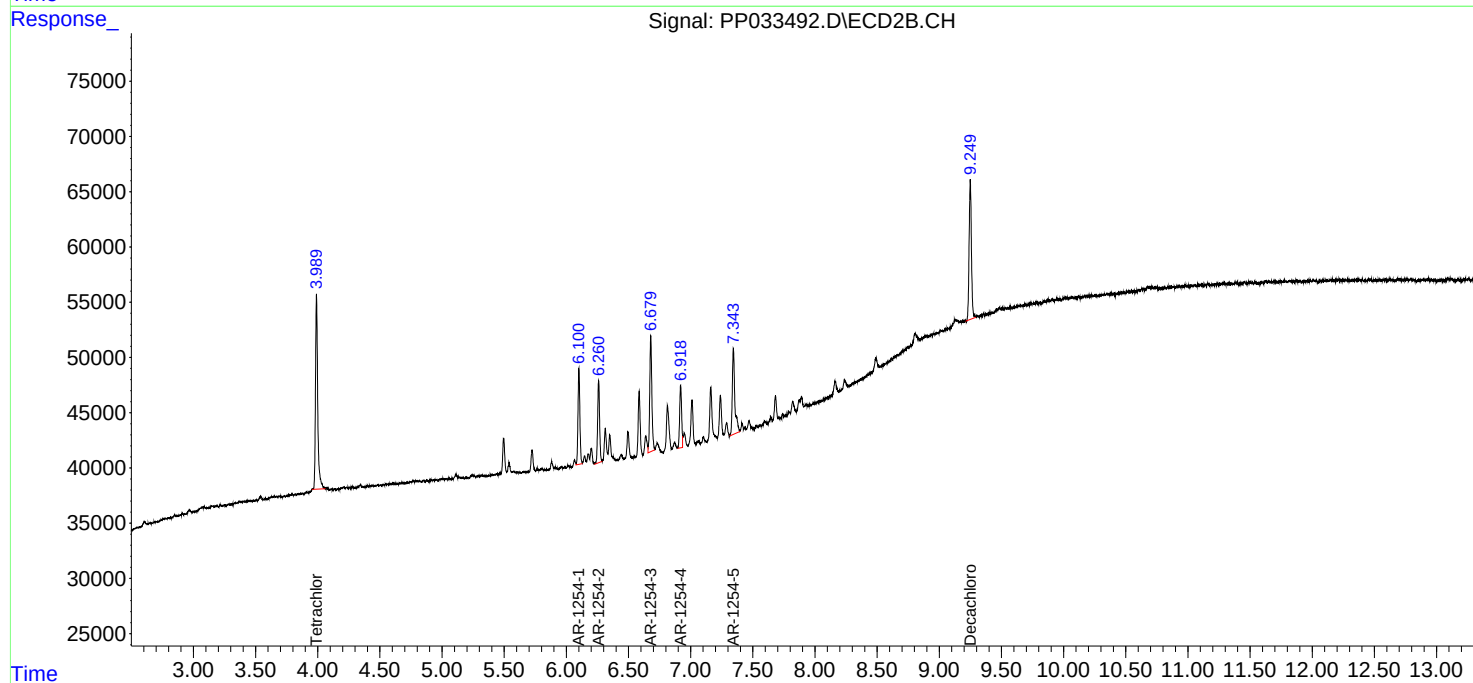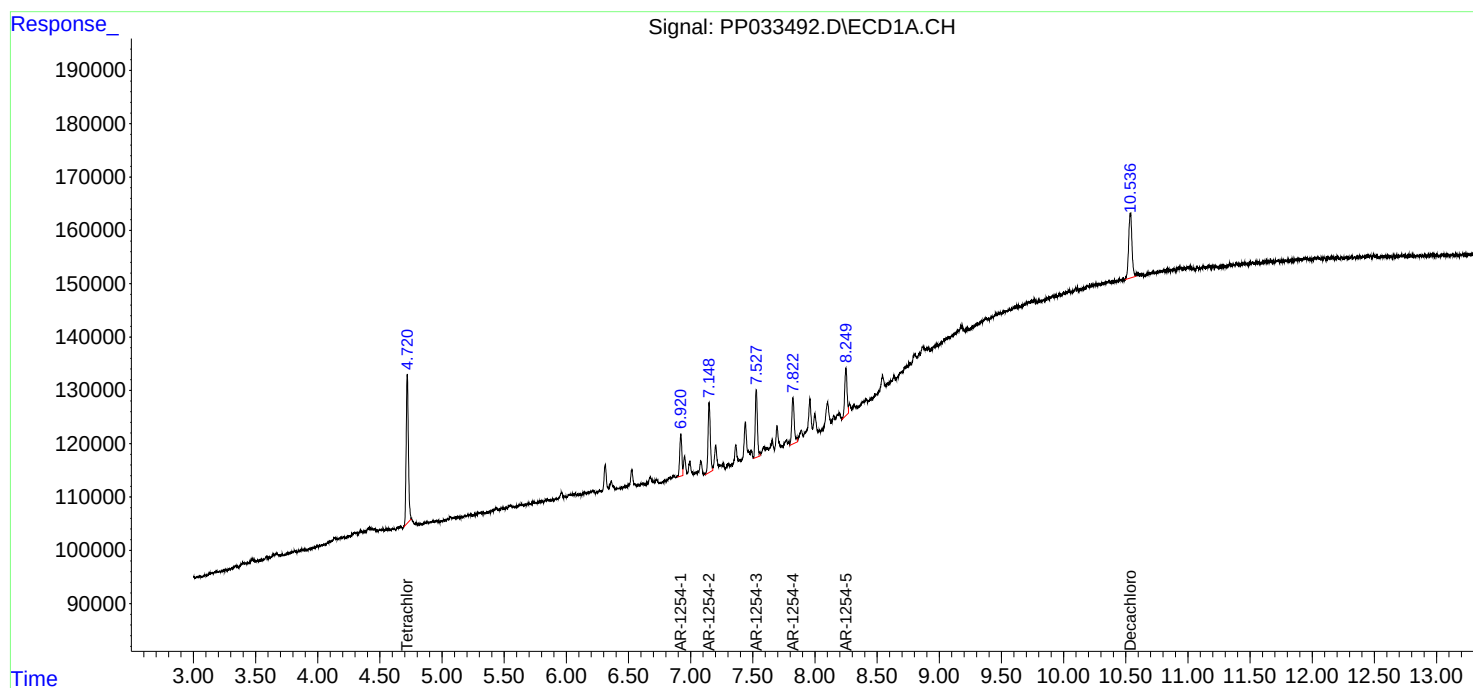

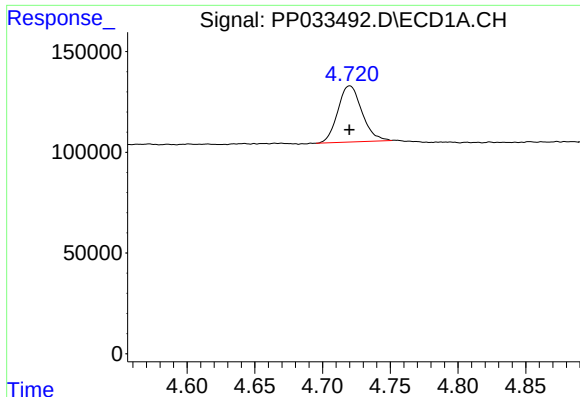


#1 Tetrachloro-m-xylene

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 345717
Conc: 4.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
2/23/2021 8:51:35 AM

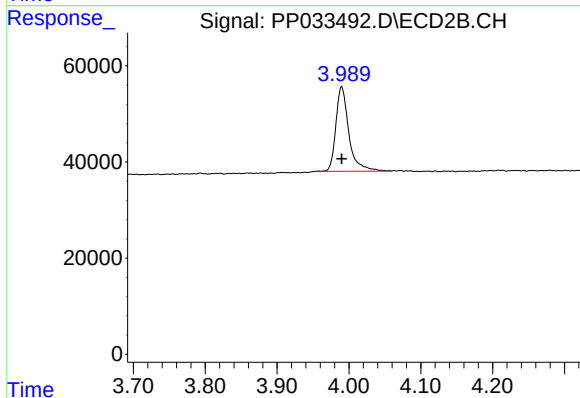


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 220199
Conc: 4.94 ng/ml

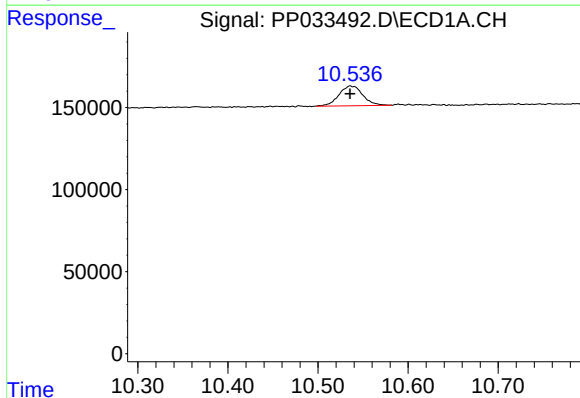


#2 Decachlorobiphenyl

R.T.: 10.536 min
Delta R.T.: 0.000 min
Response: 224895
Conc: 5.18 ng/ml m

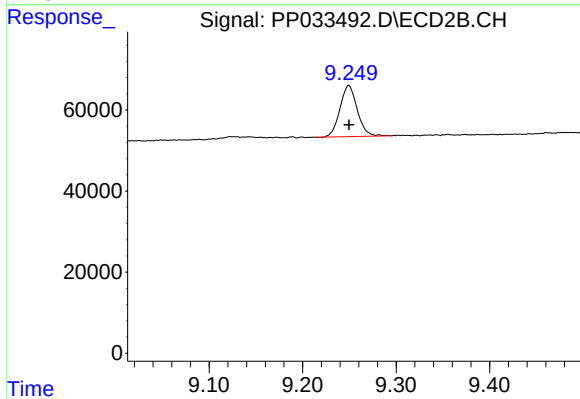

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: 0.000 min
Response: 162327
Conc: 5.26 ng/ml

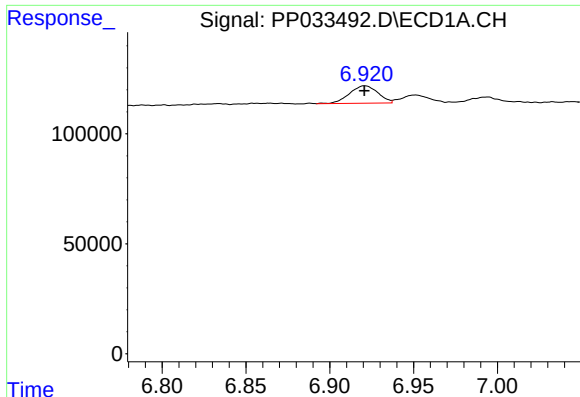


#26 AR-1254-1

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 93429
Conc: 47.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
2/23/2021 8:51:35 AM

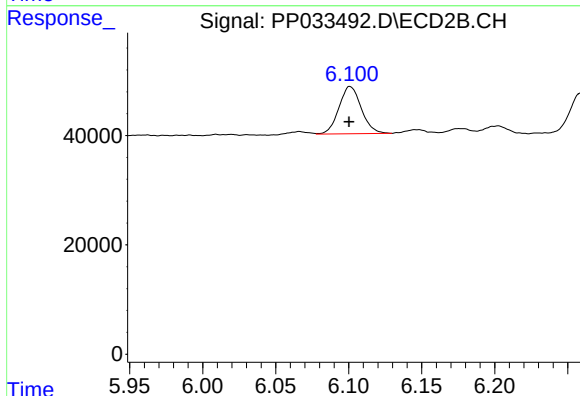


#26 AR-1254-1

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 92117
Conc: 50.44 ng/ml

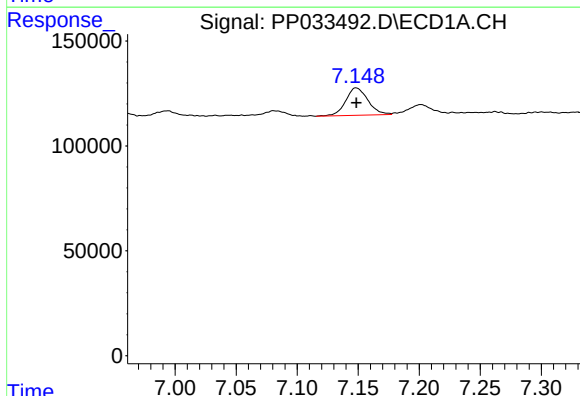


#27 AR-1254-2

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 165921
Conc: 54.07 ng/ml

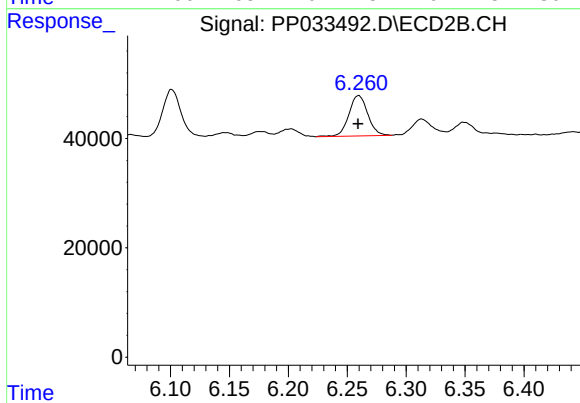

#27 AR-1254-2

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 82432
Conc: 53.55 ng/ml

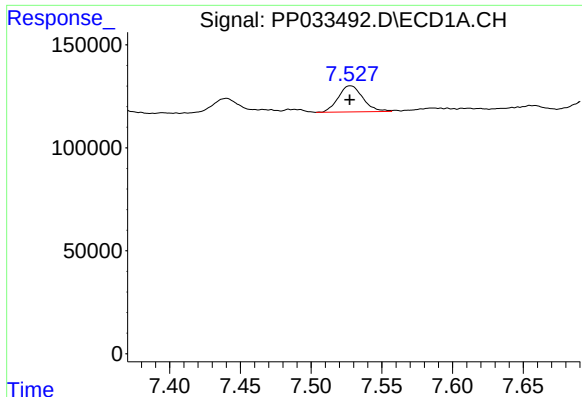


#28 AR-1254-3

R.T.: 7.528 min
Delta R.T.: 0.000 min
Response: 154448
Conc: 50.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
2/23/2021 8:51:35 AM

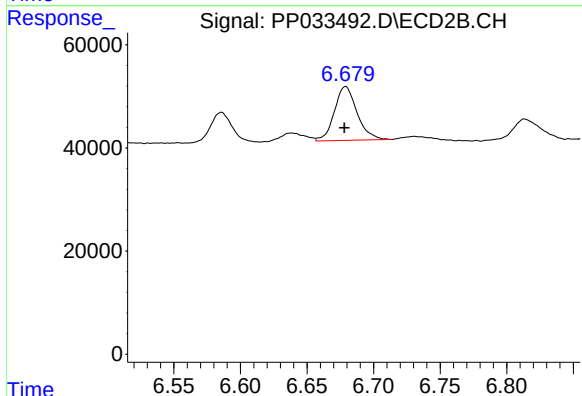


#28 AR-1254-3

R.T.: 6.679 min
Delta R.T.: 0.001 min
Response: 123980
Conc: 49.80 ng/ml

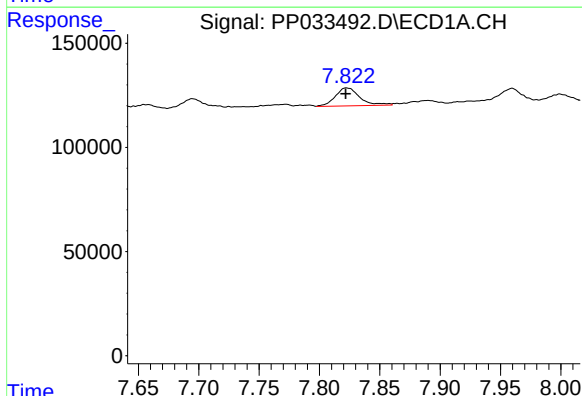


#29 AR-1254-4

R.T.: 7.822 min
Delta R.T.: 0.000 min
Response: 120641
Conc: 54.05 ng/ml

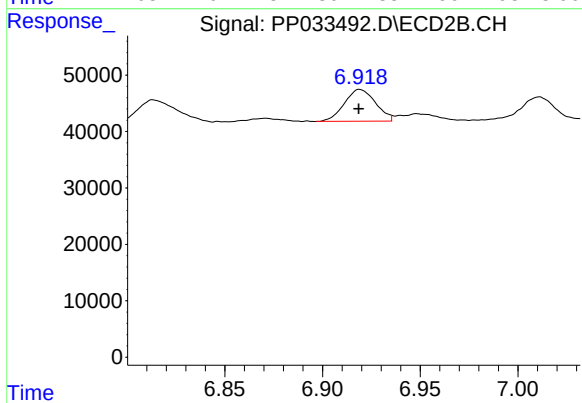

#29 AR-1254-4

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 63260
Conc: 49.49 ng/ml m

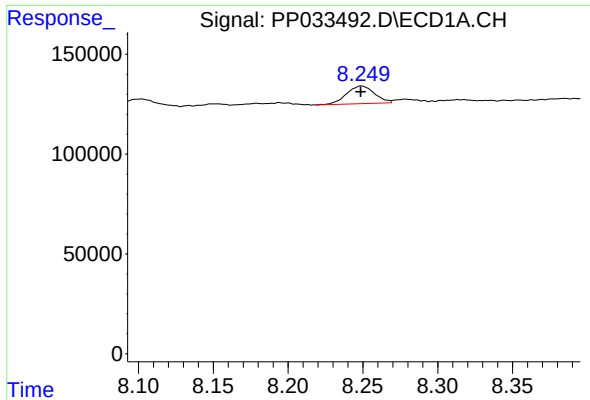


#30 AR-1254-5

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 115943
Conc: 49.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
2/23/2021 8:51:35 AM

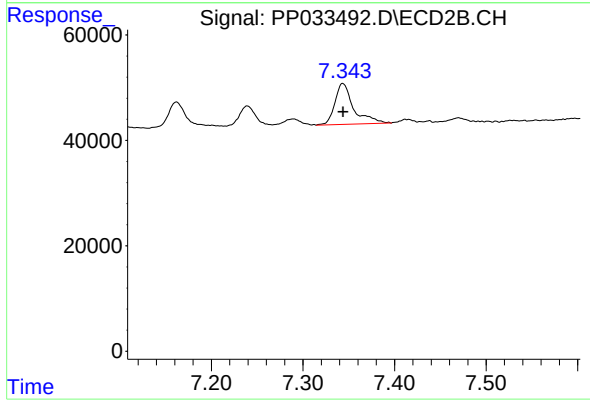

#30 AR-1254-5

R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 110353
Conc: 52.56 ng/ml