

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
 Data File : PP043873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 14:40
 Operator : YP\AJ
 Sample : N1601-24 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-21A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:13:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.914	3.171	1968300	2149339	0.890m	1.144m#
2) SA Decachlor...	10.051f	8.546	1695506	1689757	1.427m	1.042m#
Target Compounds						
26) L6 AR-1254-1	6.096	5.172	794131	1089646	10.510m	12.477
27) L6 AR-1254-2	6.334	5.332	1371545	1400897	12.228m	18.366 #
28) L6 AR-1254-3	6.734	5.764	1697942	1854987	14.674	15.136
29) L6 AR-1254-4	7.046	6.014	853390	1166222	10.690m	14.776 #
30) L6 AR-1254-5	7.505	6.465	1006049	1463718	11.731m	12.657



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
Data File : PP043873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 14:40
Operator : YP\AJ
Sample : N1601-24 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-21A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:13:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

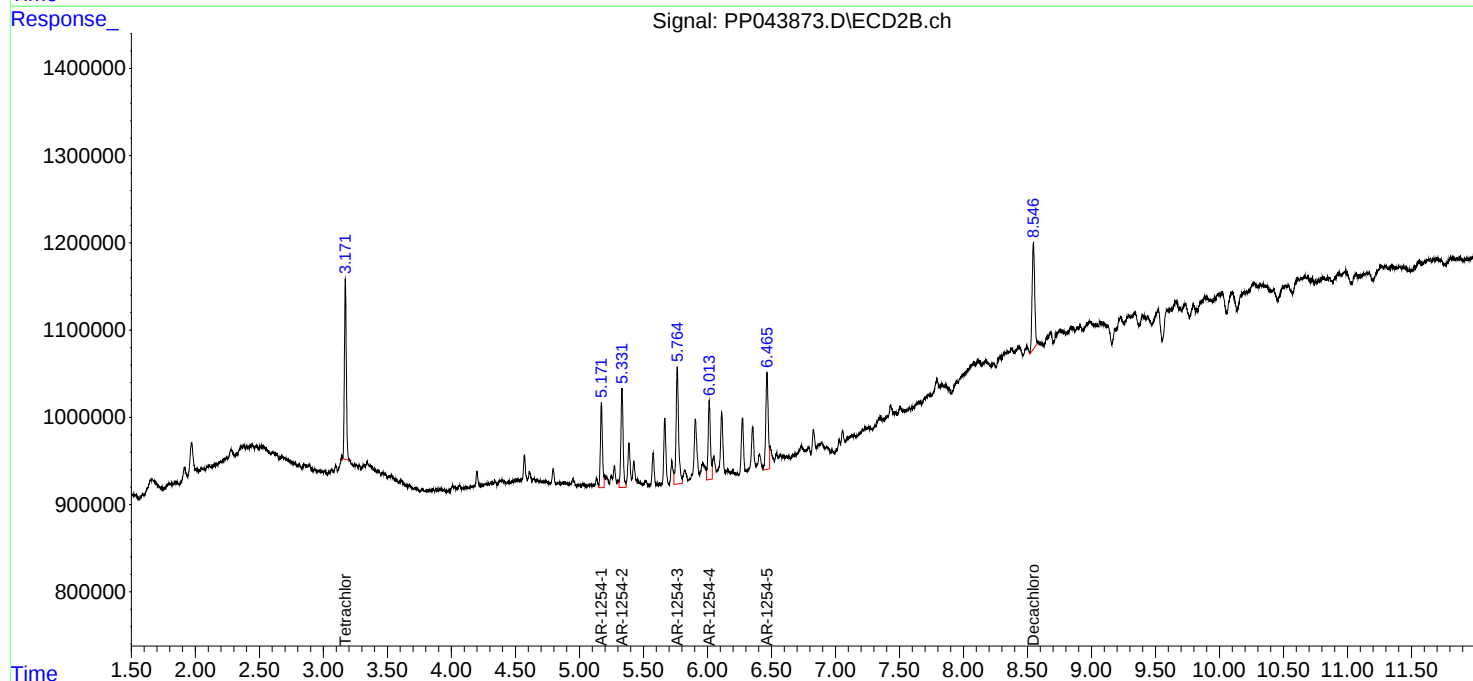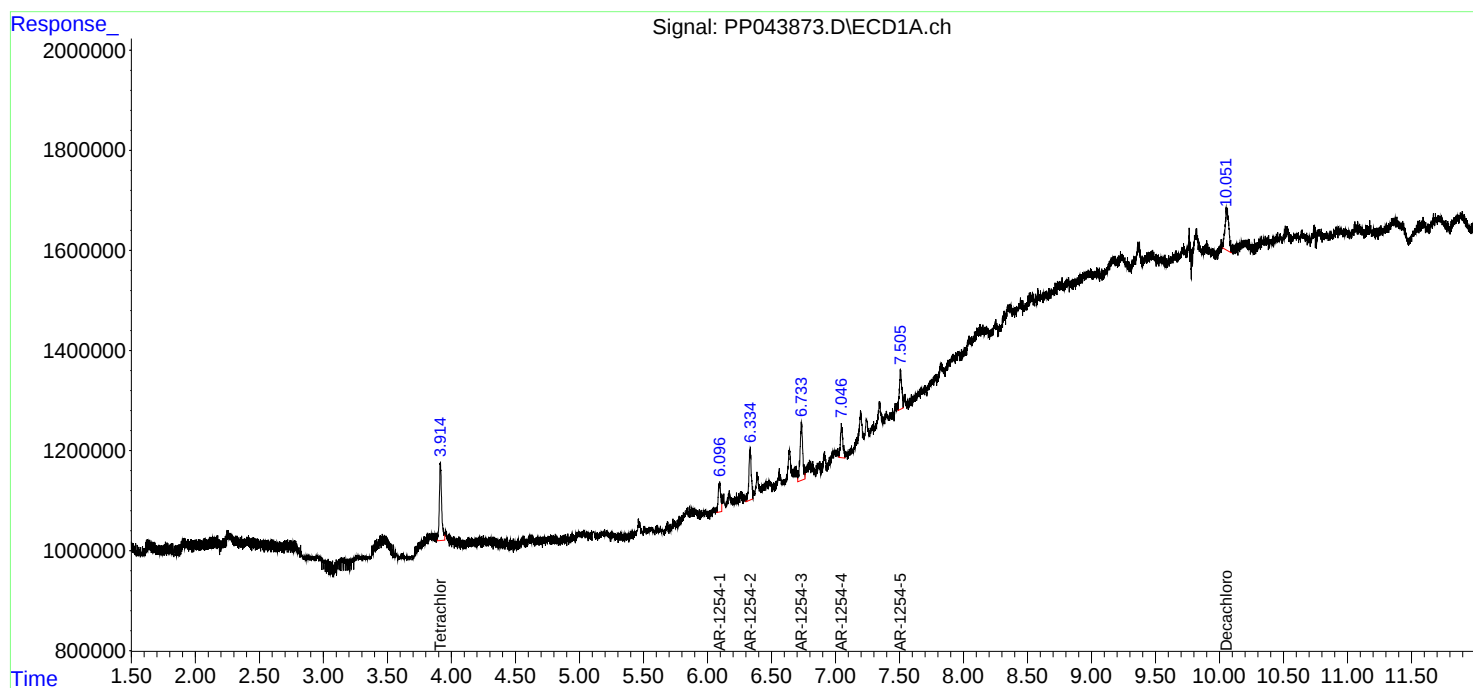


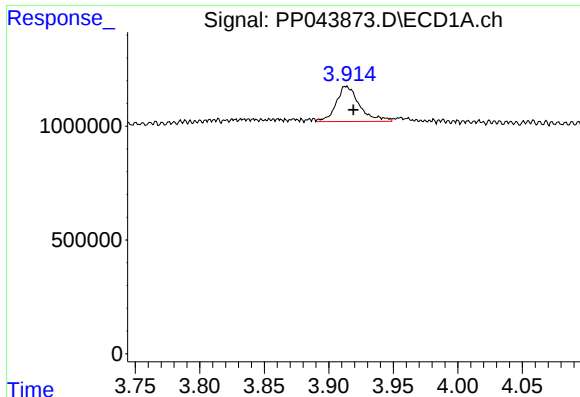

#1 Tetrachloro-m-xylene


R.T.: 3.914 min
Delta R.T.: -0.005 min
Response: 1968300
Conc: 0.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-21A

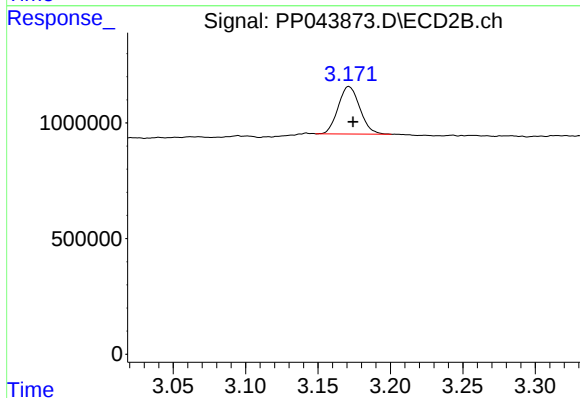


#1 Tetrachloro-m-xylene

R.T.: 3.171 min
Delta R.T.: -0.003 min
Response: 2149339
Conc: 1.14 ng/ml m

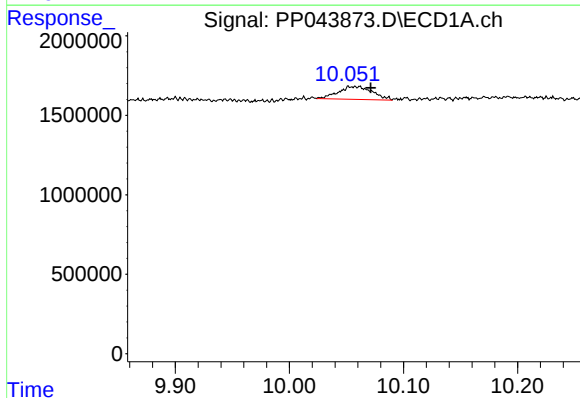


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.020 min
Response: 1695506
Conc: 1.43 ng/ml m

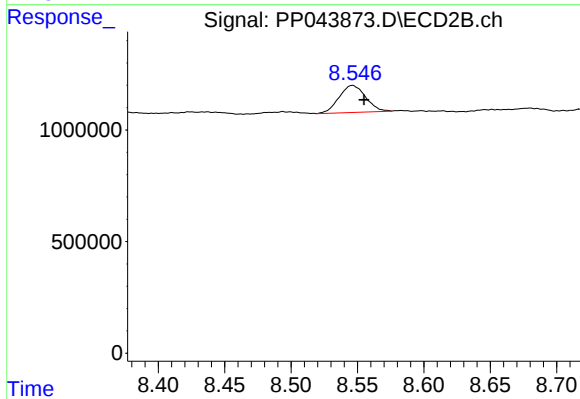

#2 Decachlorobiphenyl


R.T.: 8.546 min
Delta R.T.: -0.009 min
Response: 1689757
Conc: 1.04 ng/ml m

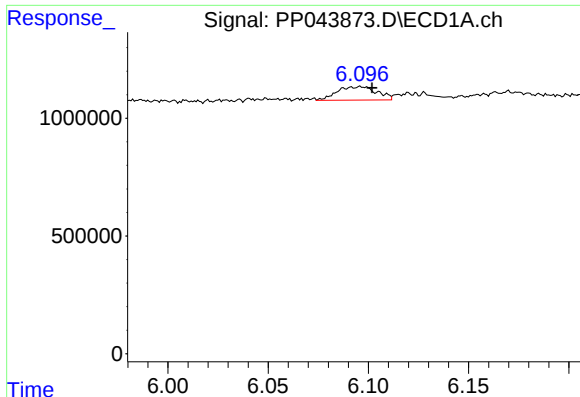

#26 AR-1254-1


R.T.: 6.096 min
Delta R.T.: -0.006 min
Response: 794131
Conc: 10.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-21A

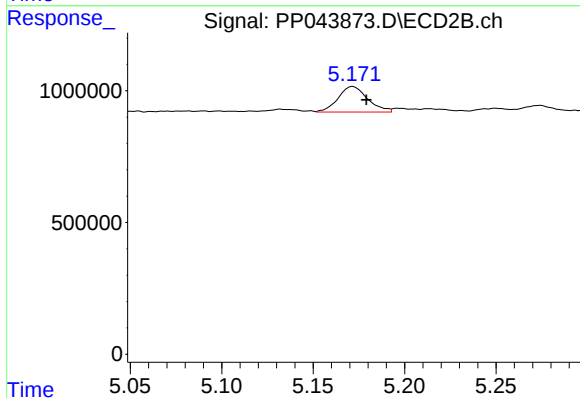


#26 AR-1254-1

R.T.: 5.172 min
Delta R.T.: -0.008 min
Response: 1089646
Conc: 12.48 ng/ml

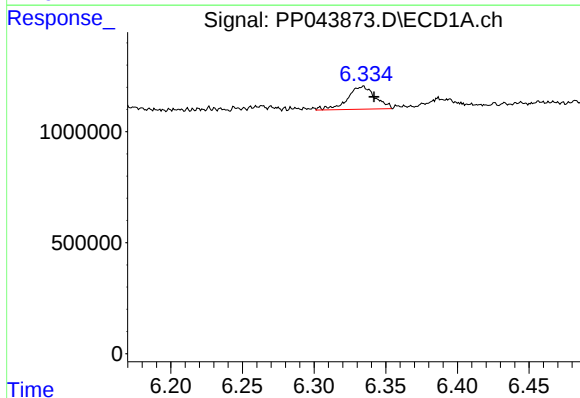


#27 AR-1254-2

R.T.: 6.334 min
Delta R.T.: -0.008 min
Response: 1371545
Conc: 12.23 ng/ml m

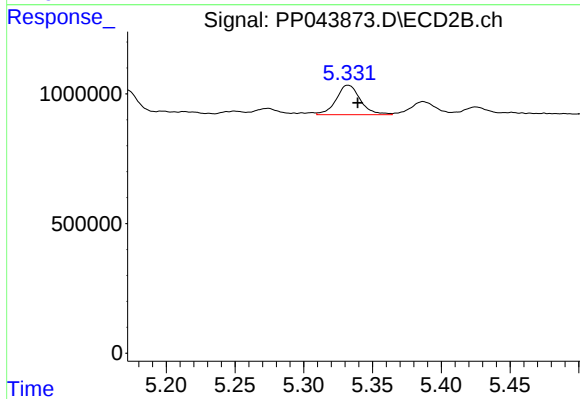

#27 AR-1254-2


R.T.: 5.332 min
Delta R.T.: -0.007 min
Response: 1400897
Conc: 18.37 ng/ml

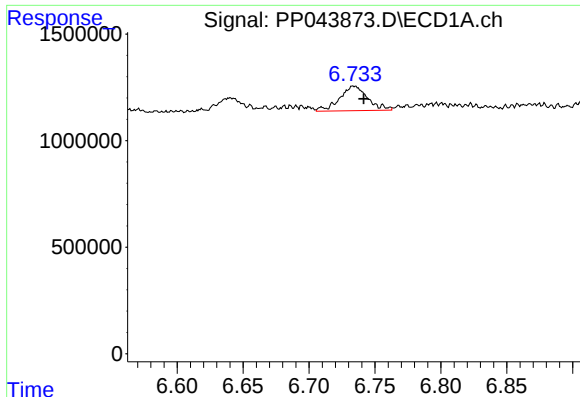

#28 AR-1254-3


R.T.: 6.734 min
Delta R.T.: -0.007 min
Response: 1697942
Conc: 14.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-21A

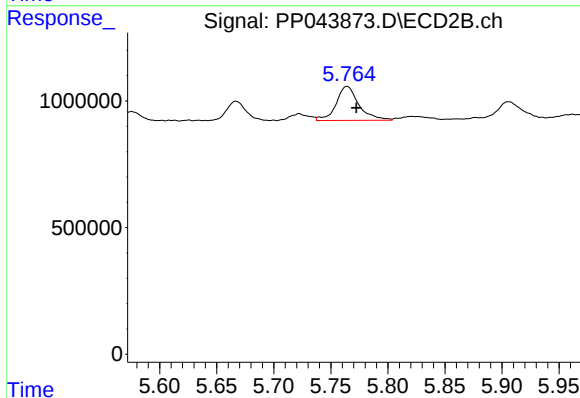


#28 AR-1254-3

R.T.: 5.764 min
Delta R.T.: -0.008 min
Response: 1854987
Conc: 15.14 ng/ml

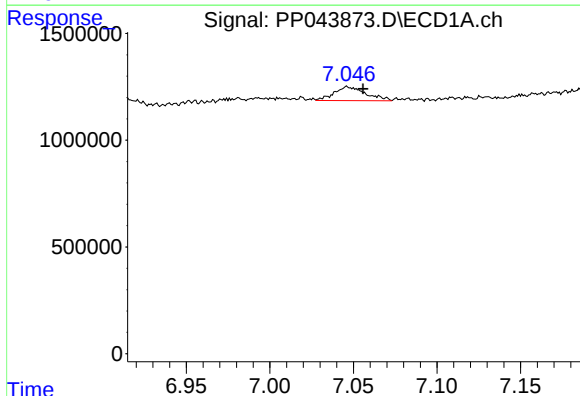


#29 AR-1254-4

R.T.: 7.046 min
Delta R.T.: -0.010 min
Response: 853390
Conc: 10.69 ng/ml m

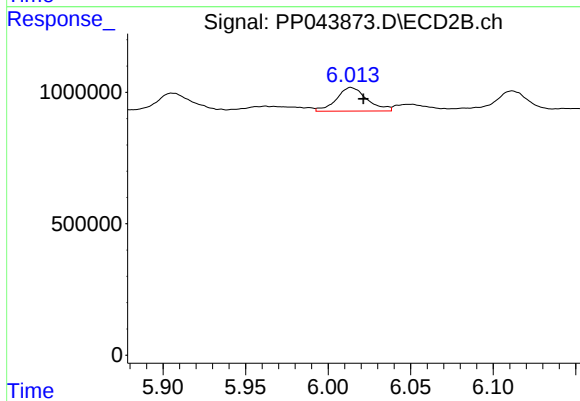

#29 AR-1254-4


R.T.: 6.014 min
Delta R.T.: -0.008 min
Response: 1166222
Conc: 14.78 ng/ml

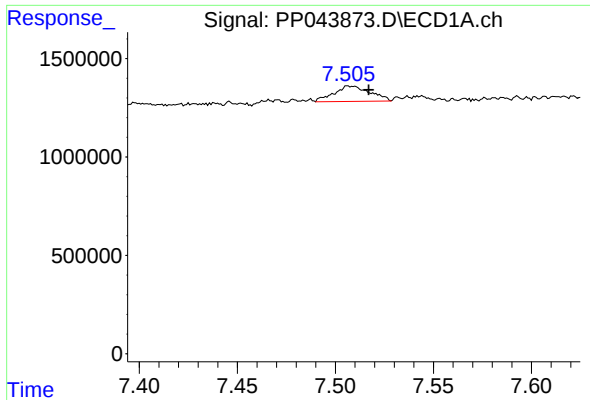

#30 AR-1254-5

R.T.: 7.505 min
Delta R.T.: -0.012 min
Response: 1006049
Conc: 11.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-21A

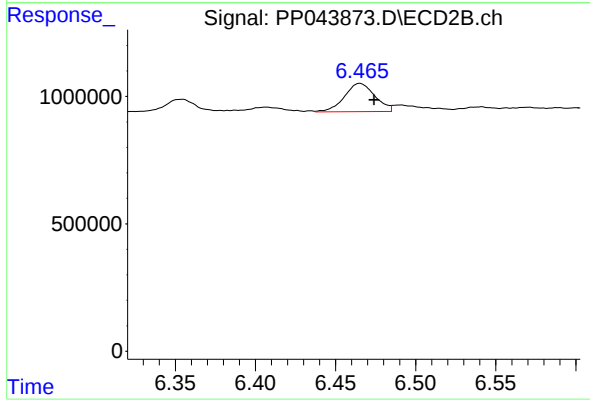

#30 AR-1254-5

R.T.: 6.465 min
Delta R.T.: -0.009 min
Response: 1463718
Conc: 12.66 ng/ml