

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
 Data File : PP043874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 14:55
 Operator : YP\AJ
 Sample : N1601-25 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-22A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:14:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.915	3.172	2728110	3432756	1.234	1.828 #
2)	SA Decachlor...	10.057	8.545	2037928	2575314	1.716	1.587
Target Compounds							
26)	L6 AR-1254-1	6.096	5.172	487123	559187	6.447m	6.403
27)	L6 AR-1254-2	6.336	5.333	783723	594395	6.987m	7.793
28)	L6 AR-1254-3	6.735	5.764	906065	680720	7.830	5.554 #
29)	L6 AR-1254-4	7.050	6.015	465870	551718	5.836m	6.990
30)	L6 AR-1254-5	7.503	6.465	574889	458872	6.703m	3.968 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
Data File : PP043874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 14:55
Operator : YP\AJ
Sample : N1601-25 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-22A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:14:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

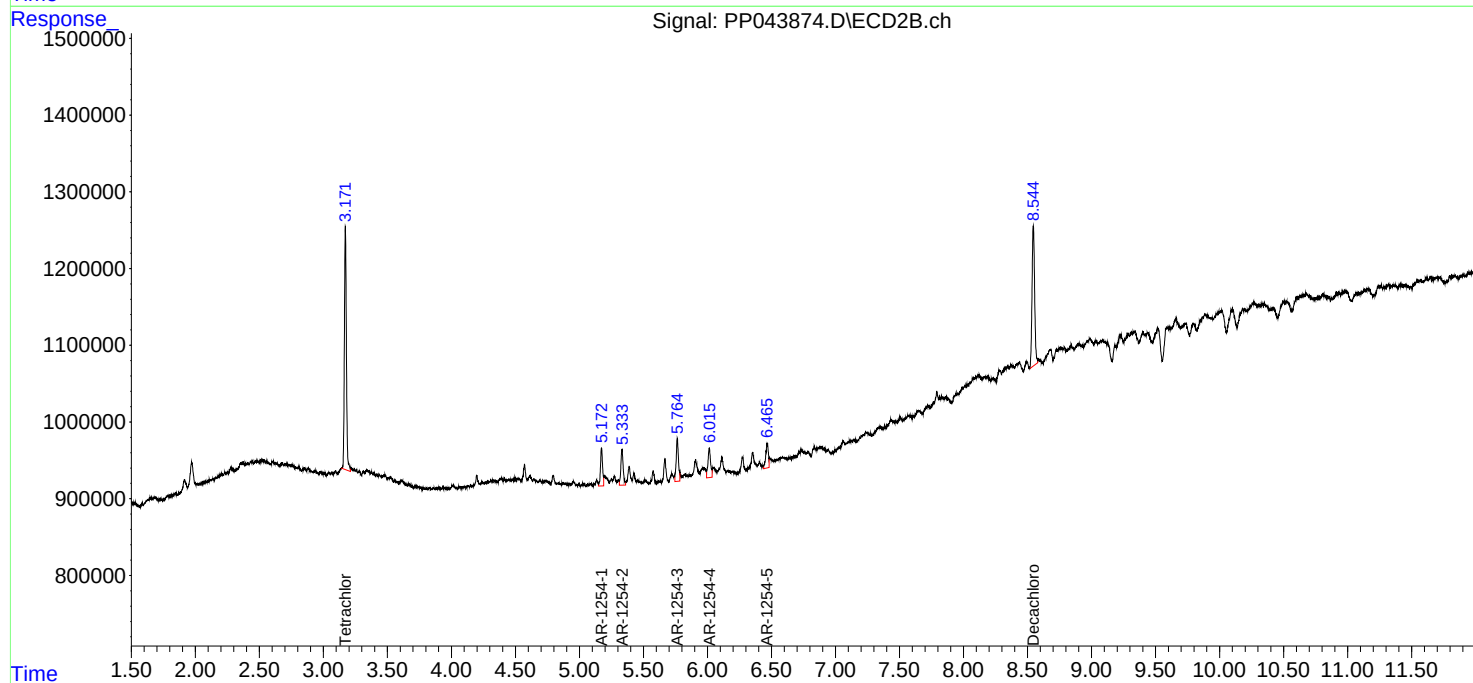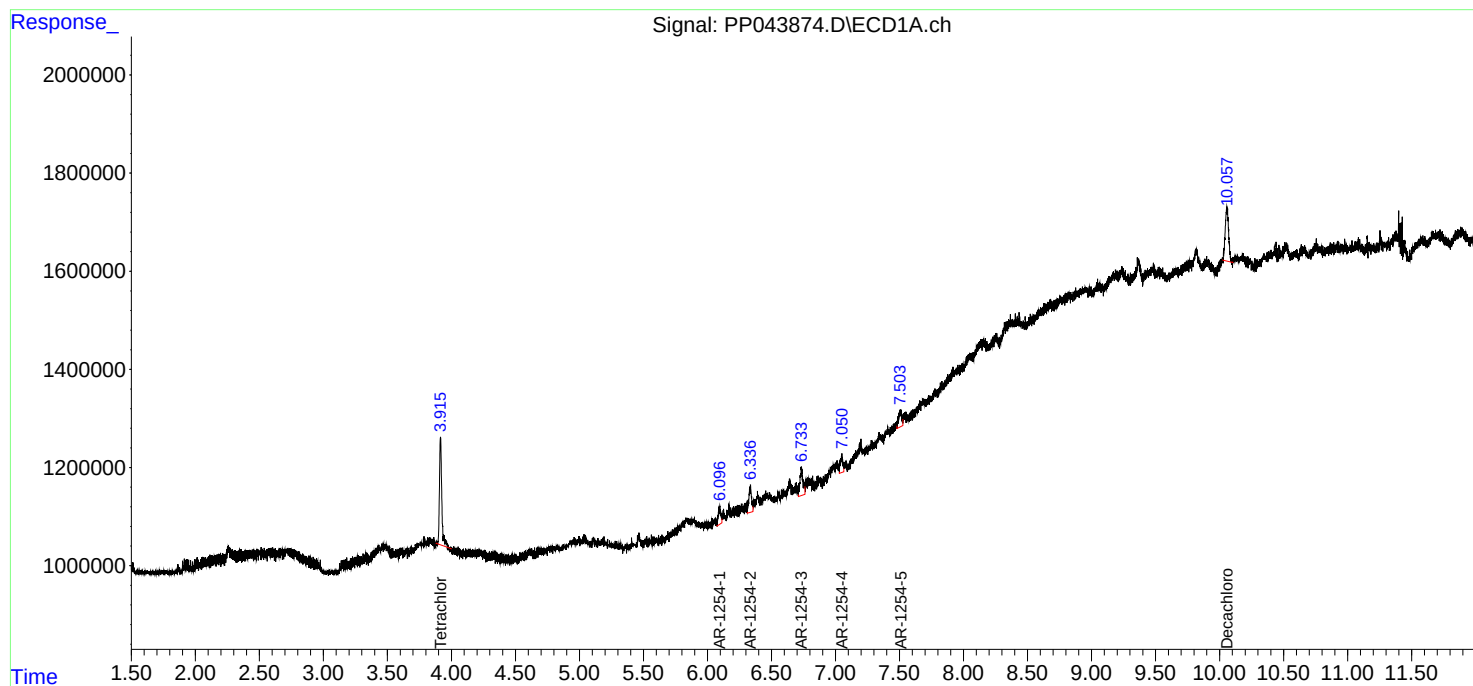


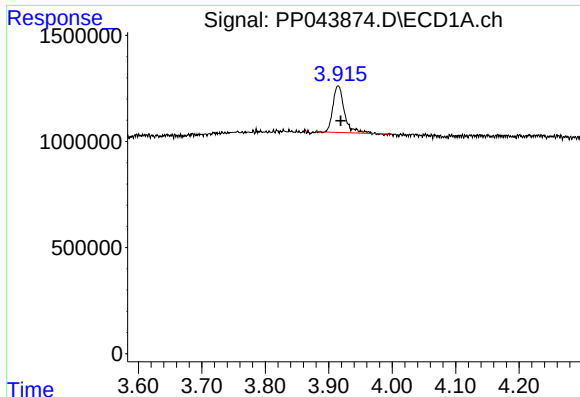

#1 Tetrachloro-m-xylene


R.T.: 3.915 min
Delta R.T.: -0.004 min
Response: 2728110
Conc: 1.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-22A

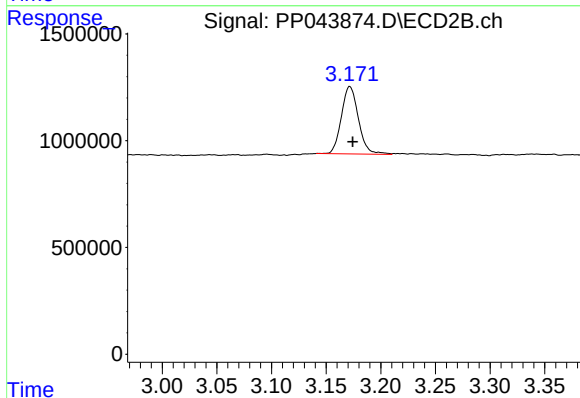


#1 Tetrachloro-m-xylene

R.T.: 3.172 min
Delta R.T.: -0.003 min
Response: 3432756
Conc: 1.83 ng/ml

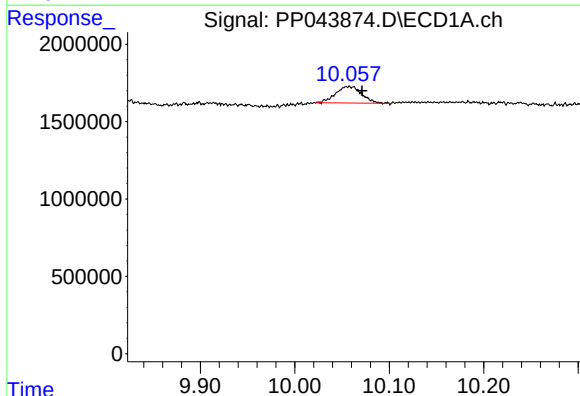


#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: -0.014 min
Response: 2037928
Conc: 1.72 ng/ml

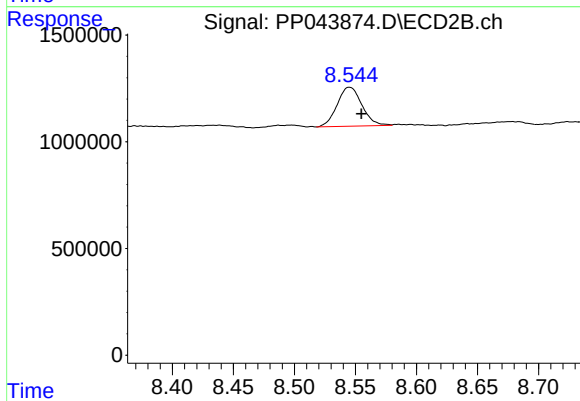

#2 Decachlorobiphenyl


R.T.: 8.545 min
Delta R.T.: -0.010 min
Response: 2575314
Conc: 1.59 ng/ml

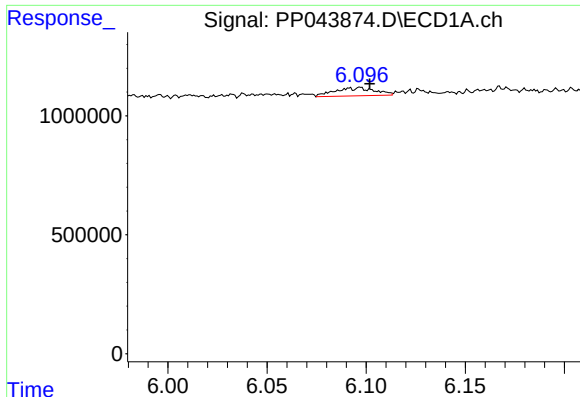

#26 AR-1254-1


R.T.: 6.096 min
Delta R.T.: -0.005 min
Response: 487123
Conc: 6.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-22A

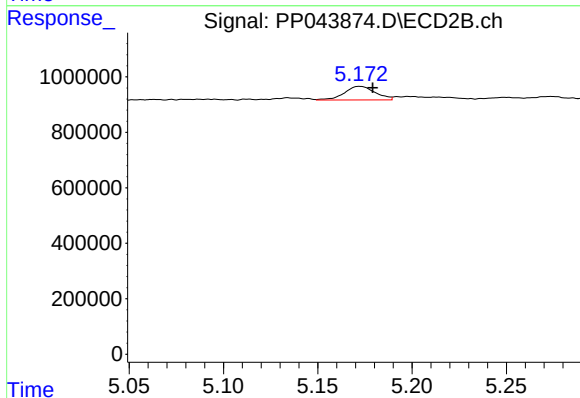


#26 AR-1254-1

R.T.: 5.172 min
Delta R.T.: -0.007 min
Response: 559187
Conc: 6.40 ng/ml

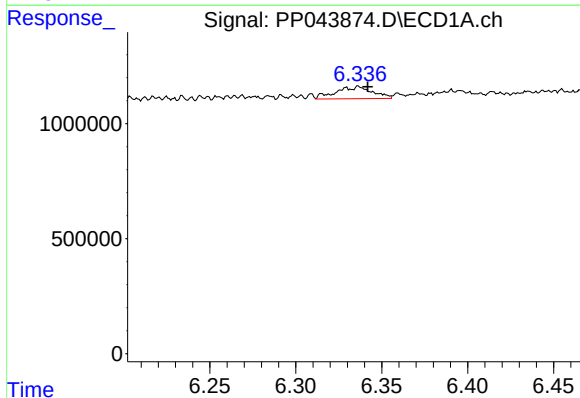


#27 AR-1254-2

R.T.: 6.336 min
Delta R.T.: -0.006 min
Response: 783723
Conc: 6.99 ng/ml m

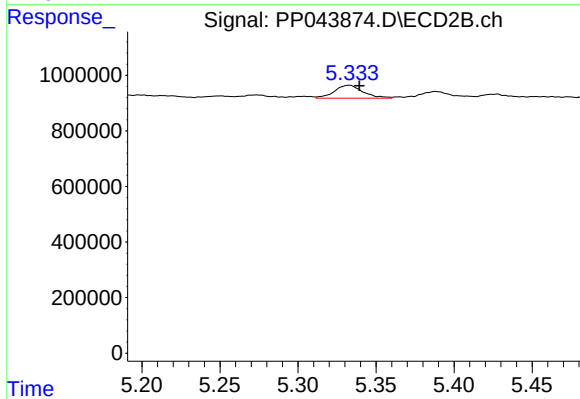

#27 AR-1254-2


R.T.: 5.333 min
Delta R.T.: -0.006 min
Response: 594395
Conc: 7.79 ng/ml

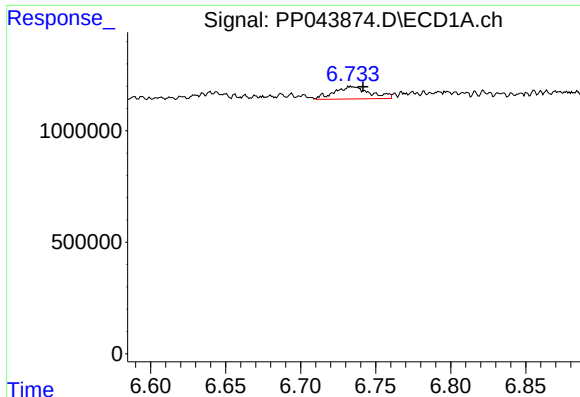

#28 AR-1254-3


R.T.: 6.735 min
Delta R.T.: -0.007 min
Response: 906065
Conc: 7.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-22A

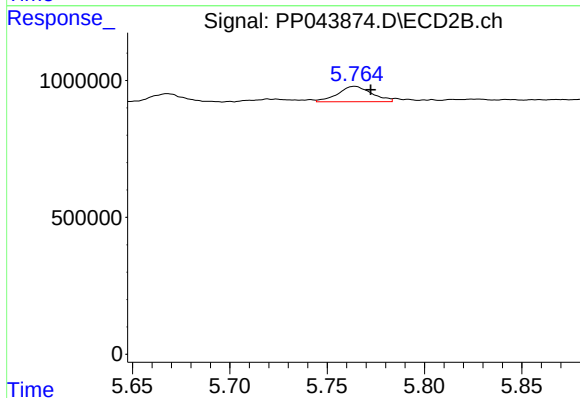


#28 AR-1254-3

R.T.: 5.764 min
Delta R.T.: -0.008 min
Response: 680720
Conc: 5.55 ng/ml

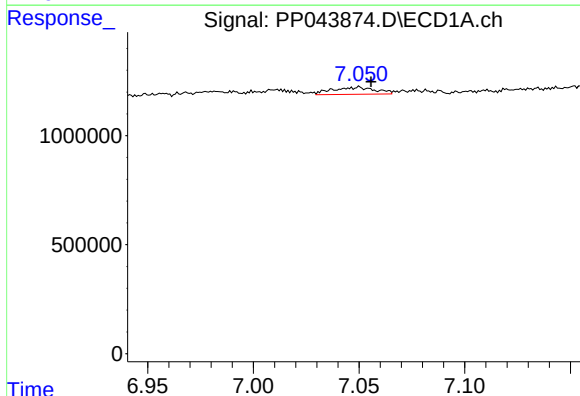


#29 AR-1254-4

R.T.: 7.050 min
Delta R.T.: -0.006 min
Response: 465870
Conc: 5.84 ng/ml m

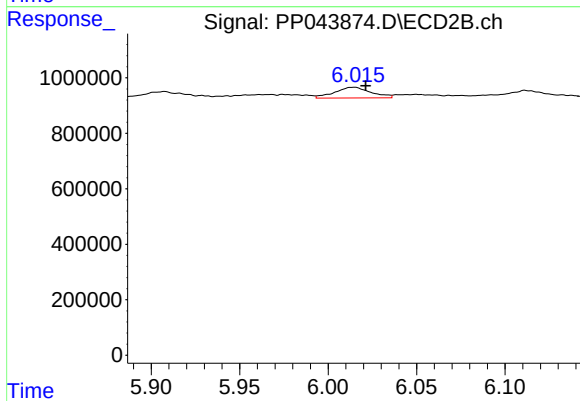

#29 AR-1254-4


R.T.: 6.015 min
Delta R.T.: -0.006 min
Response: 551718
Conc: 6.99 ng/ml

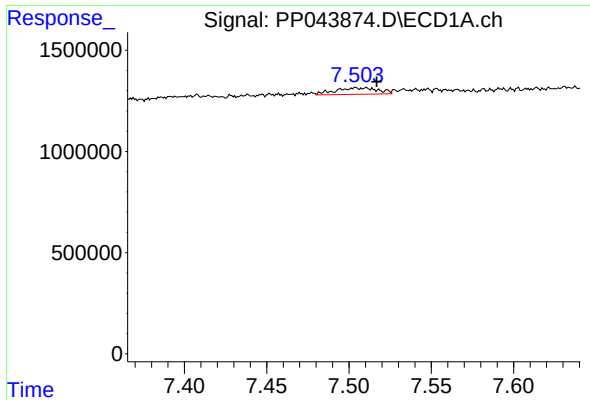

#30 AR-1254-5

R.T.: 7.503 min
Delta R.T.: -0.014 min
Response: 574889
Conc: 6.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-22A

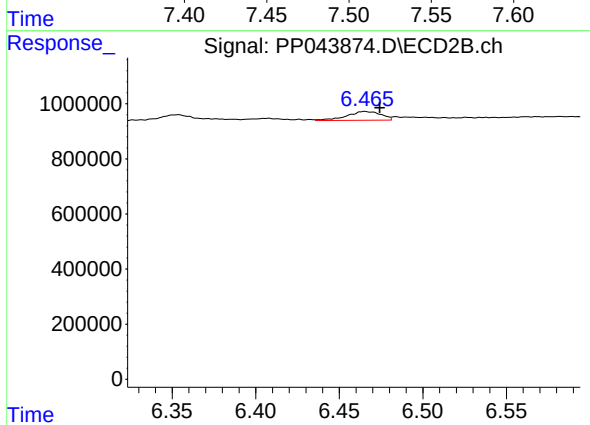

#30 AR-1254-5

R.T.: 6.465 min
Delta R.T.: -0.009 min
Response: 458872
Conc: 3.97 ng/ml