

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
 Data File : PP043894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 20:45
 Operator : YP\AJ
 Sample : N1601-12 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-14B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 00:22:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.915	3.171	3192909	3439311	1.444m	1.831m#
2) SA Decachlor...	10.057	8.545	2330619	2584410	1.962m	1.593m
Target Compounds						
26) L6 AR-1254-1	6.093	5.171	1014528	1201976	13.427m	13.763
27) L6 AR-1254-2	6.332	5.332	1573437	1123636	14.027	14.731
28) L6 AR-1254-3	6.735	5.764	1774948	1660343	15.339m	13.547
29) L6 AR-1254-4	7.046	6.013	1502998	1460496	18.827	18.505
30) L6 AR-1254-5	7.511	6.465	854193	1192903	9.960m	10.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
Data File : PP043894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 20:45
Operator : YP\AJ
Sample : N1601-12 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-14B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 00:22:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

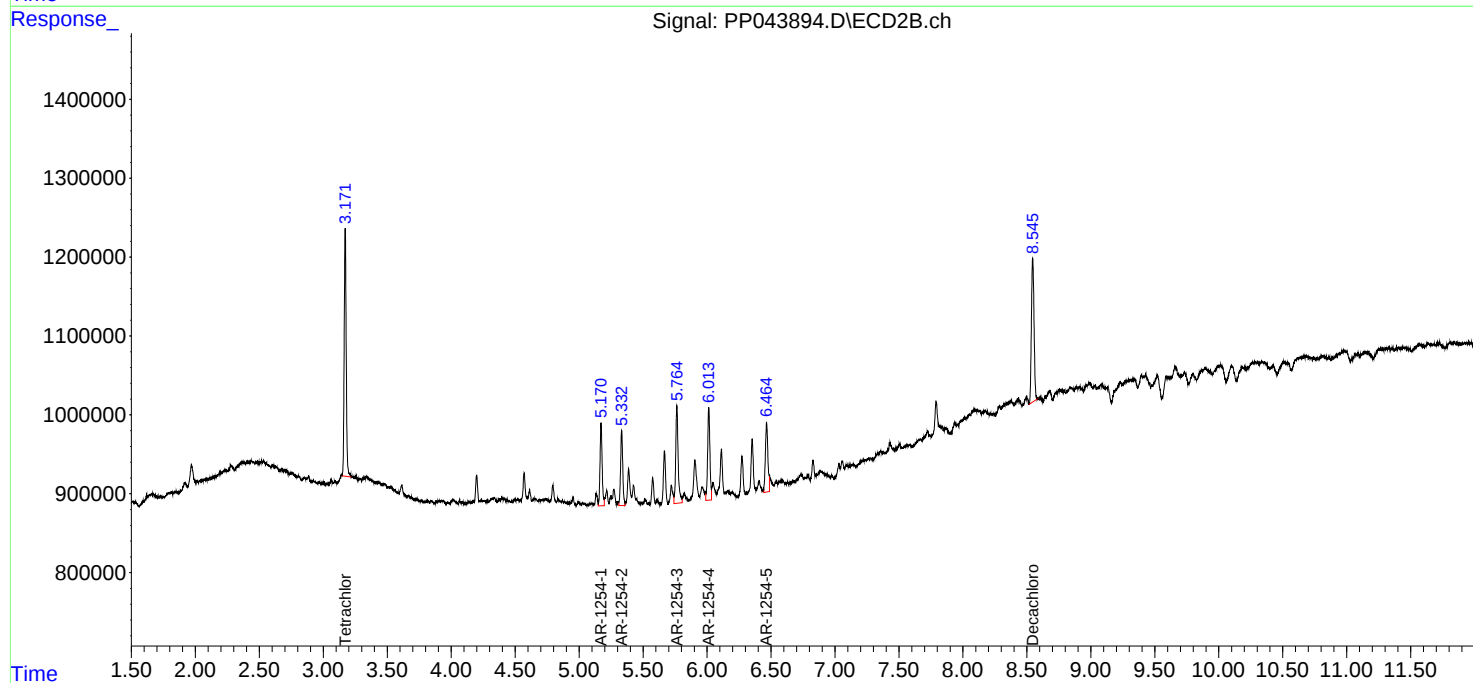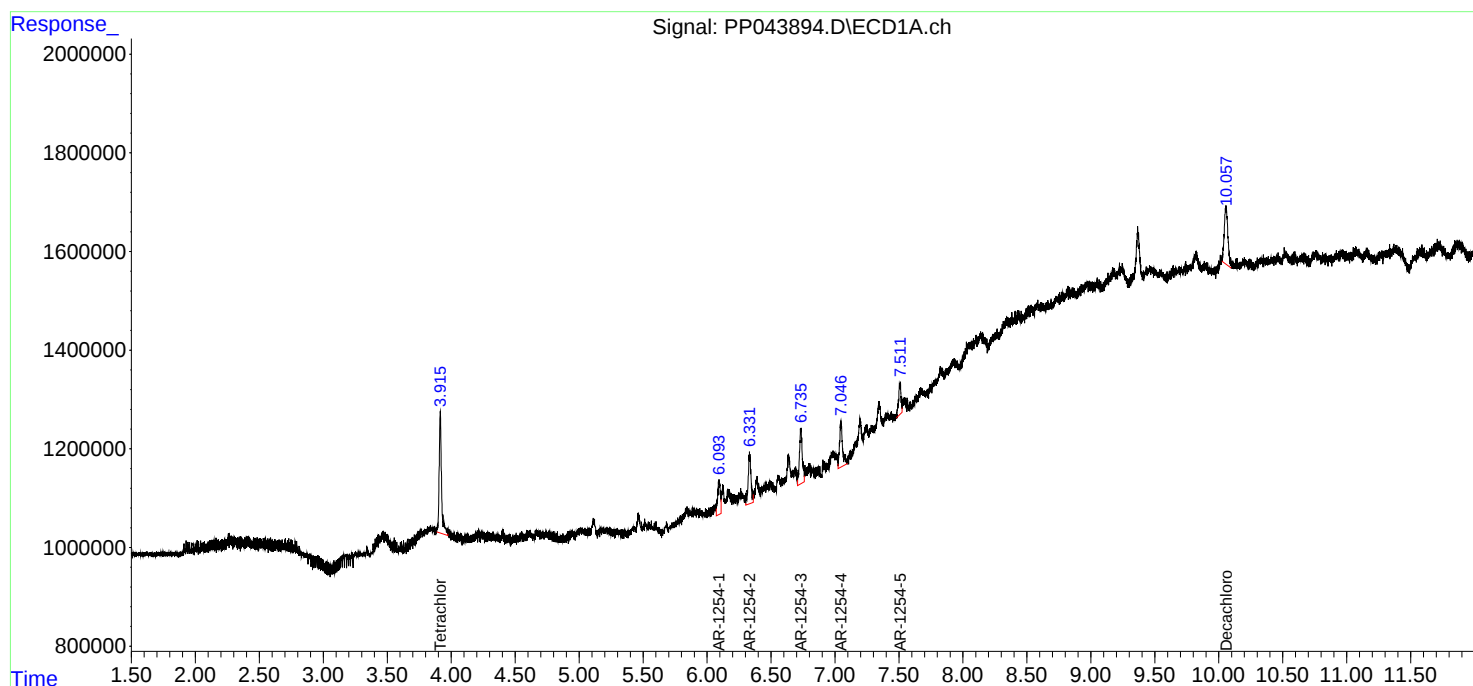


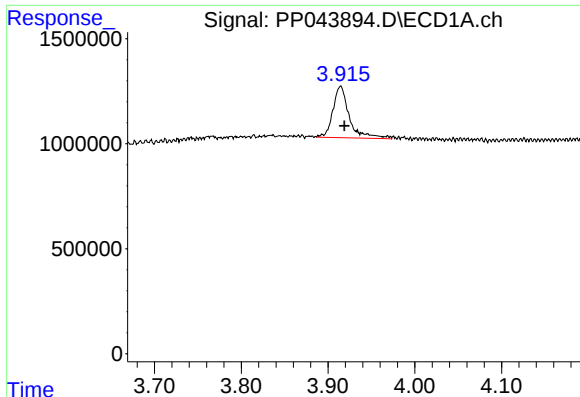

#1 Tetrachloro-m-xylene


R.T.: 3.915 min
Delta R.T.: -0.004 min
Response: 3192909
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-14B

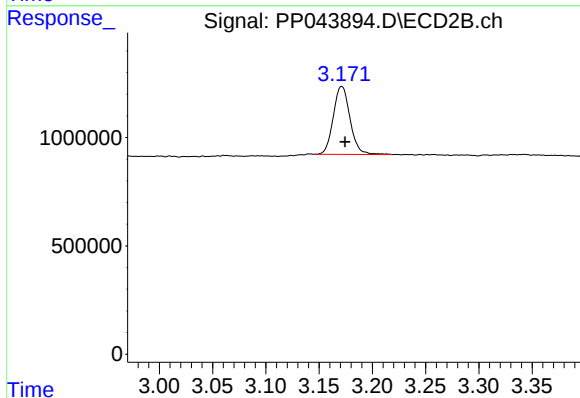


#1 Tetrachloro-m-xylene

R.T.: 3.171 min
Delta R.T.: -0.003 min
Response: 3439311
Conc: 1.83 ng/ml m

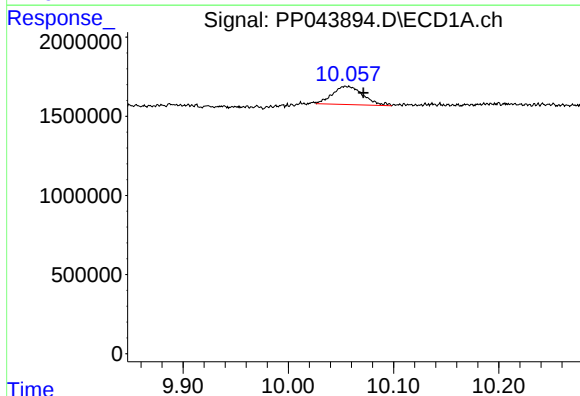


#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: -0.014 min
Response: 2330619
Conc: 1.96 ng/ml m

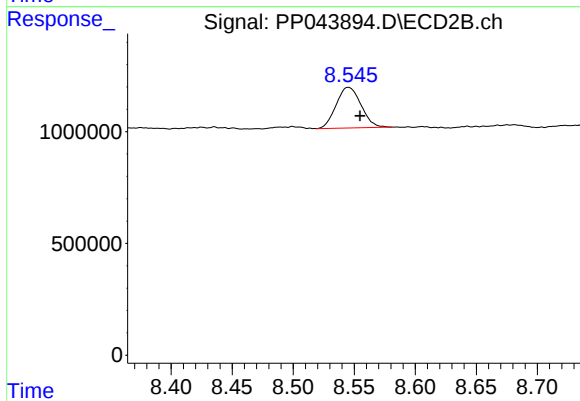

#2 Decachlorobiphenyl


R.T.: 8.545 min
Delta R.T.: -0.010 min
Response: 2584410
Conc: 1.59 ng/ml m

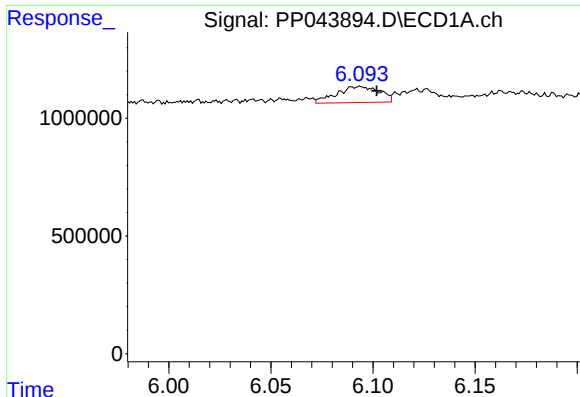

#26 AR-1254-1


R.T.: 6.093 min
Delta R.T.: -0.009 min
Response: 1014528
Conc: 13.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-14B

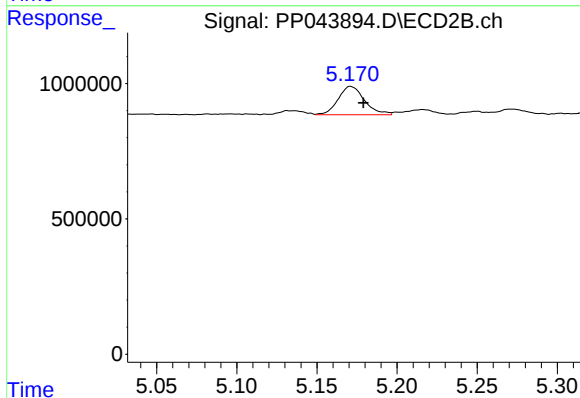


#26 AR-1254-1

R.T.: 5.171 min
Delta R.T.: -0.008 min
Response: 1201976
Conc: 13.76 ng/ml

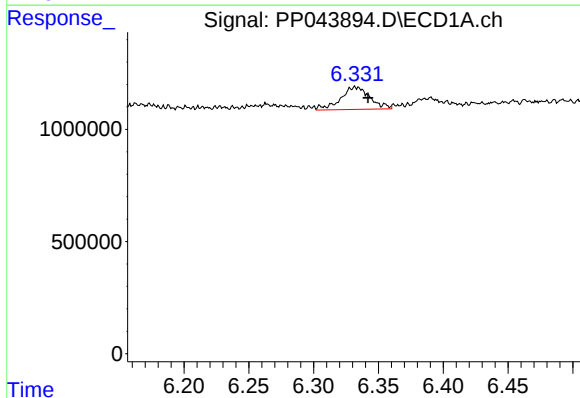


#27 AR-1254-2

R.T.: 6.332 min
Delta R.T.: -0.010 min
Response: 1573437
Conc: 14.03 ng/ml

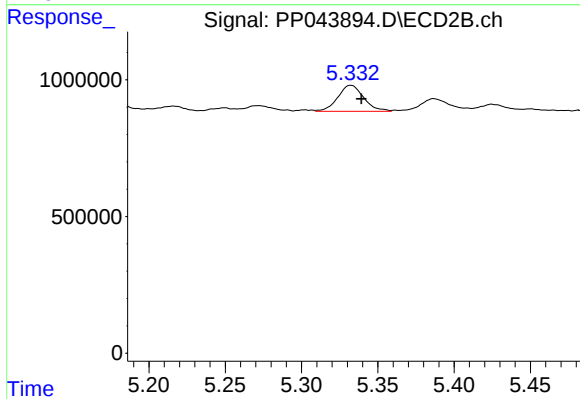

#27 AR-1254-2


R.T.: 5.332 min
Delta R.T.: -0.007 min
Response: 1123636
Conc: 14.73 ng/ml

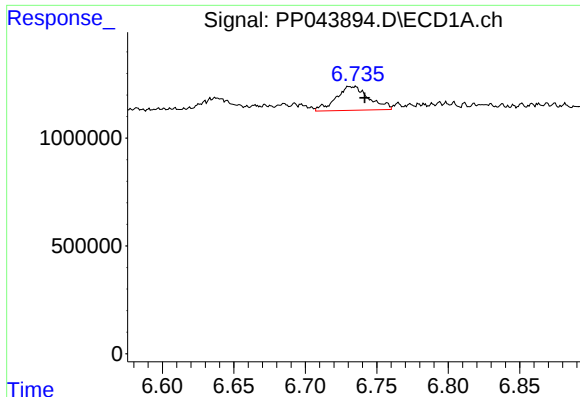

#28 AR-1254-3


R.T.: 6.735 min
Delta R.T.: -0.007 min
Response: 1774948
Conc: 15.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-14B

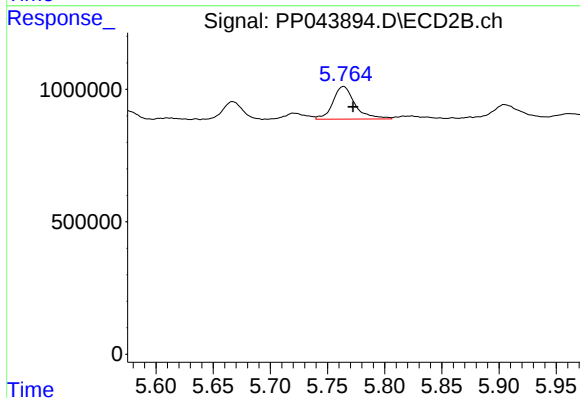


#28 AR-1254-3

R.T.: 5.764 min
Delta R.T.: -0.008 min
Response: 1660343
Conc: 13.55 ng/ml

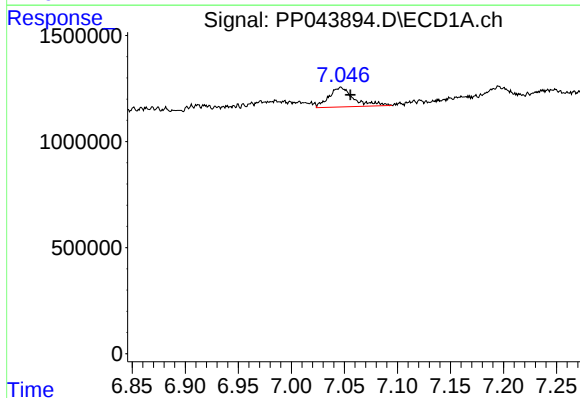


#29 AR-1254-4

R.T.: 7.046 min
Delta R.T.: -0.009 min
Response: 1502998
Conc: 18.83 ng/ml

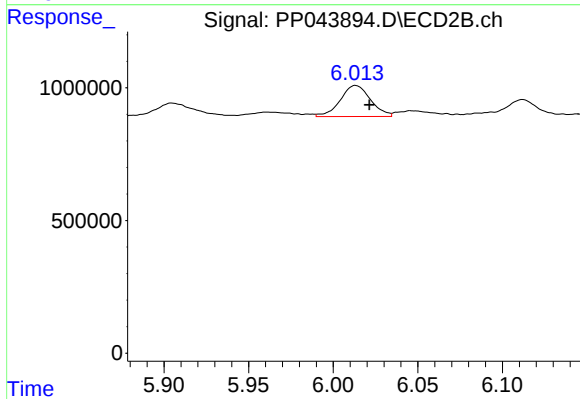

#29 AR-1254-4


R.T.: 6.013 min
Delta R.T.: -0.008 min
Response: 1460496
Conc: 18.50 ng/ml

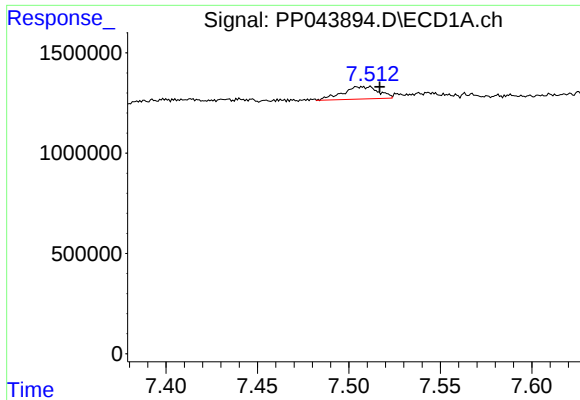

#30 AR-1254-5

R.T.: 7.511 min
Delta R.T.: -0.005 min
Response: 854193
Conc: 9.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-14B

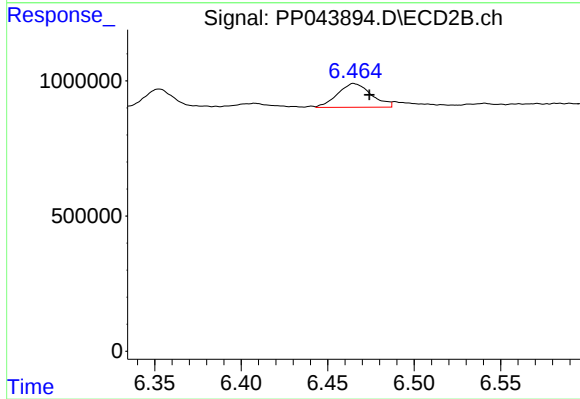

#30 AR-1254-5

R.T.: 6.465 min
Delta R.T.: -0.009 min
Response: 1192903
Conc: 10.32 ng/ml