

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
 Data File : PP043902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2022 22:47
 Operator : YP\AJ
 Sample : N1601-20 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-18B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 09:48:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.915	3.173	3166844	3057451	1.432	1.628
2) SA Decachlor...	10.059	8.547	2440548	2420473	2.055	1.492 #
Target Compounds						
26) L6 AR-1254-1	6.094	5.173	310.5E6	474.2E6	4109.326	5429.821 #
27) L6 AR-1254-2	6.334	5.333	562.9E6	400.8E6	5018.157	5254.850
28) L6 AR-1254-3	6.734	5.765	657.8E6	700.6E6	5684.473	5716.608
29) L6 AR-1254-4	7.048	6.015	597.1E6	594.0E6	7478.784	7525.525
30) L6 AR-1254-5	7.509	6.467	479.9E6	589.8E6	5595.901	5100.528


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022122\
Data File : PP043902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2022 22:47
Operator : YP\AJ
Sample : N1601-20 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-18B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 09:48:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

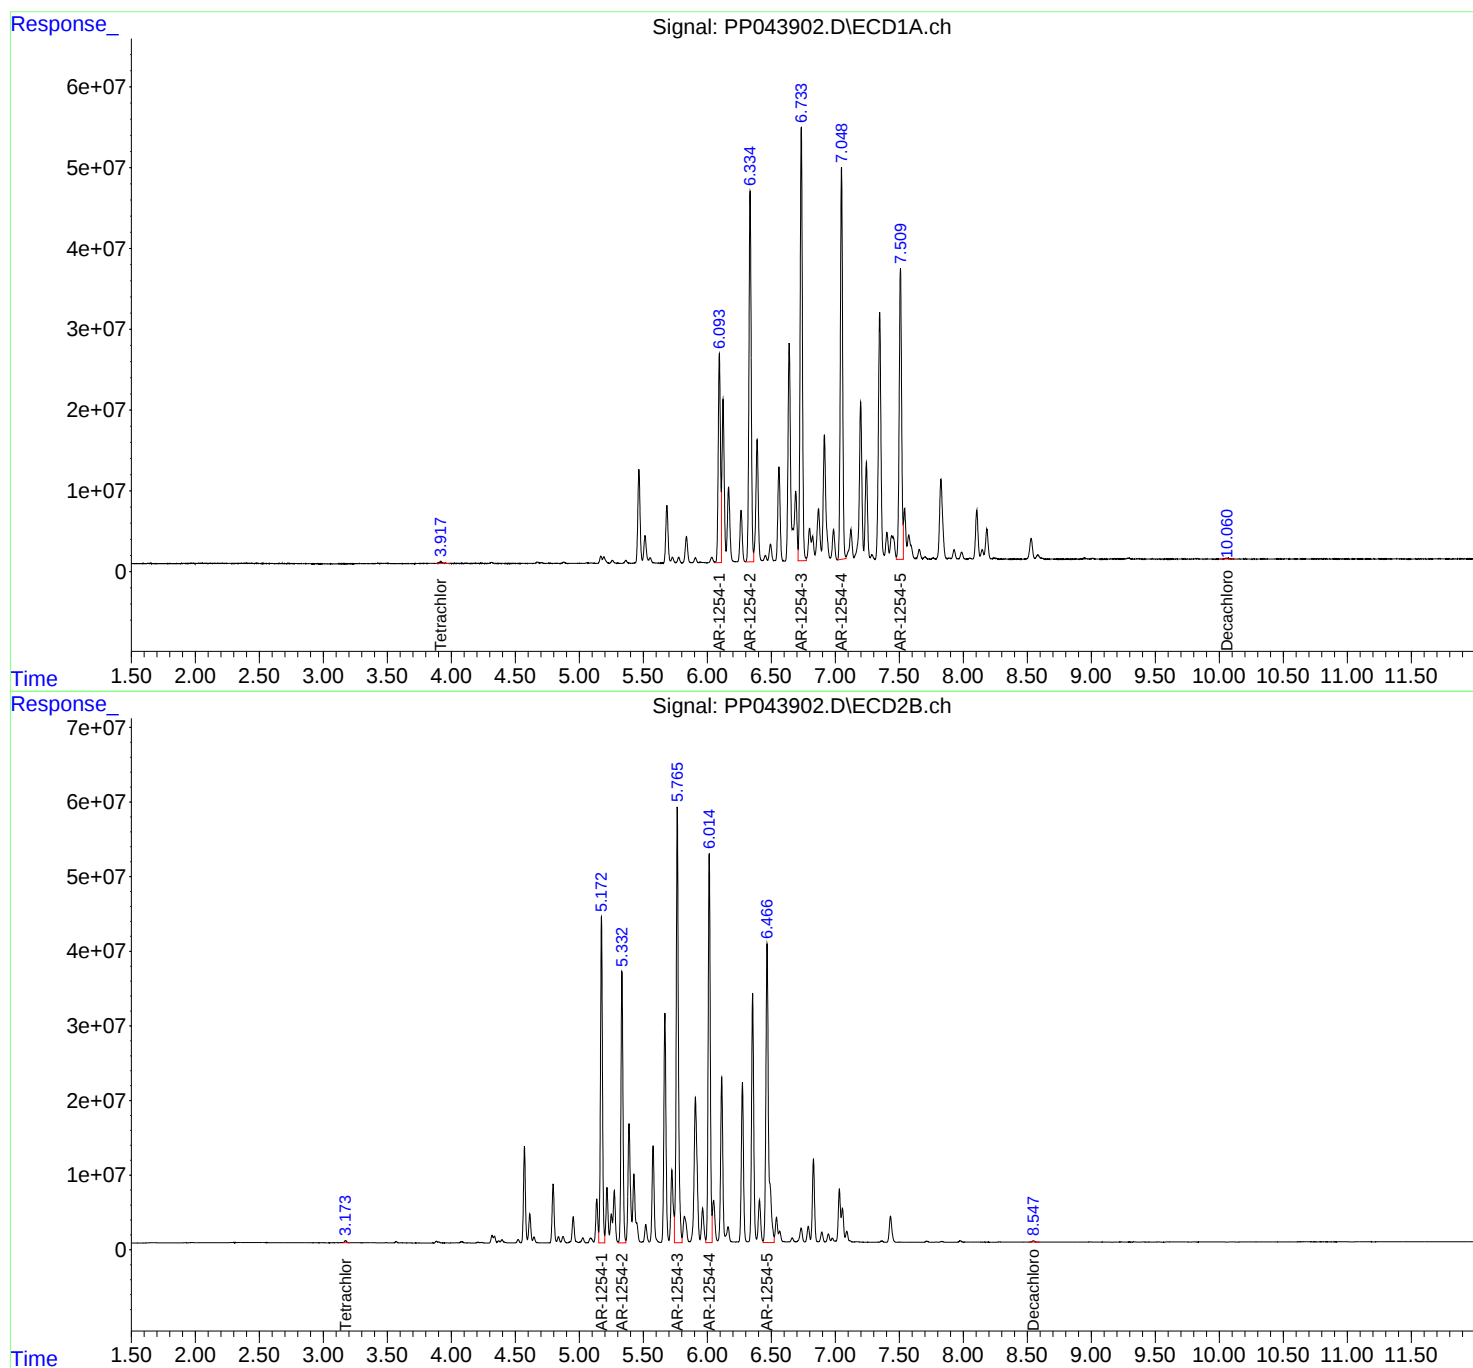


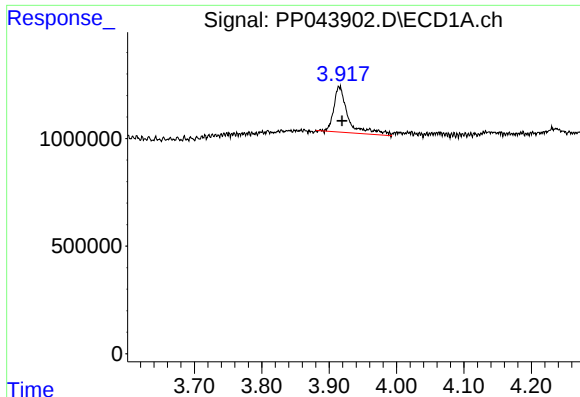

#1 Tetrachloro-m-xylene


R.T.: 3.915 min
Delta R.T.: -0.004 min
Response: 3166844
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-18B

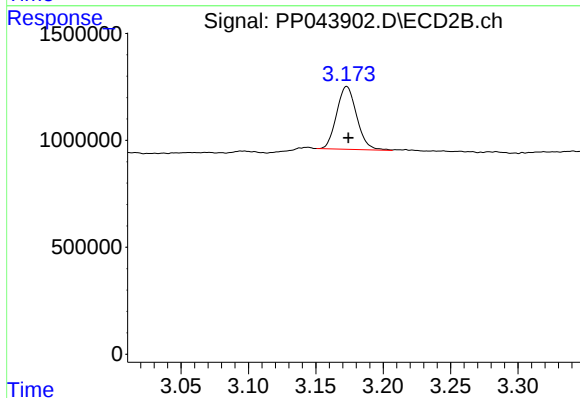


#1 Tetrachloro-m-xylene

R.T.: 3.173 min
Delta R.T.: -0.001 min
Response: 3057451
Conc: 1.63 ng/ml

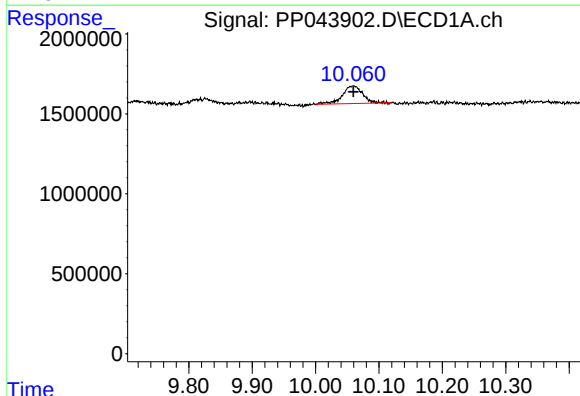


#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: 0.000 min
Response: 2440548
Conc: 2.05 ng/ml

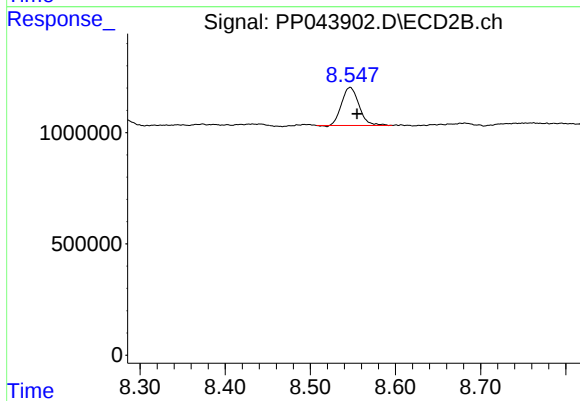

#2 Decachlorobiphenyl


R.T.: 8.547 min
Delta R.T.: -0.008 min
Response: 2420473
Conc: 1.49 ng/ml

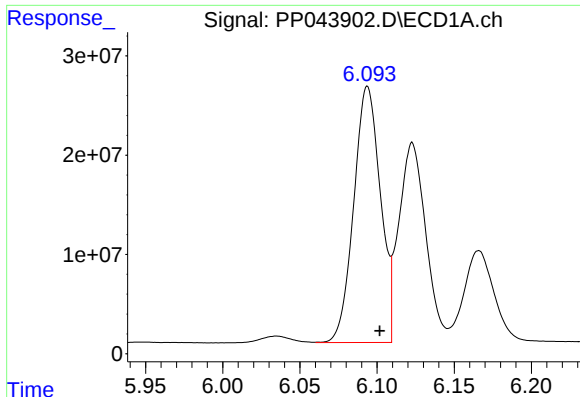

#26 AR-1254-1


R.T.: 6.094 min
Delta R.T.: -0.008 min
Response: 310486236
Conc: 4109.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-18B

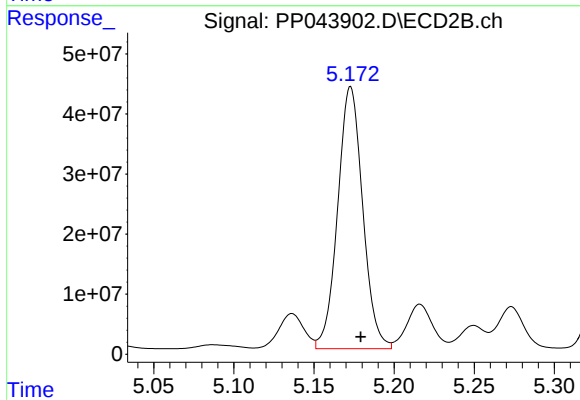


#26 AR-1254-1

R.T.: 5.173 min
Delta R.T.: -0.006 min
Response: 474200348
Conc: 5429.82 ng/ml

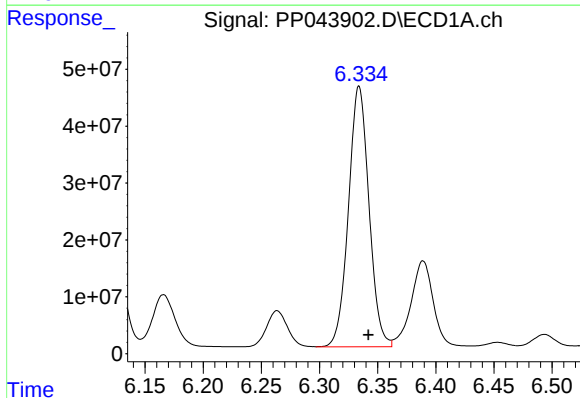


#27 AR-1254-2

R.T.: 6.334 min
Delta R.T.: -0.008 min
Response: 562879487
Conc: 5018.16 ng/ml

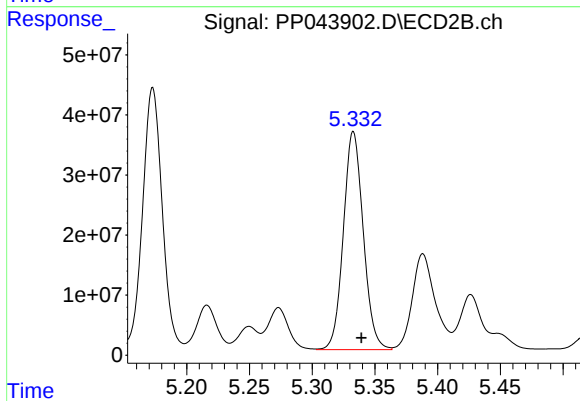

#27 AR-1254-2


R.T.: 5.333 min
Delta R.T.: -0.006 min
Response: 400825479
Conc: 5254.85 ng/ml

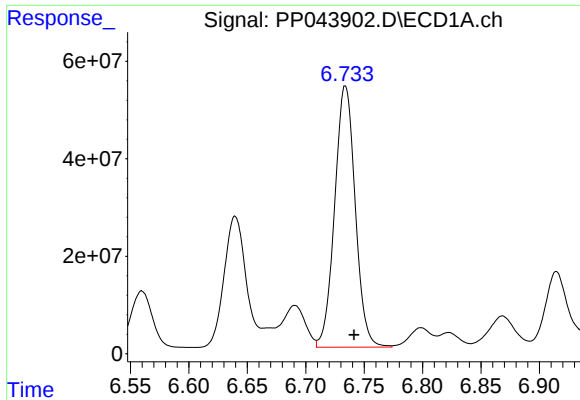

#28 AR-1254-3


R.T.: 6.734 min
Delta R.T.: -0.008 min
Response: 657765109
Conc: 5684.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-18B

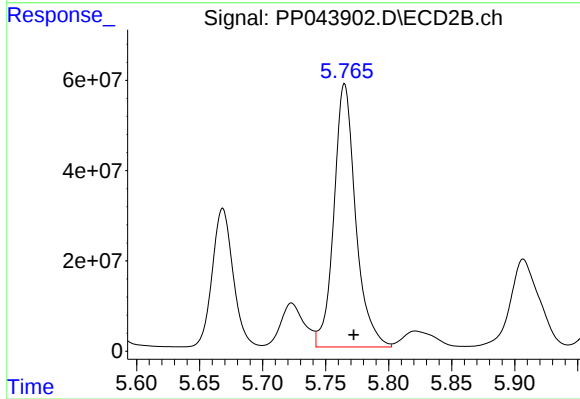


#28 AR-1254-3

R.T.: 5.765 min
Delta R.T.: -0.007 min
Response: 700617326
Conc: 5716.61 ng/ml

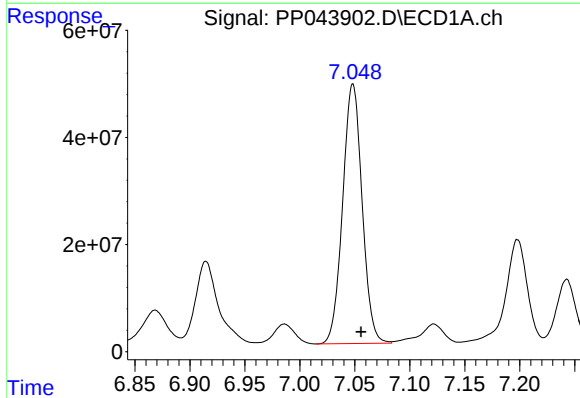


#29 AR-1254-4

R.T.: 7.048 min
Delta R.T.: -0.007 min
Response: 597057945
Conc: 7478.78 ng/ml

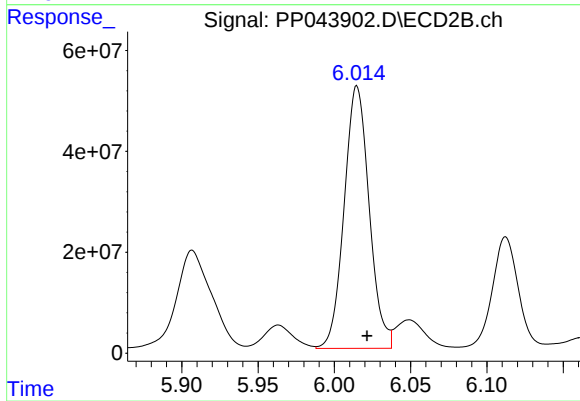

#29 AR-1254-4


R.T.: 6.015 min
Delta R.T.: -0.007 min
Response: 593951883
Conc: 7525.53 ng/ml

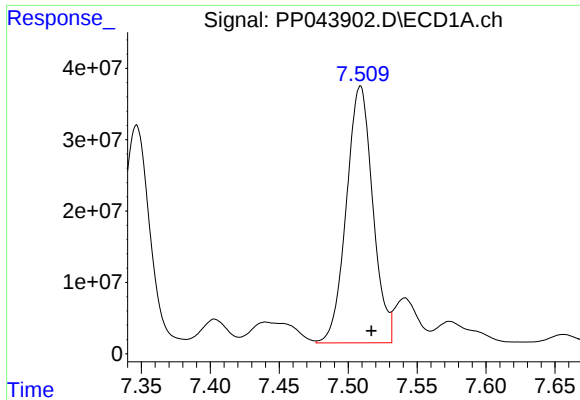

#30 AR-1254-5

R.T.: 7.509 min
Delta R.T.: -0.008 min
Response: 479921597
Conc: 5595.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-18B

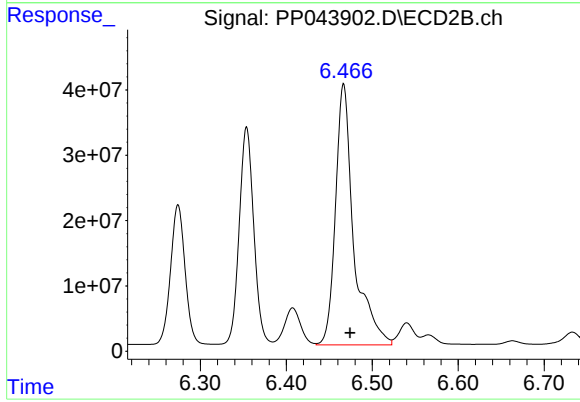

#30 AR-1254-5

R.T.: 6.467 min
Delta R.T.: -0.007 min
Response: 589848223
Conc: 5100.53 ng/ml