

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022125\
 Data File : PP069963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 13:20
 Operator : YP\AJ
 Sample : Q1396-04 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEH4134-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2025
 Supervised By :Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 05:15:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 29 00:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	2018061	1301970	1.410m	1.459m
2) SA Decachlor...	10.249	8.885	2514114	2825849	2.300	2.526m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022125\
Data File : PP069963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 13:20
Operator : YP\AJ
Sample : Q1396-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEH4134-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2025
Supervised By :Ankita Jodhani 02/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 05:15:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 29 00:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

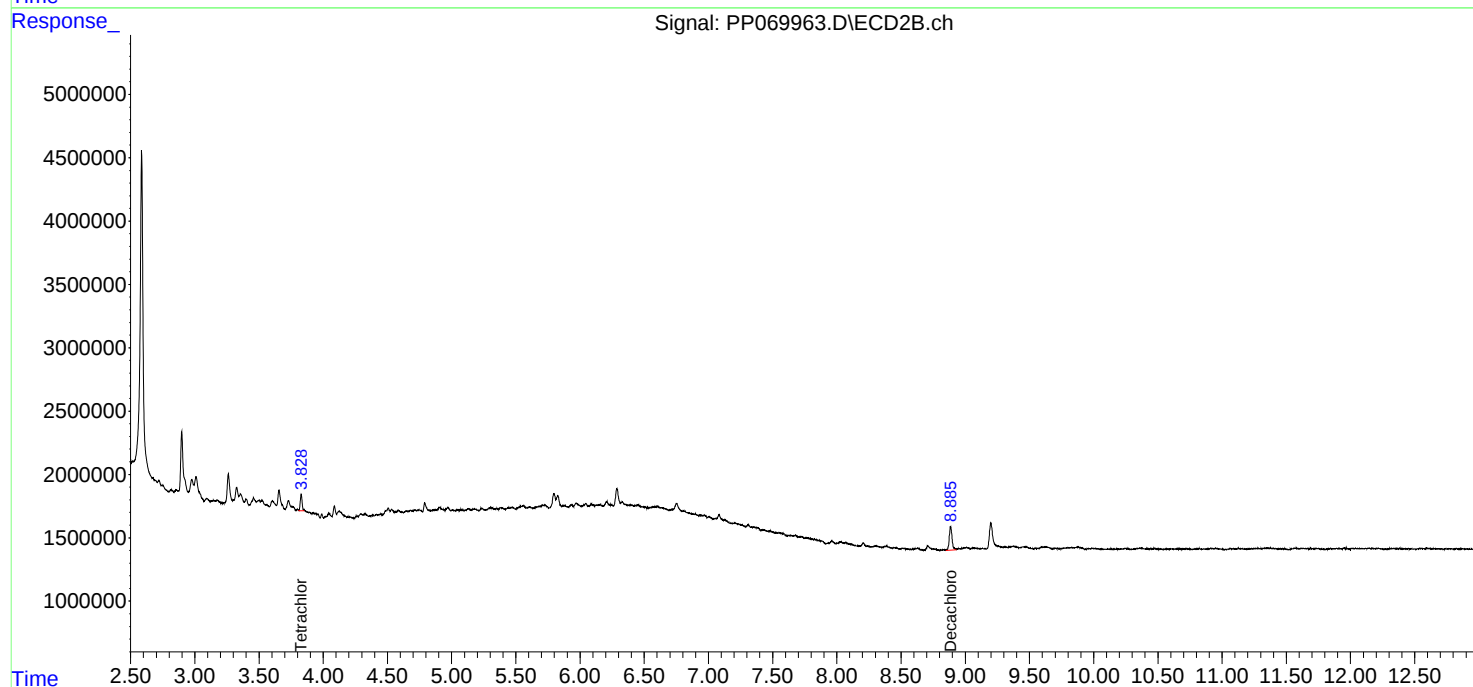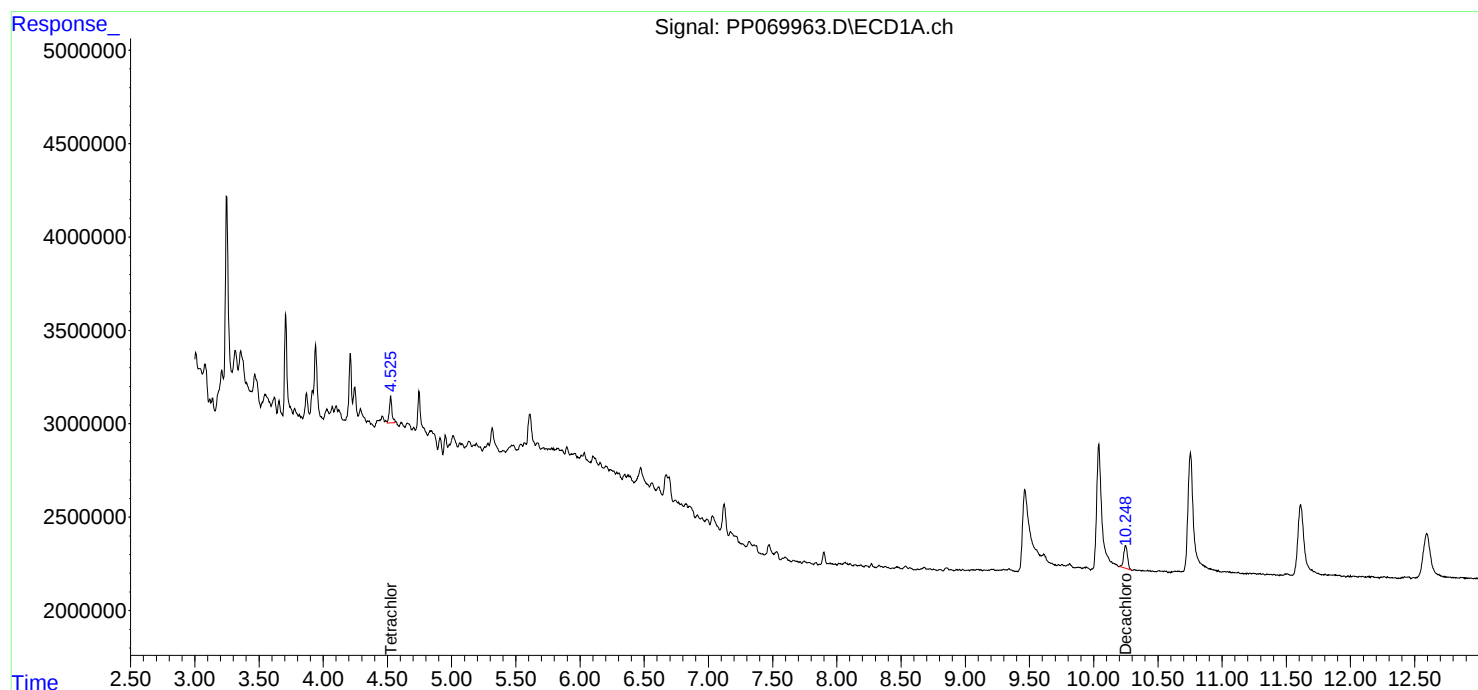

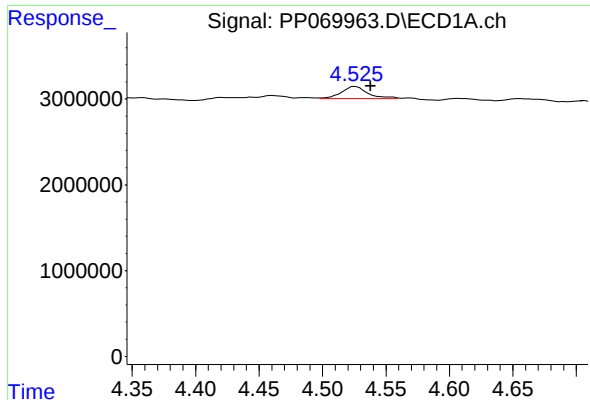


#1 Tetrachloro-m-xylene

R.T.: 4.525 min
Delta R.T.: -0.013 min
Response: 2018061
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEH4134-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2025
Supervised By :Ankita Jodhani 02/24/2025

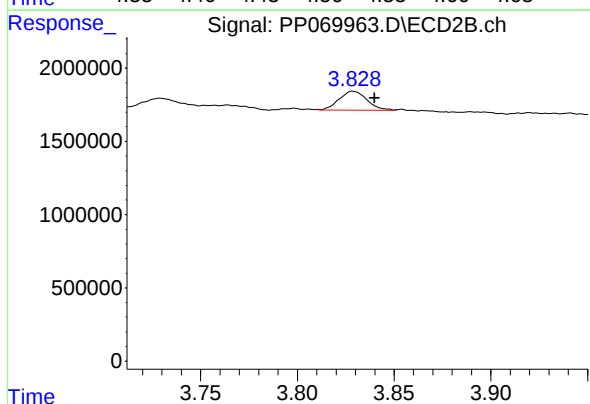


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.012 min
Response: 1301970
Conc: 1.46 ng/ml m

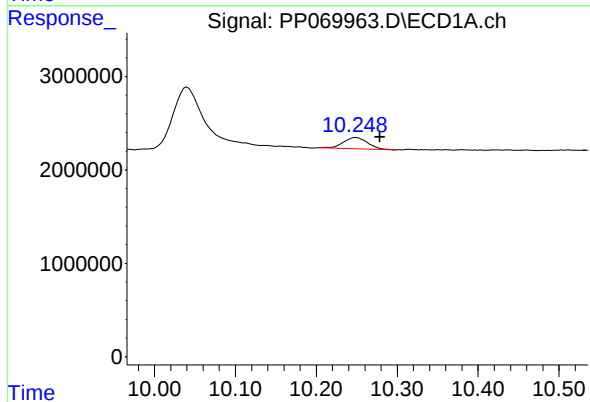

#2 Decachlorobiphenyl

R.T.: 10.249 min
Delta R.T.: -0.029 min
Response: 2514114
Conc: 2.30 ng/ml

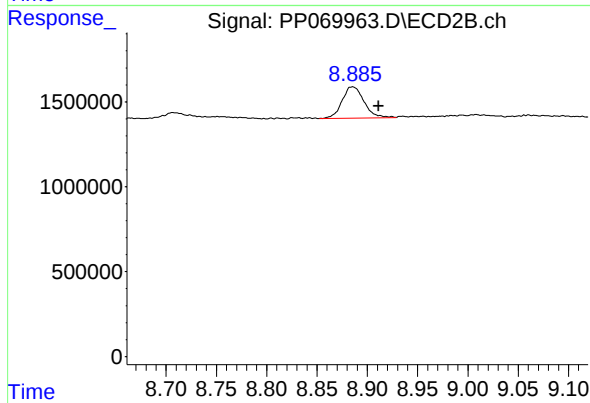

#2 Decachlorobiphenyl

R.T.: 8.885 min
Delta R.T.: -0.026 min
Response: 2825849
Conc: 2.53 ng/ml m