

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022222\
 Data File : PP043935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2022 18:19
 Operator : YP\AJ
 Sample : N1633-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20220099-MR-2-(DISCRETE)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/23/2022
 Supervised By :Ankita Jodhani 02/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 00:41:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.915	3.172	37739832	35384147	17.069	18.839
2) SA Decachlor...	10.058	8.542	22173883	8551677	18.667	5.271m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022222\
Data File : PP043935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2022 18:19
Operator : YP\AJ
Sample : N1633-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20220099-MR-2-(DISCRETE)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 00:41:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

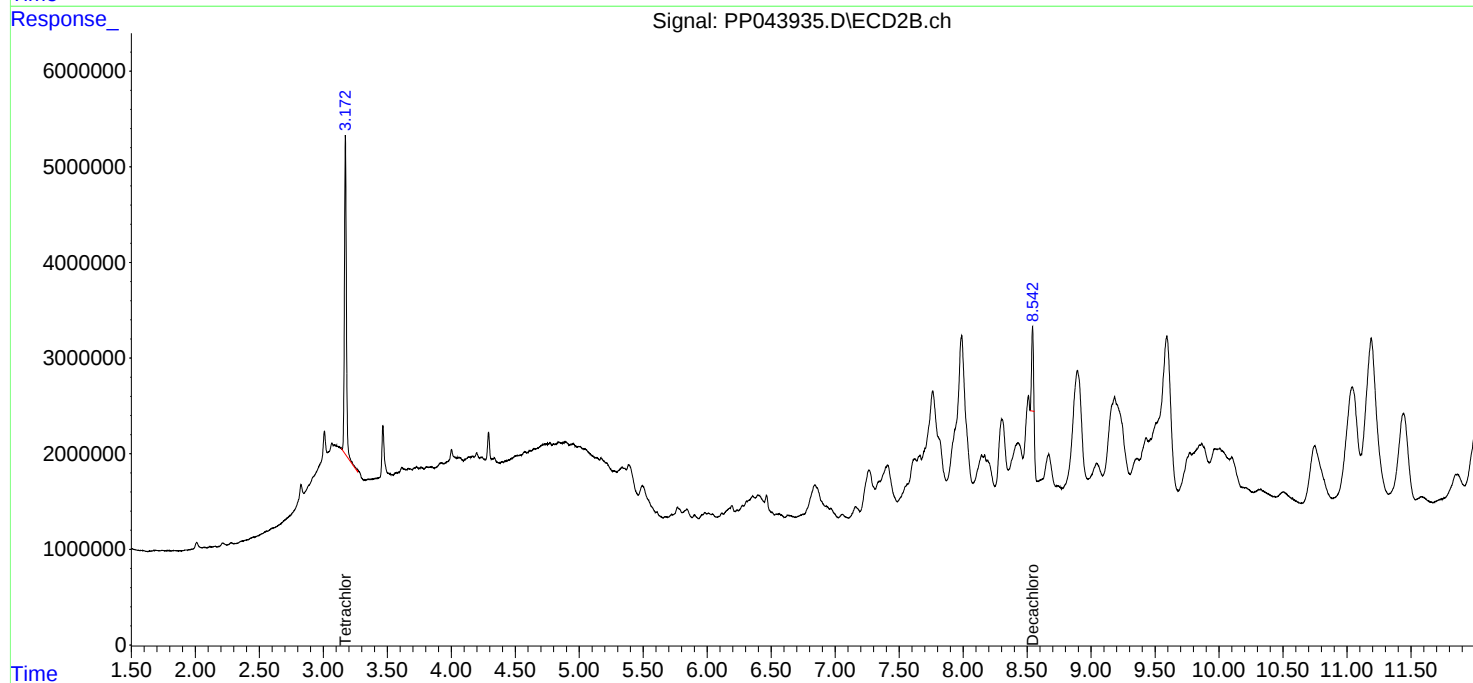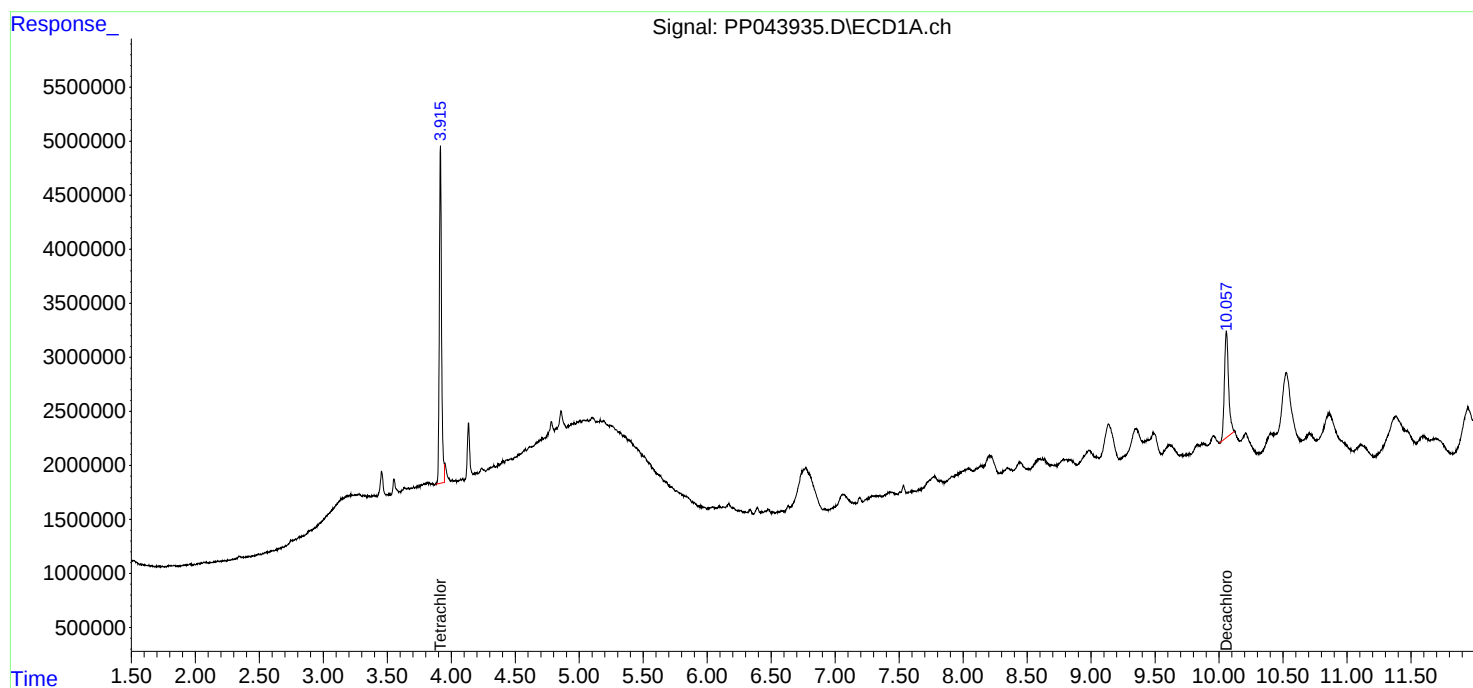

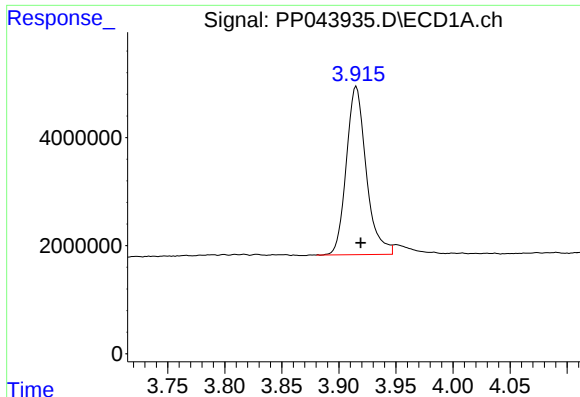


#1 Tetrachloro-m-xylene

R.T.: 3.915 min
Delta R.T.: -0.004 min
Response: 37739832
Conc: 17.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
20220099-MR-2-(DISCRETE)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

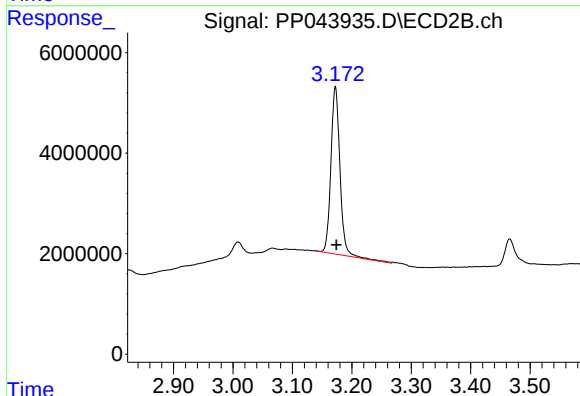


#1 Tetrachloro-m-xylene

R.T.: 3.172 min
Delta R.T.: -0.002 min
Response: 35384147
Conc: 18.84 ng/ml

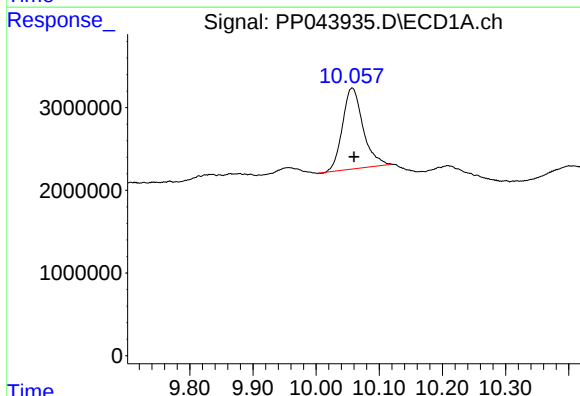

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: -0.002 min
Response: 22173883
Conc: 18.67 ng/ml

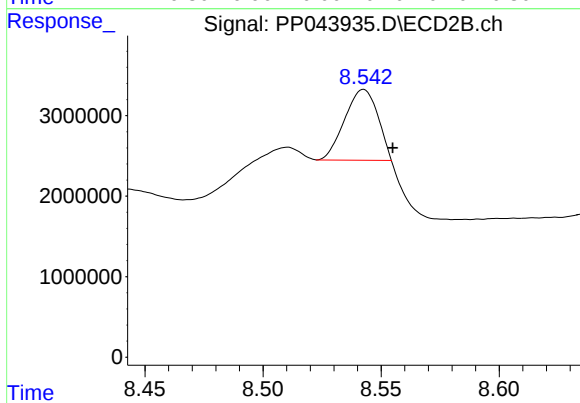

#2 Decachlorobiphenyl

R.T.: 8.542 min
Delta R.T.: -0.012 min
Response: 8551677
Conc: 5.27 ng/ml m