

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
 Data File : PP055881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2023 21:23
 Operator : YP\AJ
 Sample : 01647-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ACADEMY-SUBSTATION

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2023
 Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 23:24:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.569	41581848	20974975	25.807	14.365 #
2) SA Decachlor...	10.072	8.570	18970007	12245502	9.299	10.794m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
Data File : PP055881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2023 21:23
Operator : YP\AJ
Sample : 01647-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ACADEMY-SUBSTATION


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 23:24:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

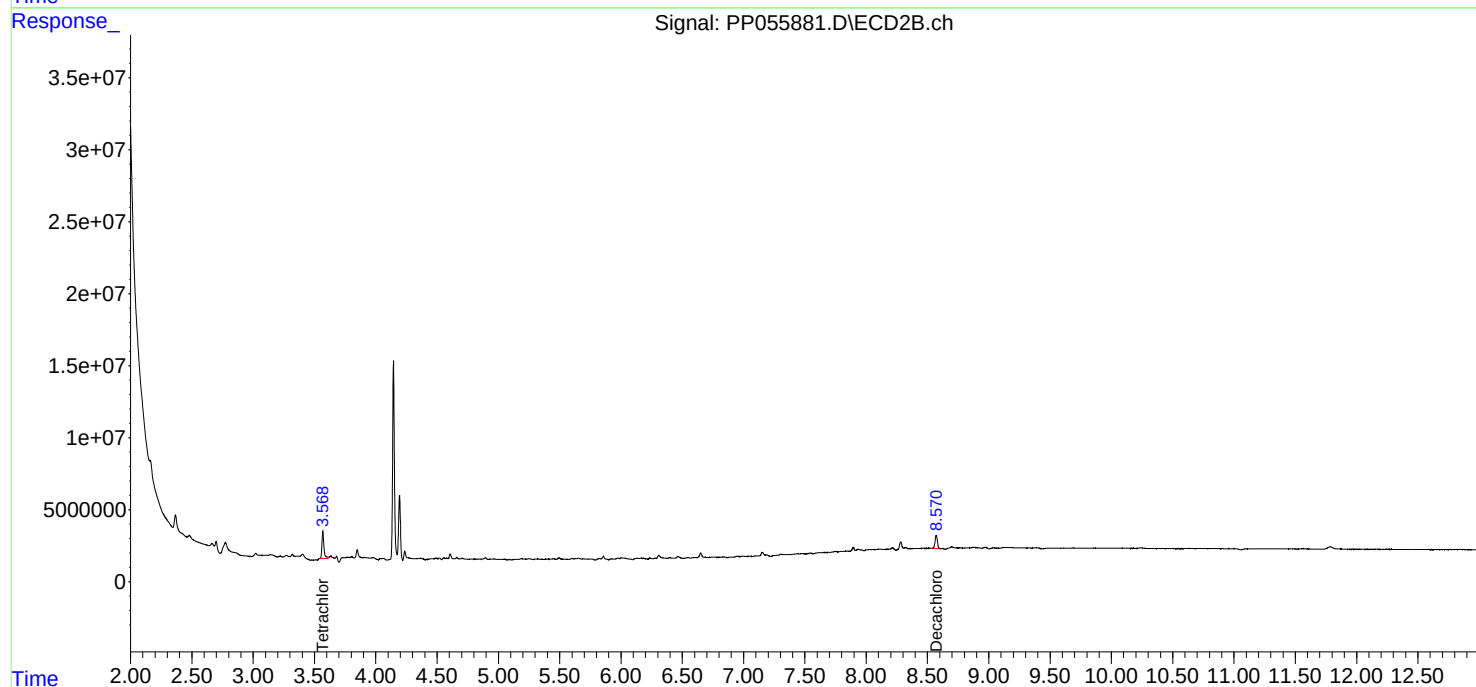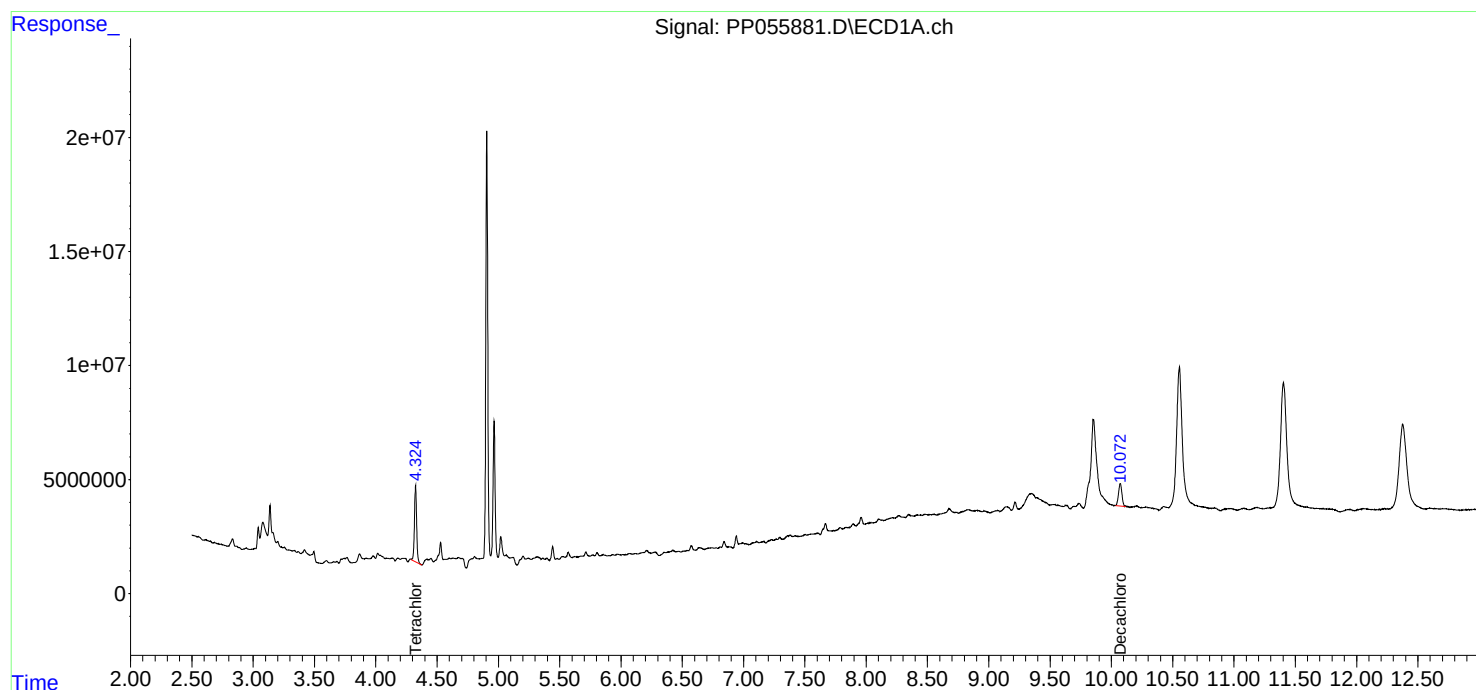

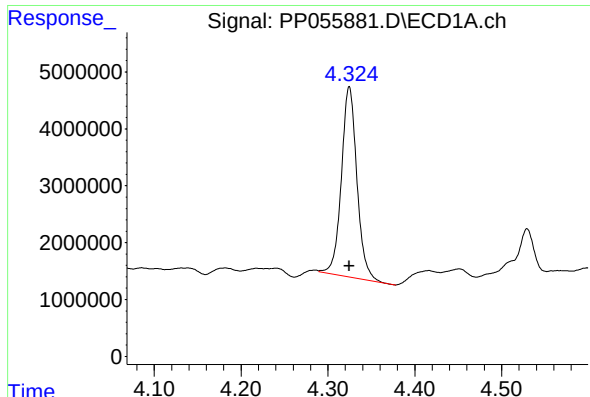


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 41581848
Conc: 25.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
ACADEMY-SUBSTATION


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

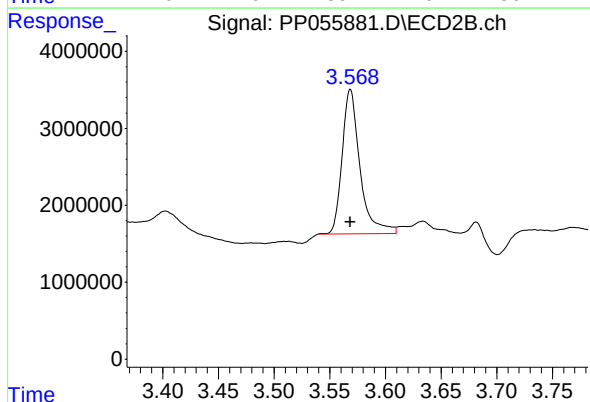


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 20974975
Conc: 14.36 ng/ml

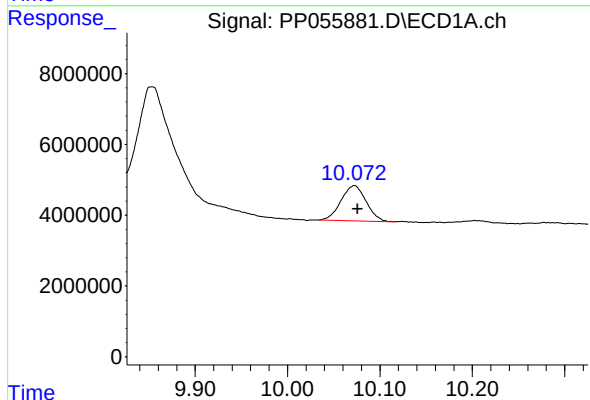

#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: -0.003 min
Response: 18970007
Conc: 9.30 ng/ml

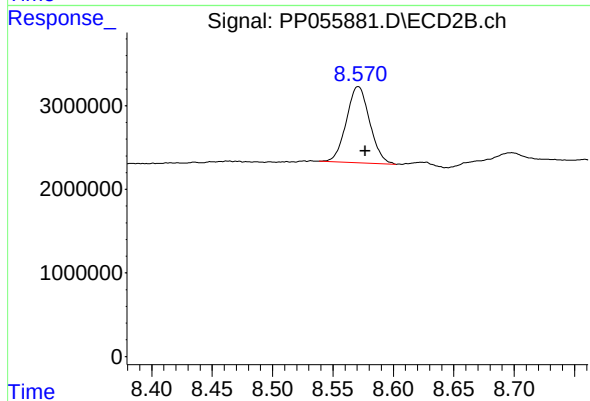

#2 Decachlorobiphenyl

R.T.: 8.570 min
Delta R.T.: -0.006 min
Response: 12245502
Conc: 10.79 ng/ml m