

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
 Data File : PP055888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2023 23:18
 Operator : YP\AJ
 Sample : 01655-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2023
 Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 02:09:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.324	3.568	35624694	29981442	22.110m	20.533
2) SA Decachlor...	10.074	8.571	33324611	20496373	16.336m	18.067

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
Data File : PP055888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2023 23:18
Operator : YP\AJ
Sample : 01655-05
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 02:09:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

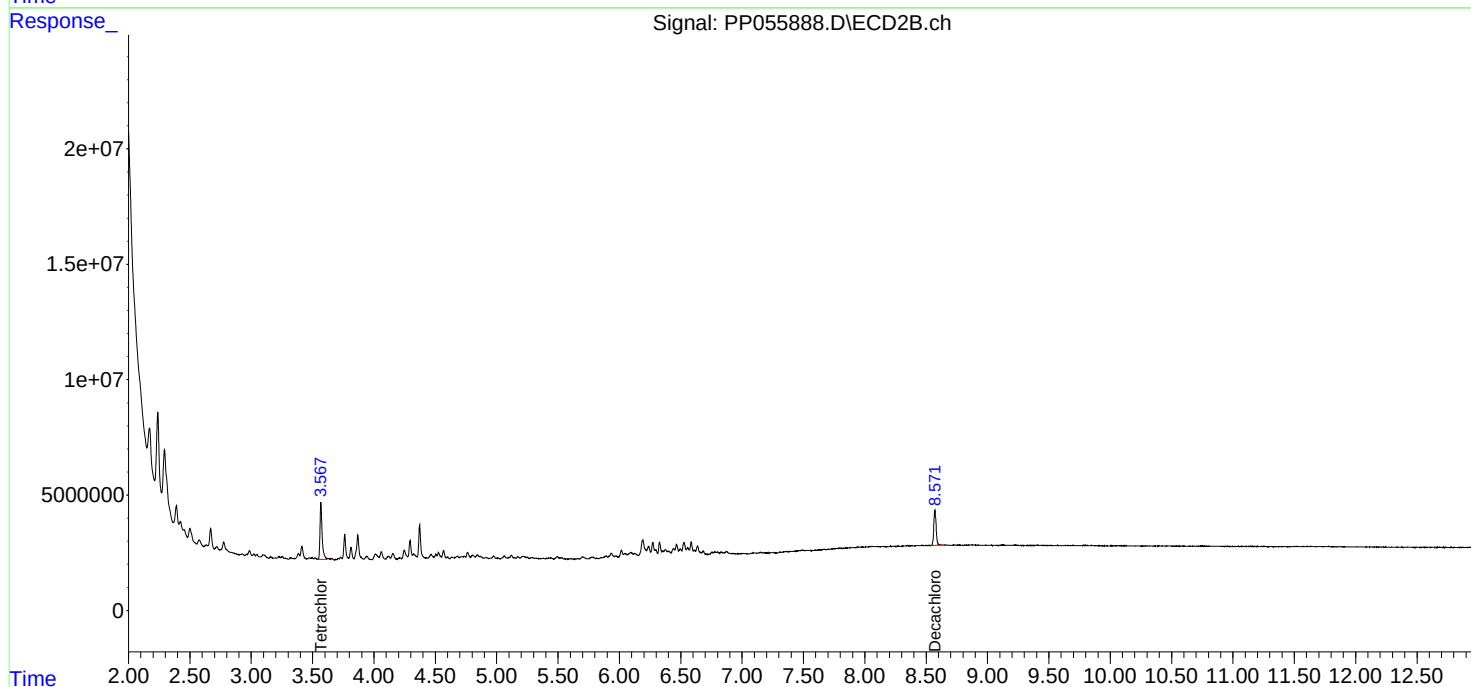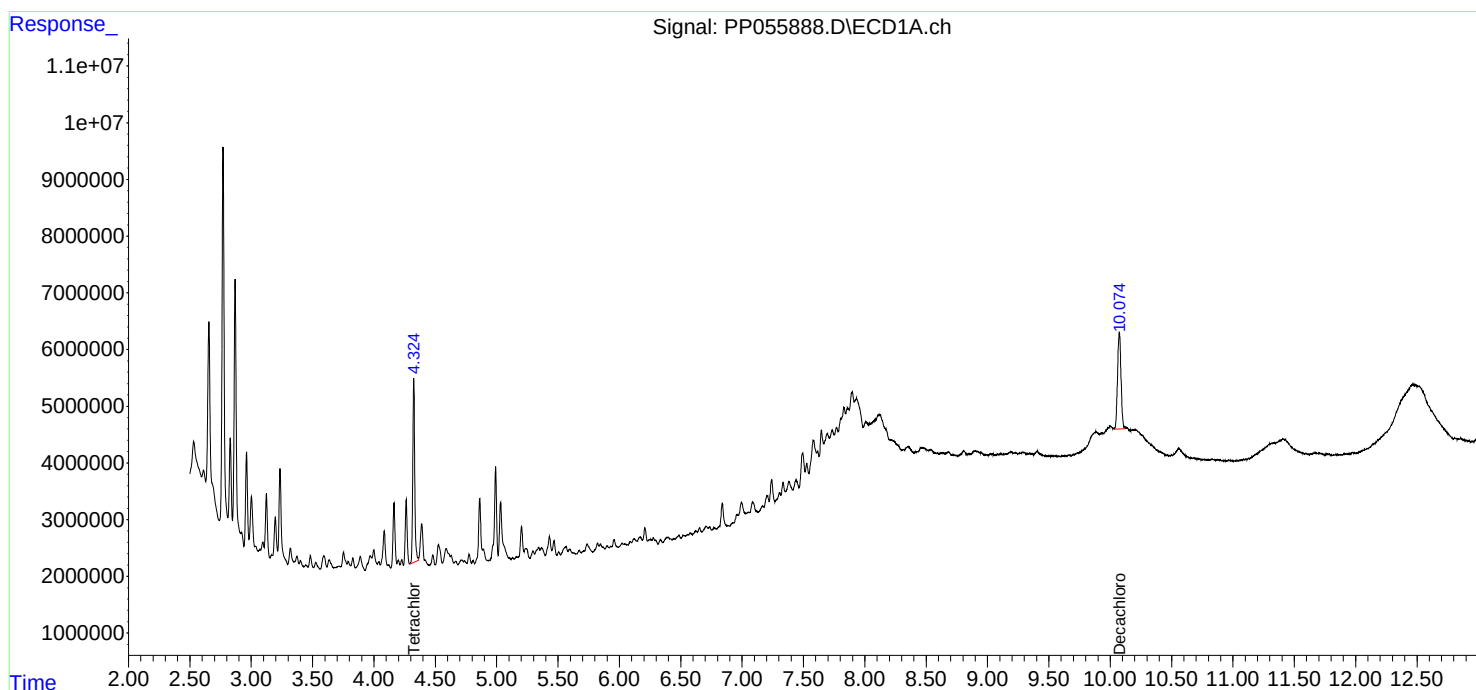

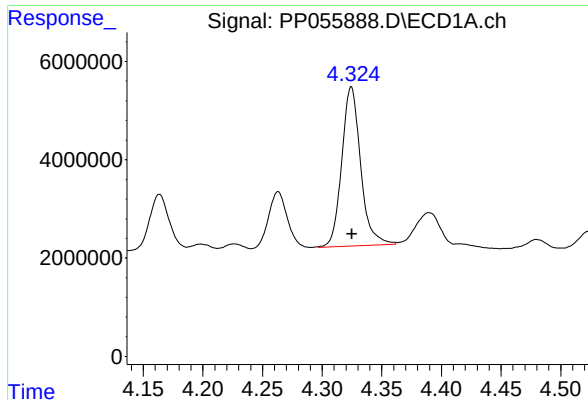


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 35624694
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

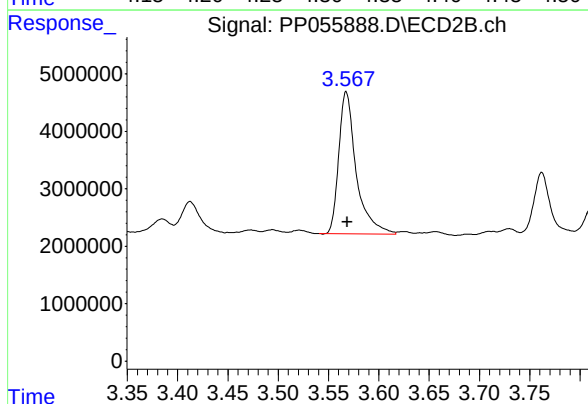


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.001 min
Response: 29981442
Conc: 20.53 ng/ml

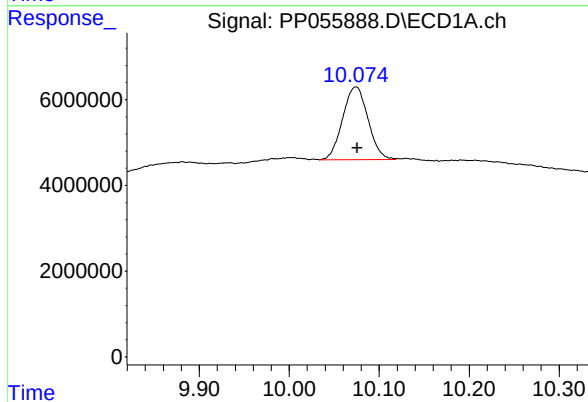

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: -0.002 min
Response: 33324611
Conc: 16.34 ng/ml m

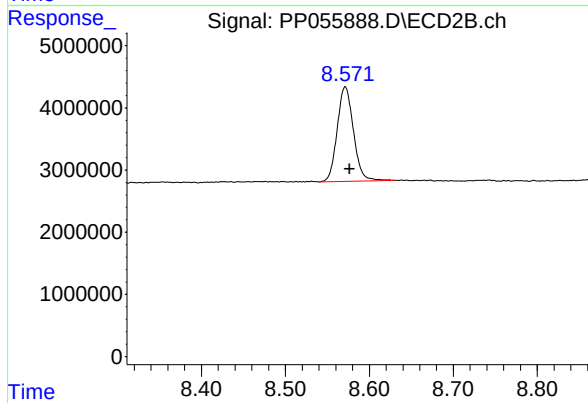

#2 Decachlorobiphenyl

R.T.: 8.571 min
Delta R.T.: -0.005 min
Response: 20496373
Conc: 18.07 ng/ml