

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
 Data File : PP055896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2023 02:11
 Operator : YP\AJ
 Sample : 01643-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34292

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2023
 Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 03:20:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.566	22976526	20775266	14.260	14.228
2) SA Decachlor...	10.070	8.568	20025296	14435601	9.817m	12.724m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022323\
Data File : PP055896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2023 02:11
Operator : YP\AJ
Sample : 01643-06
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
34292


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 03:20:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

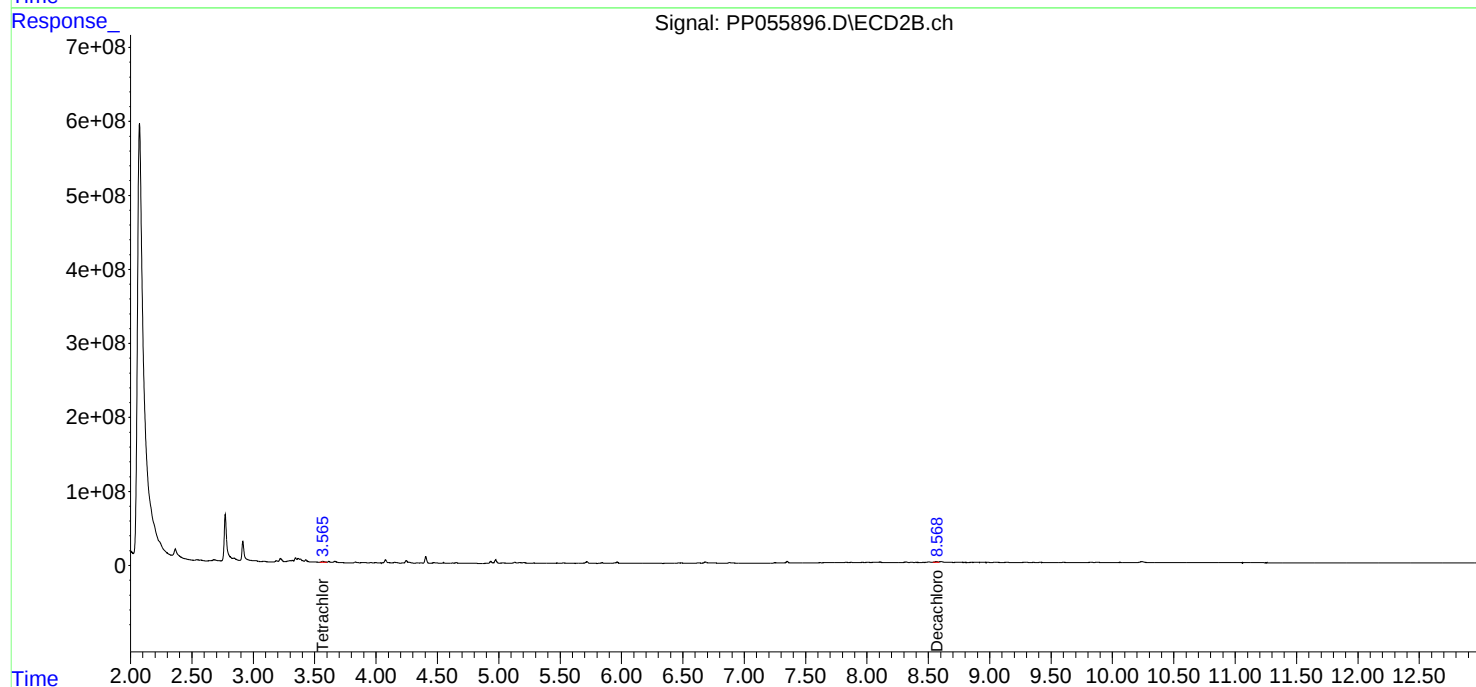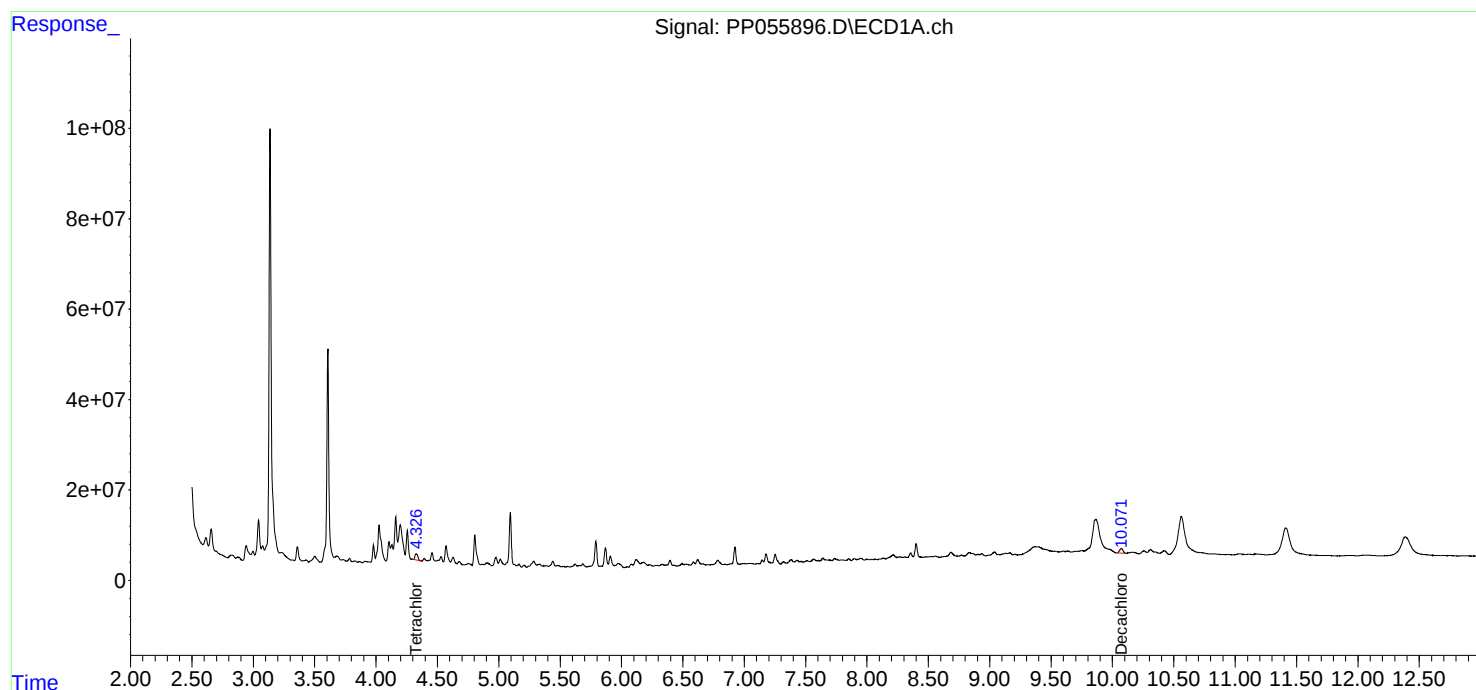

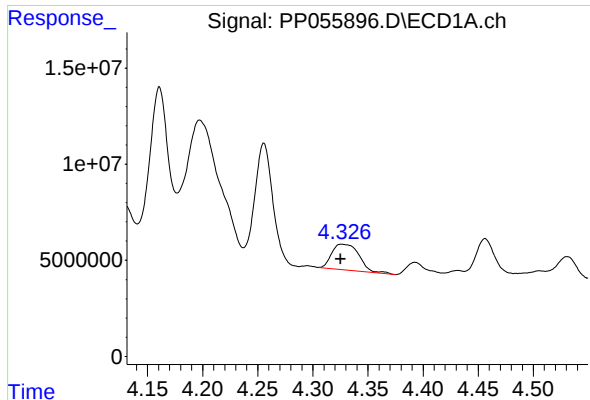


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: 0.001 min
Response: 22976526
Conc: 14.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
34292


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/24/2023
Supervised By :Ankita Jodhani 02/24/2023

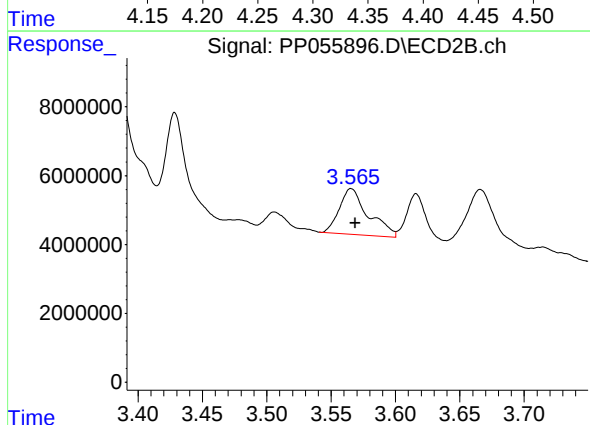


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 20775266
Conc: 14.23 ng/ml

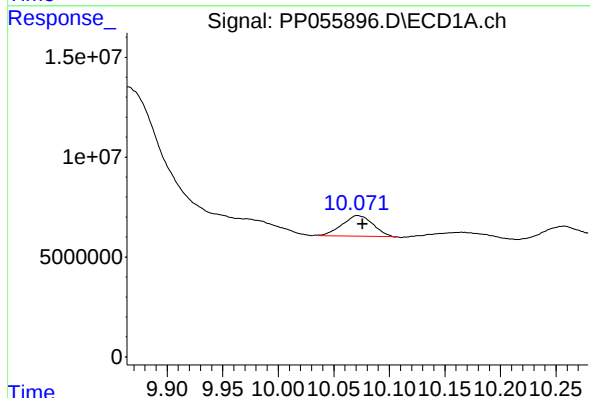

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: -0.005 min
Response: 20025296
Conc: 9.82 ng/ml m

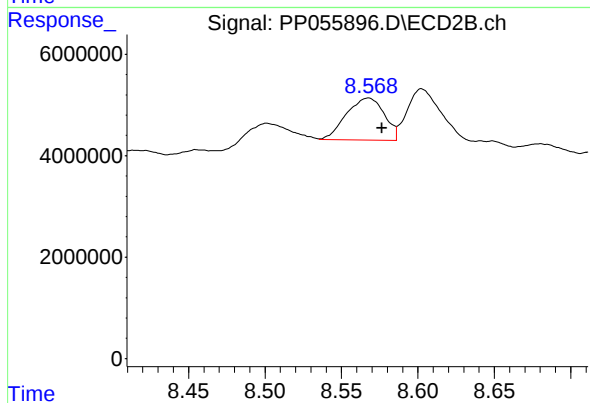

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: -0.009 min
Response: 14435601
Conc: 12.72 ng/ml m