

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022324\
 Data File : PP063377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2024 20:06
 Operator : YP\AJ
 Sample : PB159224BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB159224BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 00:23:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 05 12:13:11 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.642	48375516	48697770	20.224	20.488
2) SA Decachlor...	10.369	8.693	49902268	53517434	22.190	21.605
Target Compounds						
9) L2 AR-1221-2	0.000	3.944	0	628132	N.D.	31.801 #
28) L6 AR-1254-3	7.130	0.000	1176271	0	8.557	N.D. #
32) L7 AR-1260-2	0.000	6.401f	0	380871	N.D.	2.579 #
35) L7 AR-1260-5	0.000	7.293	0	557339	N.D.	2.243 #
40) L8 AR-1262-5	0.000	8.136f	0	174359	N.D.	2.136 #
43) L9 AR-1268-3	9.142	0.000	23735815	0	99.575	N.D. #
44) L9 AR-1268-4	0.000	8.136	0	174359	N.D.	1.986 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022324\
Data File : PP063377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2024 20:06
Operator : YP\AJ
Sample : PB159224BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB159224BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 00:23:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 05 12:13:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

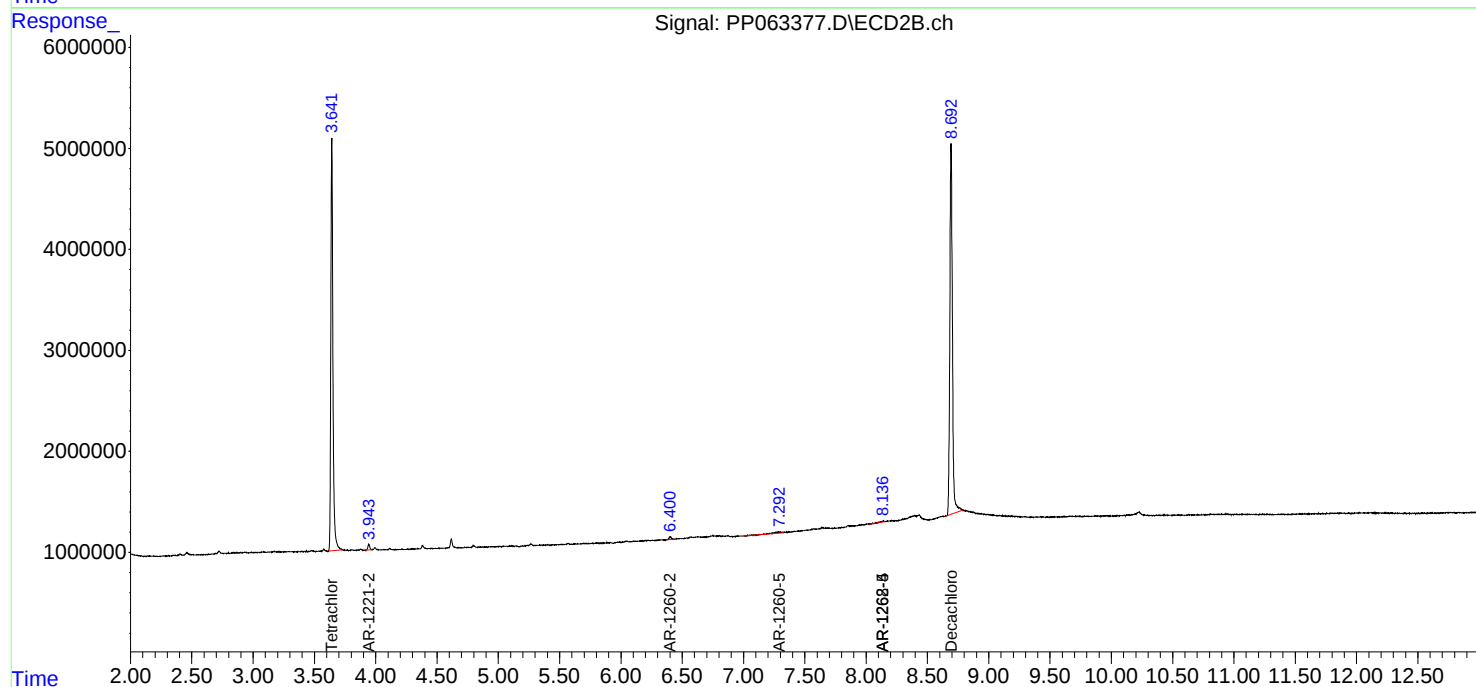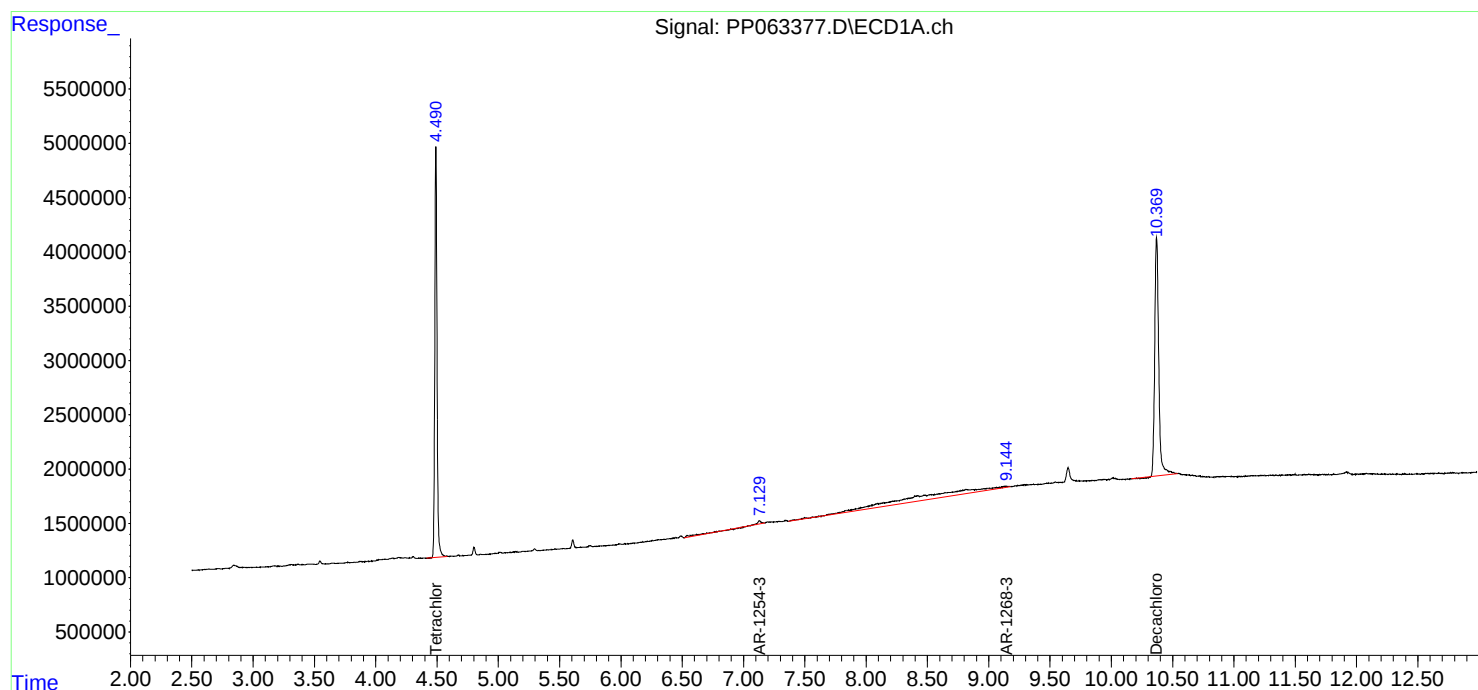


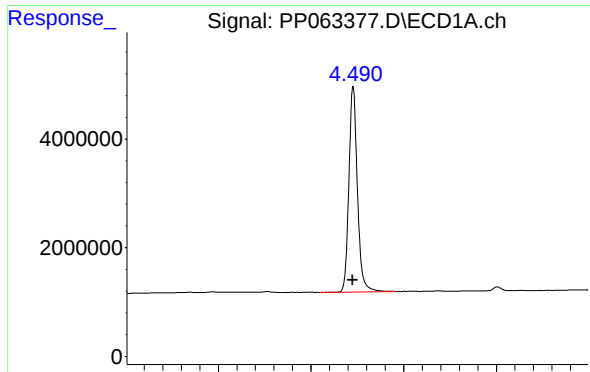

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: 0.001 min
Response: 48375516
Conc: 20.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB159224BL

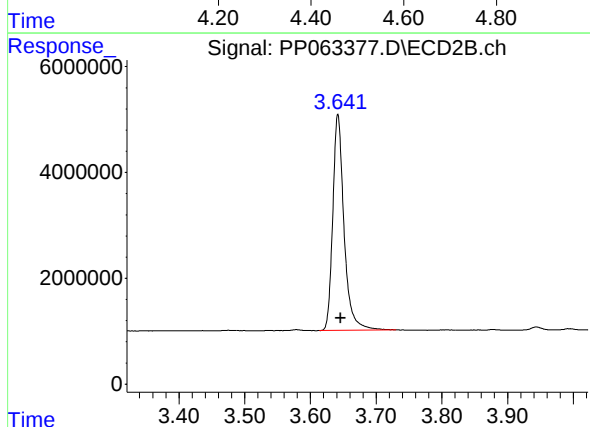


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 48697770
Conc: 20.49 ng/ml

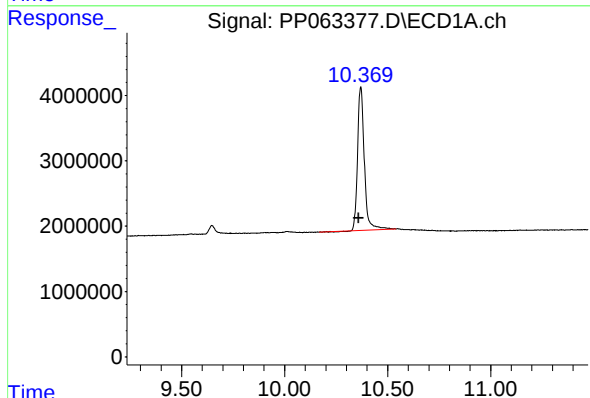


#2 Decachlorobiphenyl

R.T.: 10.369 min
Delta R.T.: 0.010 min
Response: 49902268
Conc: 22.19 ng/ml

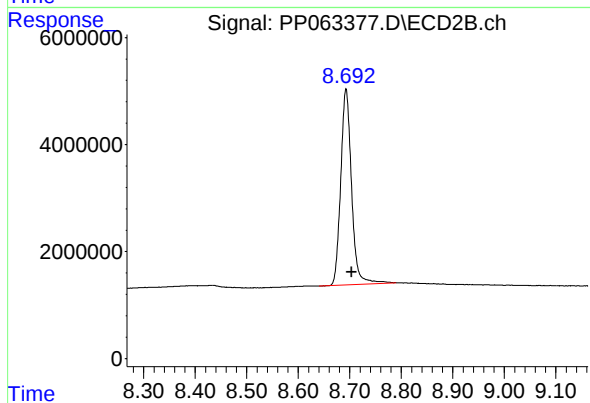

#2 Decachlorobiphenyl


R.T.: 8.693 min
Delta R.T.: -0.011 min
Response: 53517434
Conc: 21.60 ng/ml

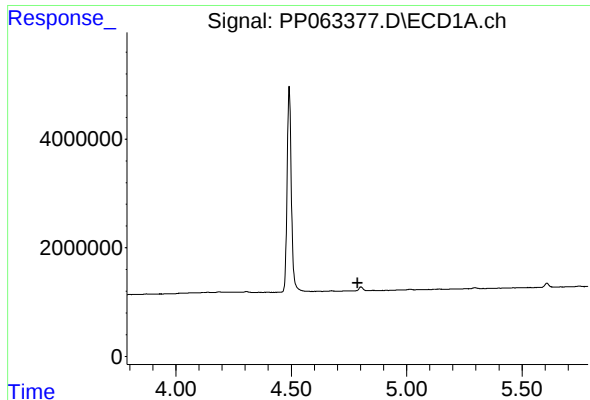

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB159224BL

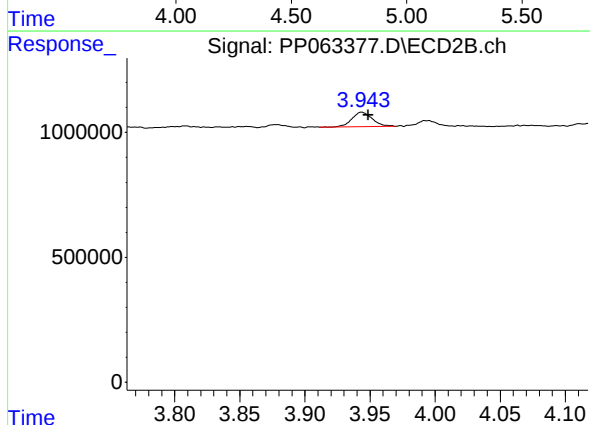


#9 AR-1221-2

R.T.: 3.944 min
Delta R.T.: -0.005 min
Response: 628132
Conc: 31.80 ng/ml

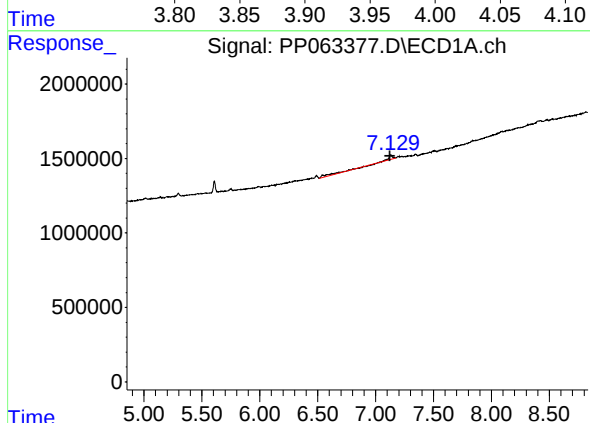


#28 AR-1254-3

R.T.: 7.130 min
Delta R.T.: 0.003 min
Response: 1176271
Conc: 8.56 ng/ml

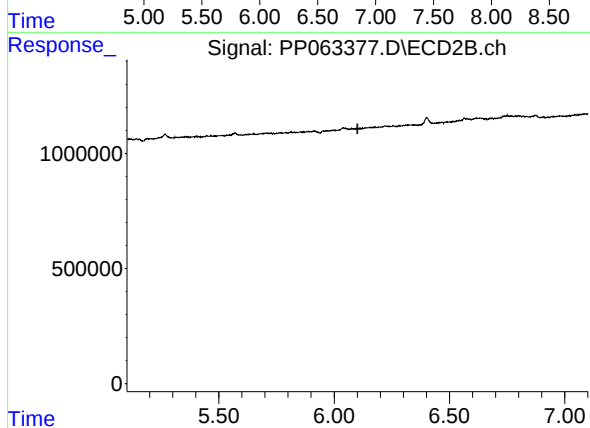

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.101 min
Response: 0
Conc: N.D.

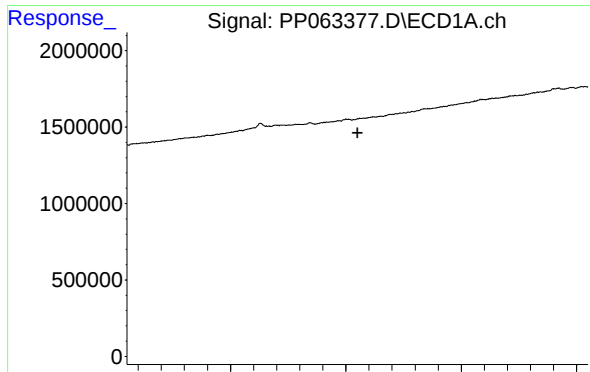

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB159224BL

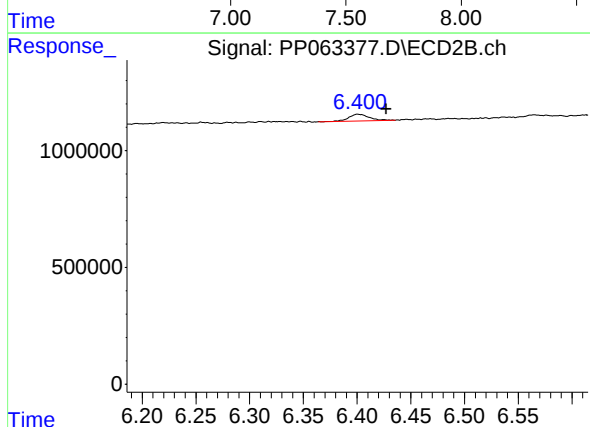


#32 AR-1260-2

R.T.: 6.401 min
Delta R.T.: -0.026 min
Response: 380871
Conc: 2.58 ng/ml

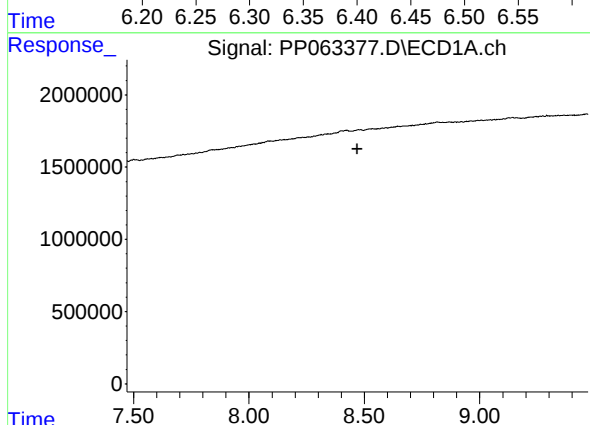


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.469 min
Response: 0
Conc: N.D.

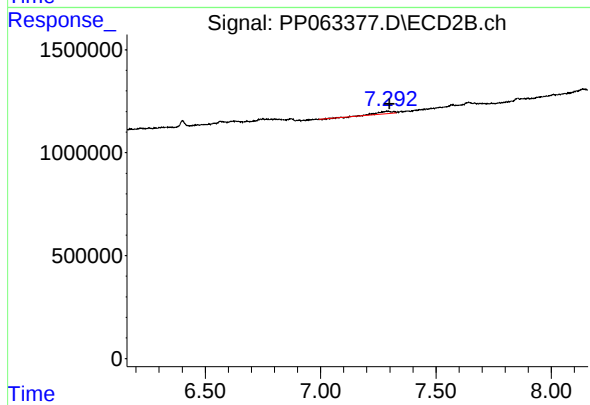

#35 AR-1260-5


R.T.: 7.293 min
Delta R.T.: -0.006 min
Response: 557339
Conc: 2.24 ng/ml

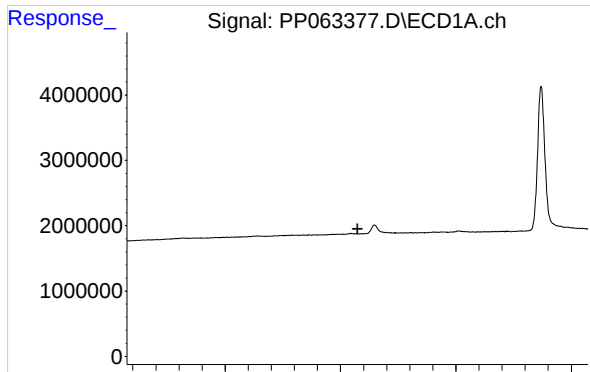

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB159224BL

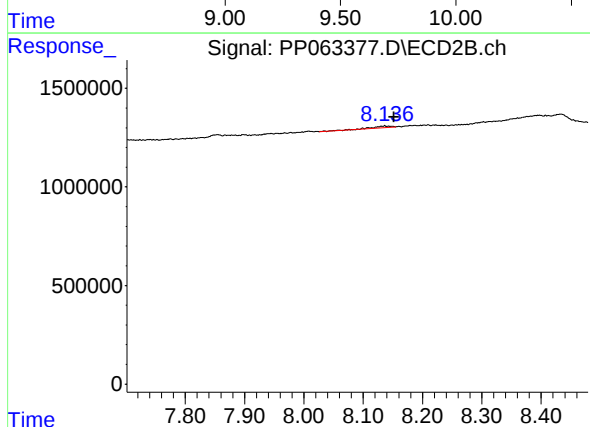


#40 AR-1262-5

R.T.: 8.136 min
Delta R.T.: -0.015 min
Response: 174359
Conc: 2.14 ng/ml

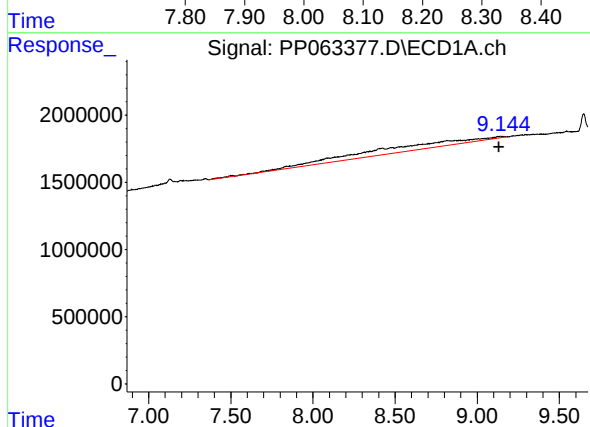


#43 AR-1268-3

R.T.: 9.142 min
Delta R.T.: 0.011 min
Response: 23735815
Conc: 99.57 ng/ml

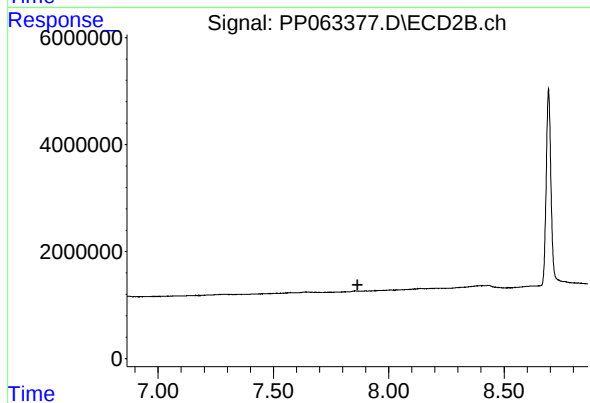

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 7.864 min
Response: 0
Conc: N.D.

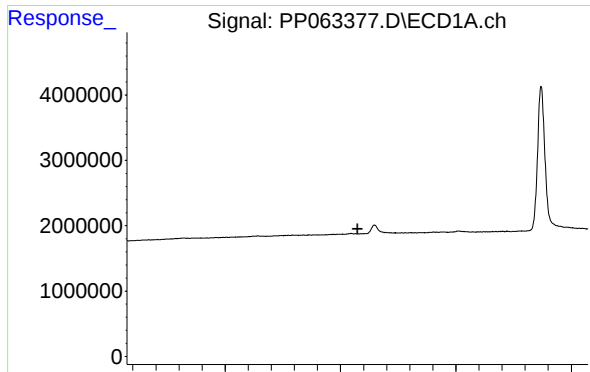

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB159224BL

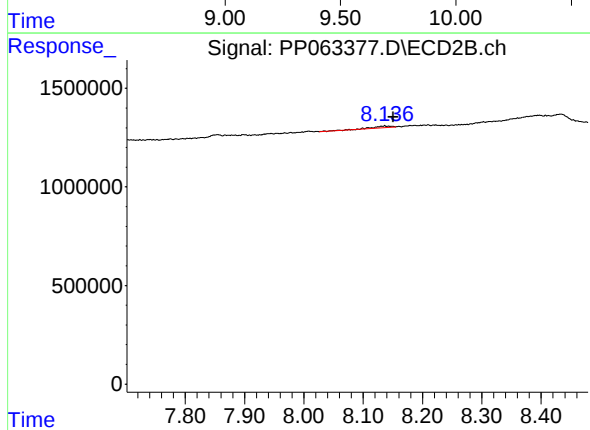

#44 AR-1268-4

R.T.: 8.136 min
Delta R.T.: -0.015 min
Response: 174359
Conc: 1.99 ng/ml