

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022324\
 Data File : PP063347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Feb 2024 10:03
 Operator : YP\AJ
 Sample : P1540-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-1325RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/26/2024
 Supervised By :Ankita Jodhani 02/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 23 12:17:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 05 12:13:11 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.644	28859886	25266597	12.065	10.630
2) SA Decachlor...	10.370	8.693	13132367	13514300	5.840m	5.456

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022324\
Data File : PP063347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Feb 2024 10:03
Operator : YP\AJ
Sample : P1540-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-1325RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/26/2024
Supervised By :Ankita Jodhani 02/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 23 12:17:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP020124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 05 12:13:11 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

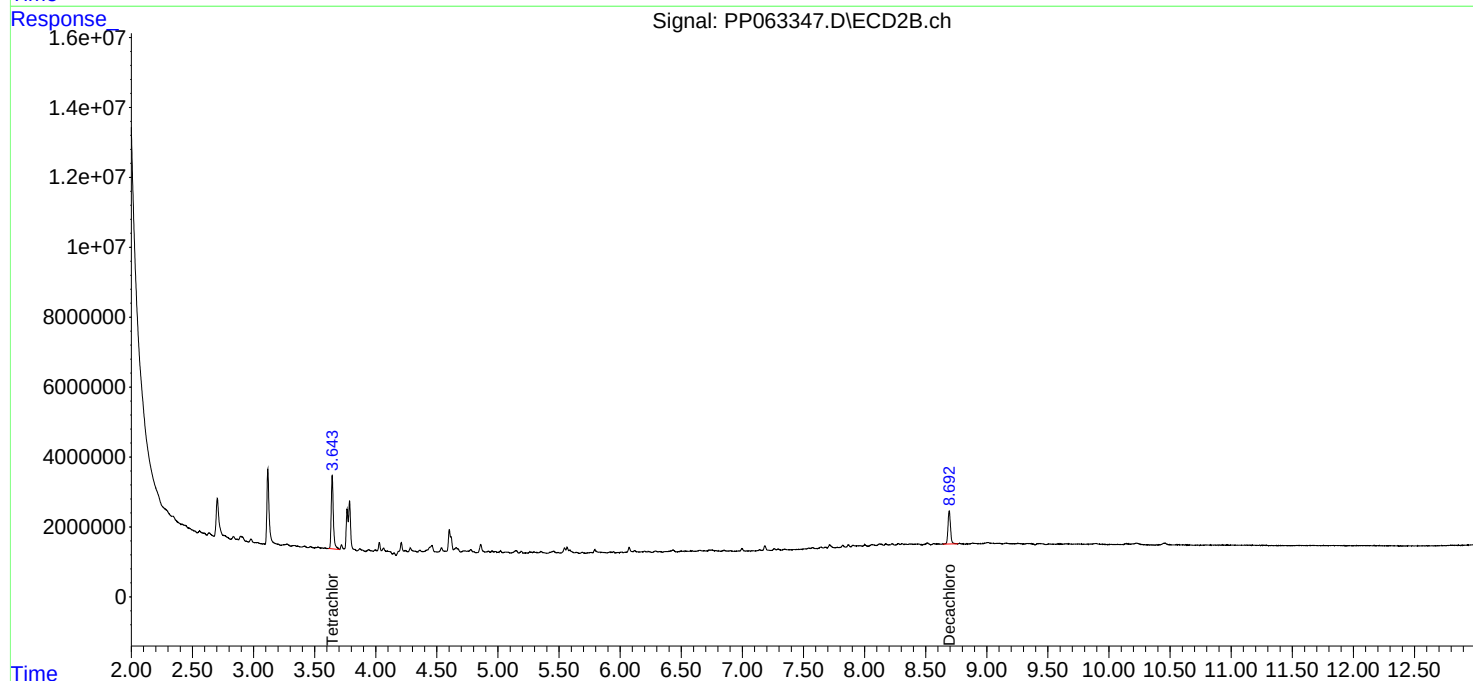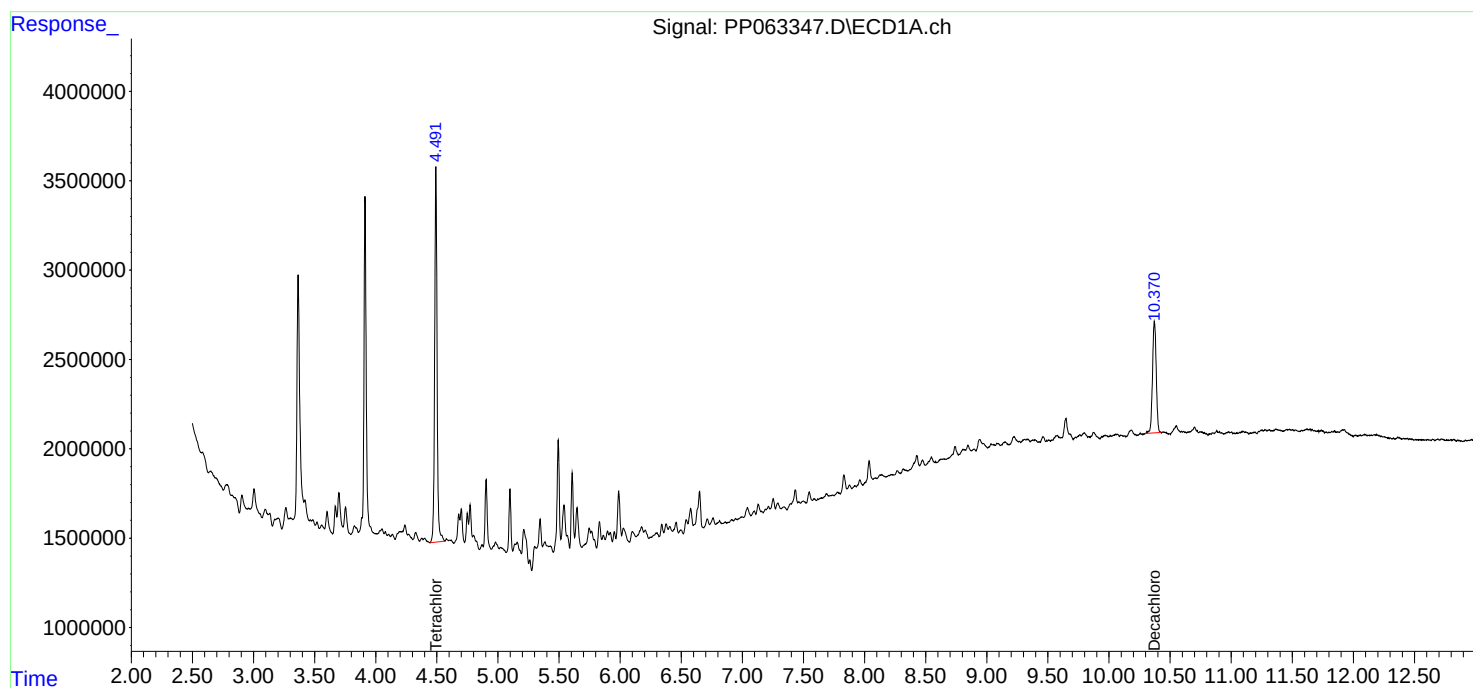

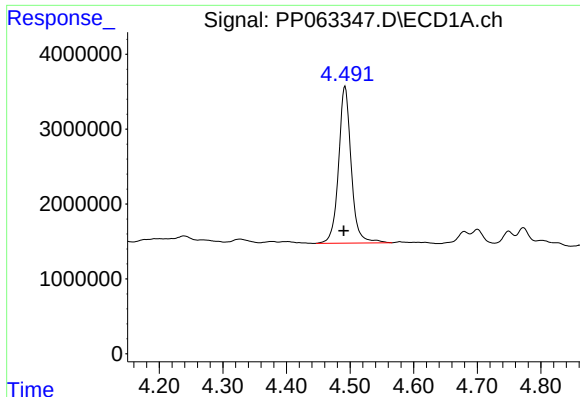


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.002 min
Response: 28859886
Conc: 12.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-1325RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/26/2024
Supervised By :Ankita Jodhani 02/26/2024

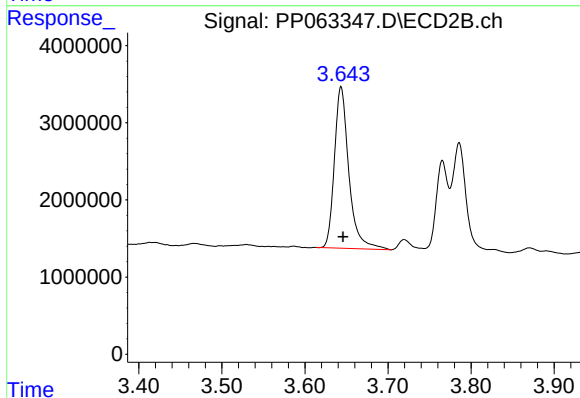


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 25266597
Conc: 10.63 ng/ml

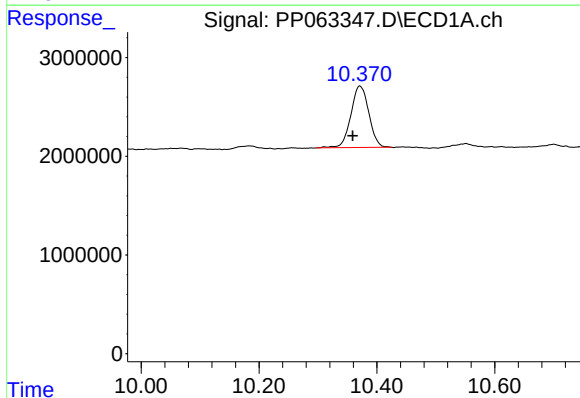

#2 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: 0.011 min
Response: 13132367
Conc: 5.84 ng/ml m

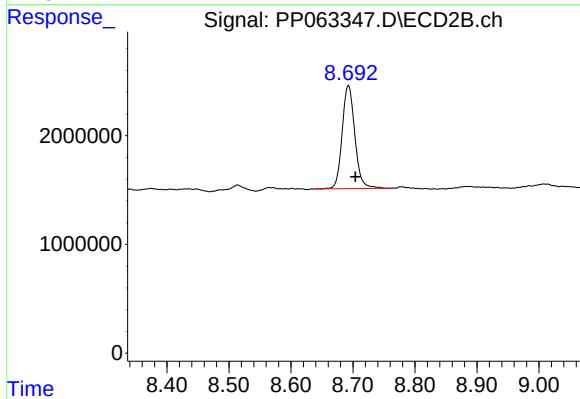

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: -0.011 min
Response: 13514300
Conc: 5.46 ng/ml