

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022421\
 Data File : PP033539.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Feb 2021 15:33
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 17:36:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	#
28) L6 AR-1254-3	7.550f	0.000	6842	0	2.242	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022421\
Data File : PP033539.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Feb 2021 15:33
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 17:36:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

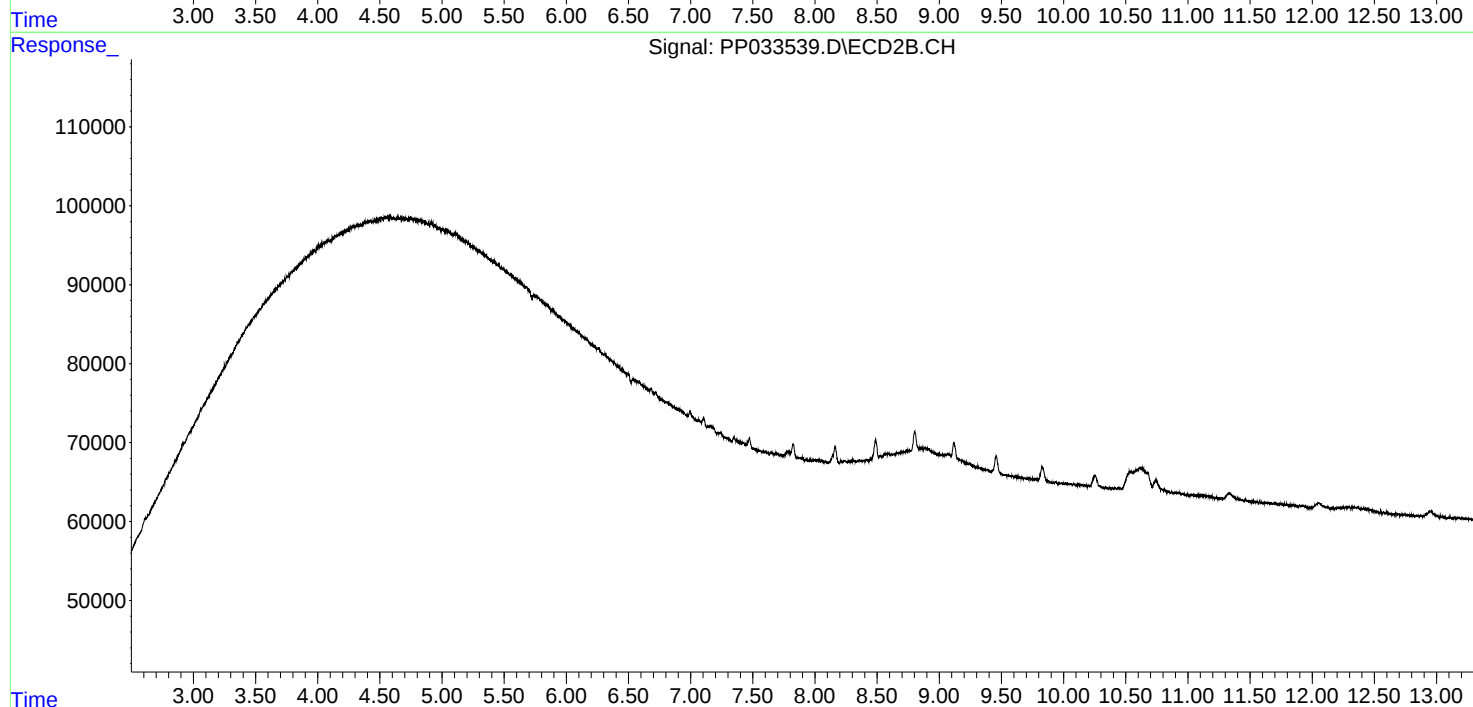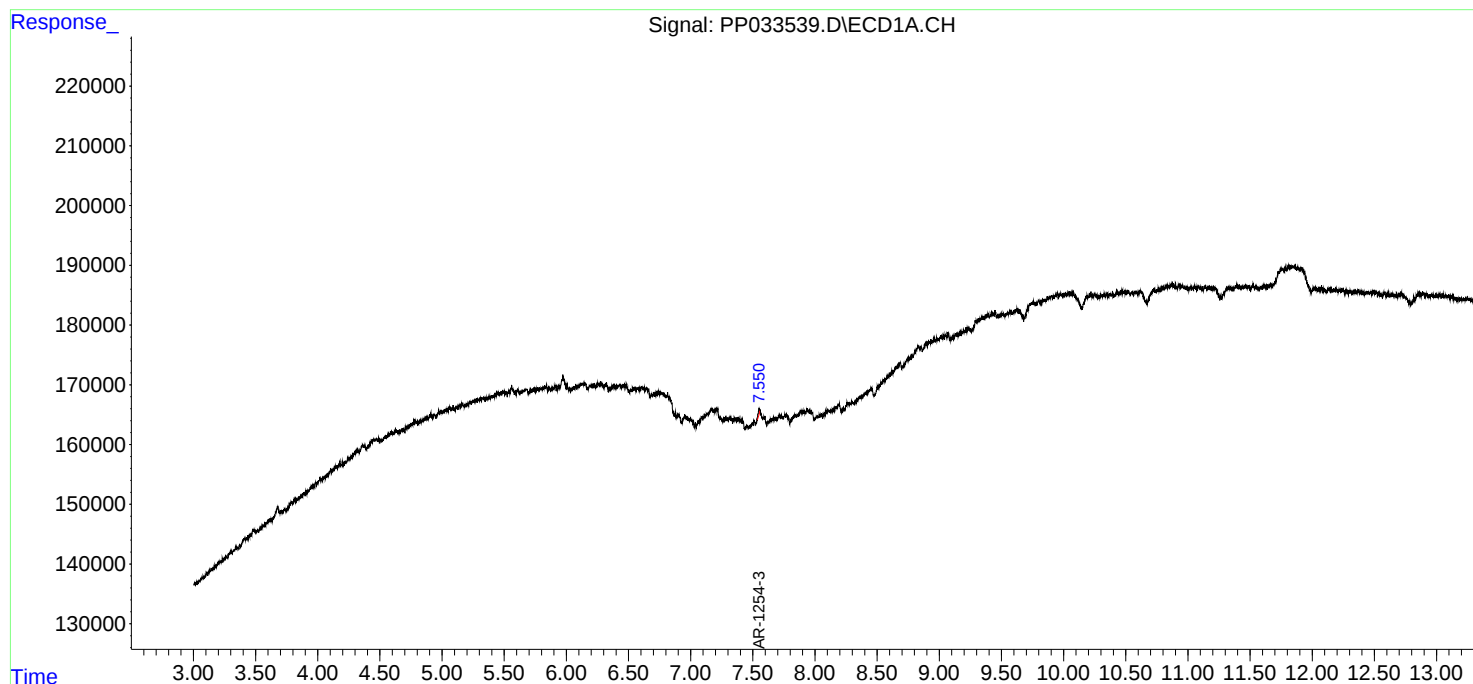


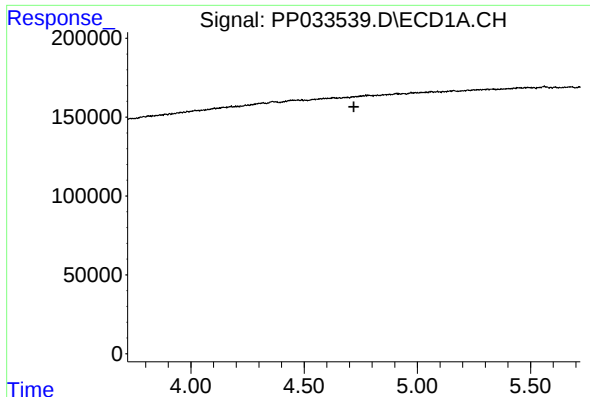

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.720 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

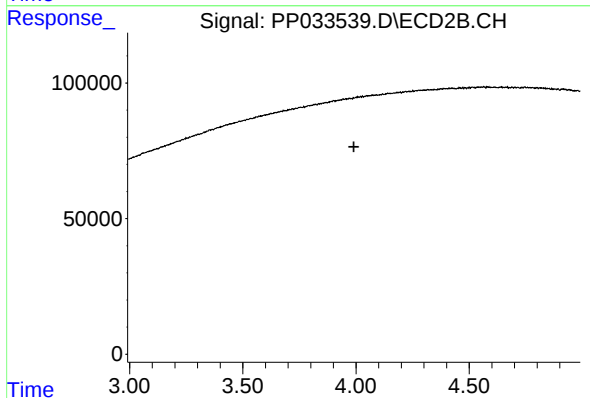


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.990 min
Response: 0
Conc: N.D.

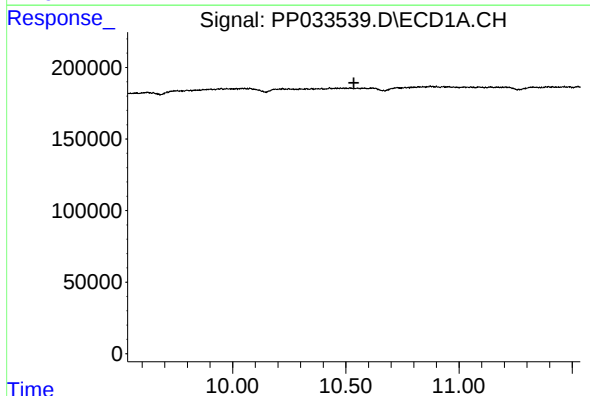


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.536 min
Response: 0
Conc: N.D.

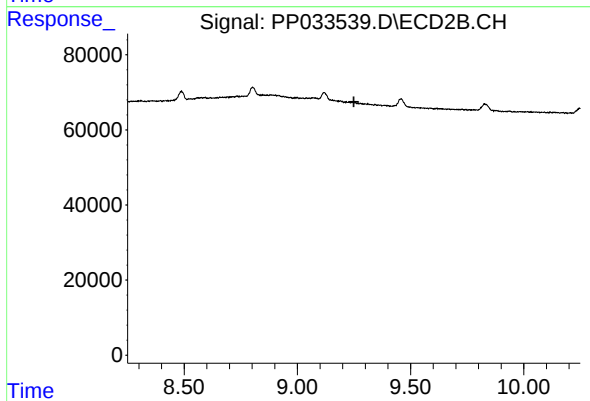

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 9.250 min
Response: 0
Conc: N.D.

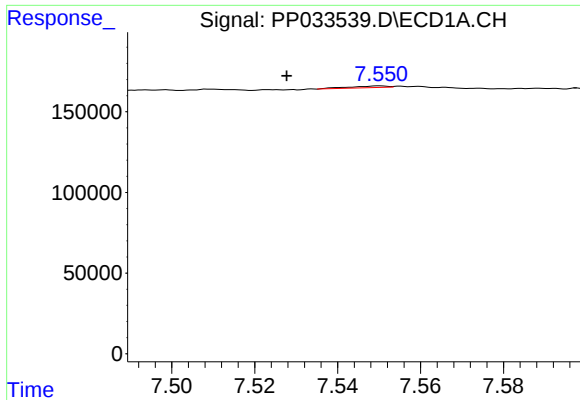

#28 AR-1254-3

R.T.: 7.550 min
Delta R.T.: 0.022 min
Response: 6842
Conc: 2.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

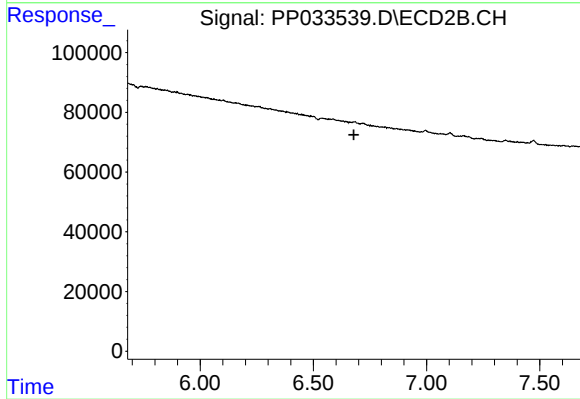

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.679 min
Response: 0
Conc: N.D.