

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022421\
 Data File : PP033546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Feb 2021 17:29
 Operator : DD\AJ
 Sample : M1470-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CBH-591

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 17:51:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.721	3.993	1495577	832213	20.320	18.897
2)	SA Decachlor...	10.537	9.251	822829	576304	17.691	18.239
Target Compounds							
8)	L2 AR-1221-1	4.963	0.000	76250	0	113.137	N.D. #
9)	L2 AR-1221-2	5.067	0.000	15767	0	30.995	N.D. #
32)	L7 AR-1260-2	7.935f	0.000	6579	0	2.067	N.D. #
34)	L7 AR-1260-4	8.560	0.000	3481	0	1.334	N.D. #
35)	L7 AR-1260-5	8.837f	0.000	5620	0	0.952	N.D. #
37)	L8 AR-1262-2	8.837f	0.000	5620	0	0.915	N.D. #
40)	L8 AR-1262-5	0.000	8.762f	0	11857	N.D.	9.899 #
44)	L9 AR-1268-4	0.000	8.762f	0	11857	N.D.	8.595 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022421\
Data File : PP033546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Feb 2021 17:29
Operator : DD\AJ
Sample : M1470-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CBH-591

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 17:51:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

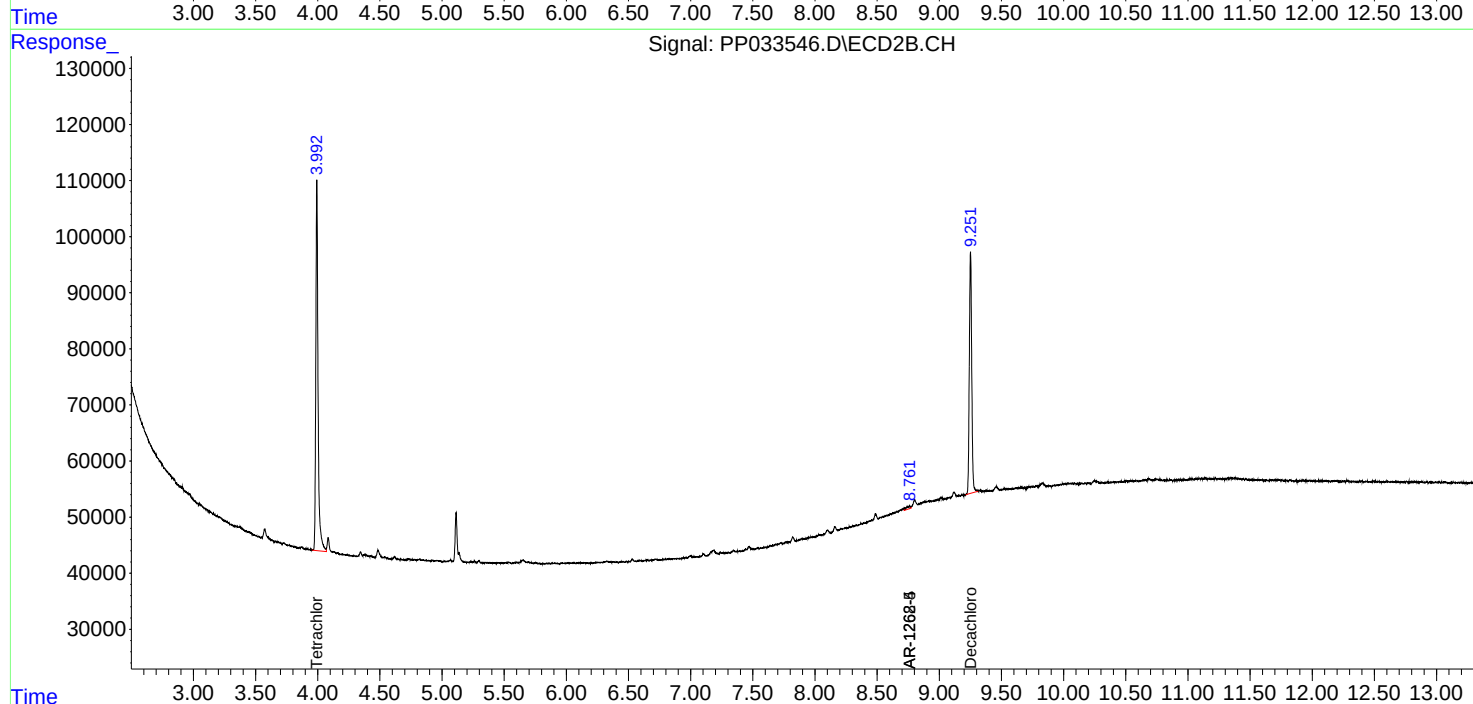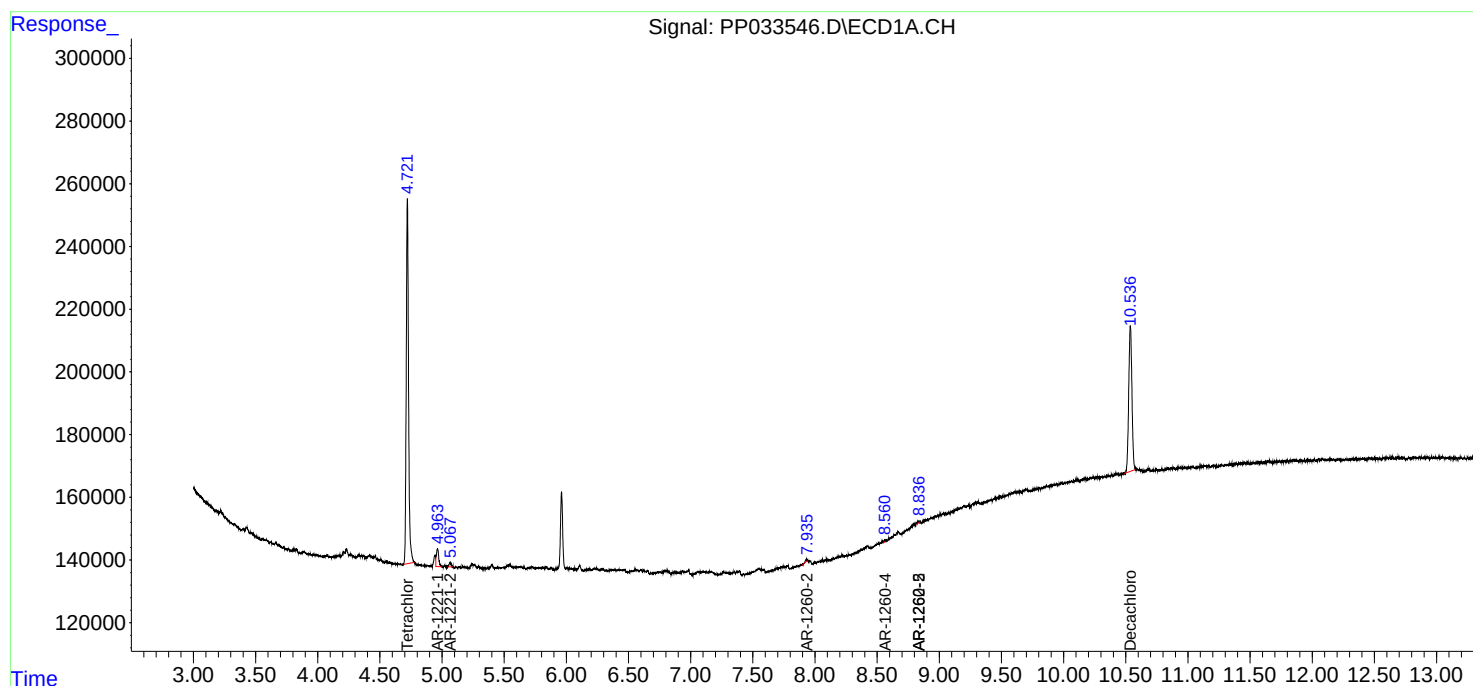


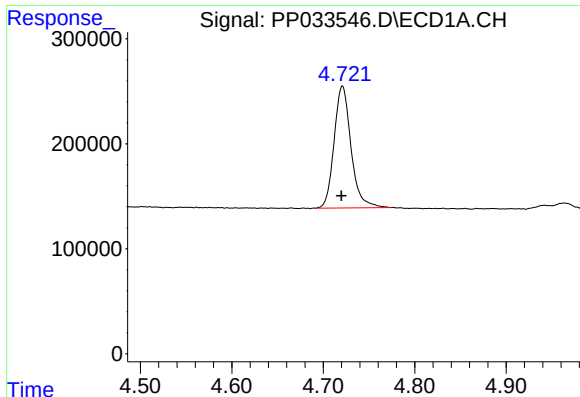

#1 Tetrachloro-m-xylene


R.T.: 4.721 min
Delta R.T.: 0.001 min
Response: 1495577
Conc: 20.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
CBH-591

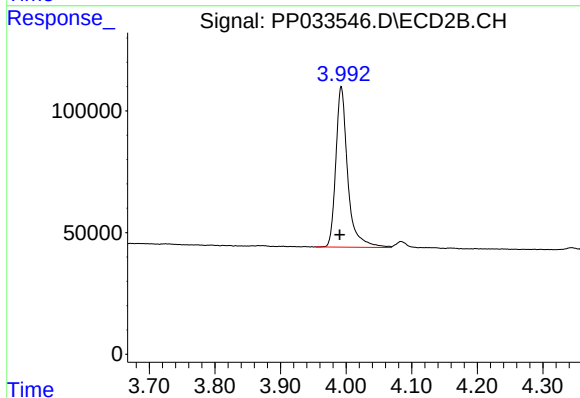


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.002 min
Response: 832213
Conc: 18.90 ng/ml

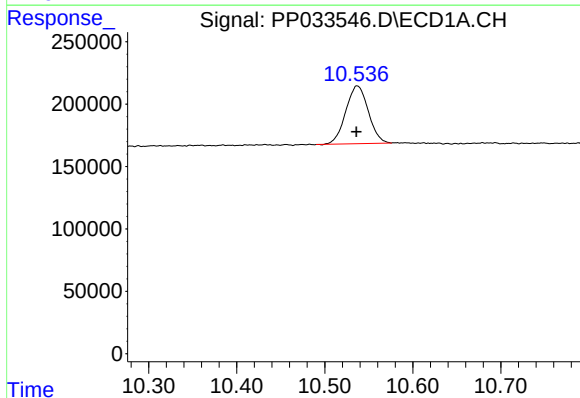


#2 Decachlorobiphenyl

R.T.: 10.537 min
Delta R.T.: 0.000 min
Response: 822829
Conc: 17.69 ng/ml

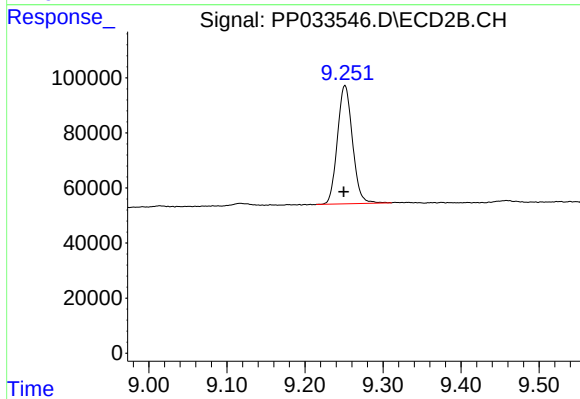

#2 Decachlorobiphenyl


R.T.: 9.251 min
Delta R.T.: 0.002 min
Response: 576304
Conc: 18.24 ng/ml

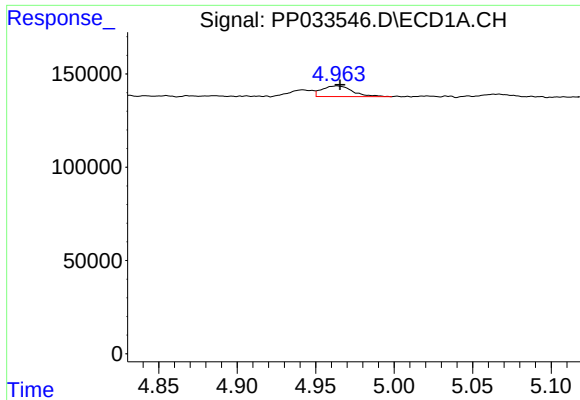

#8 AR-1221-1


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 76250
Conc: 113.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
CBH-591

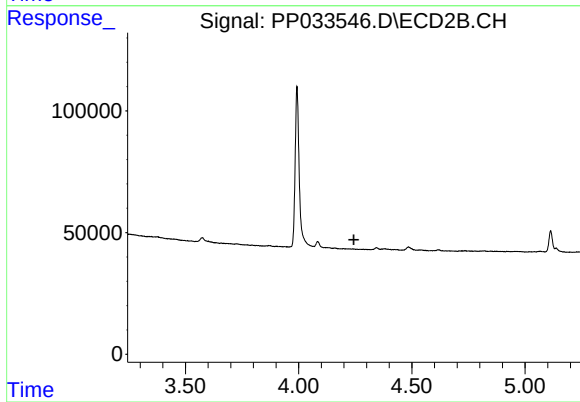


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.244 min
Response: 0
Conc: N.D.

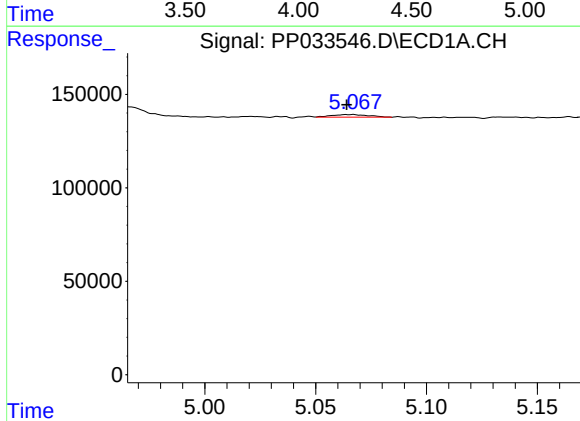


#9 AR-1221-2

R.T.: 5.067 min
Delta R.T.: 0.003 min
Response: 15767
Conc: 31.00 ng/ml

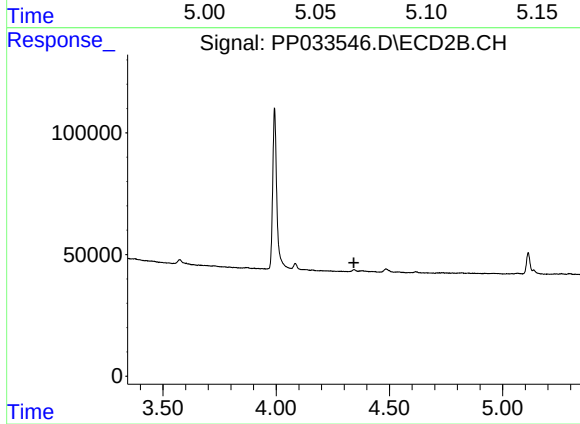

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

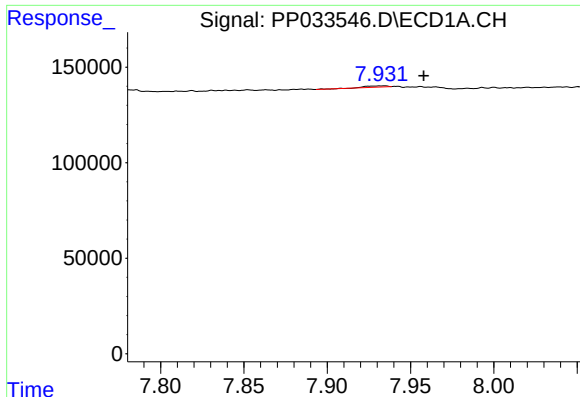

#32 AR-1260-2


R.T.: 7.935 min
Delta R.T.: -0.023 min
Response: 6579
Conc: 2.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
CBH-591

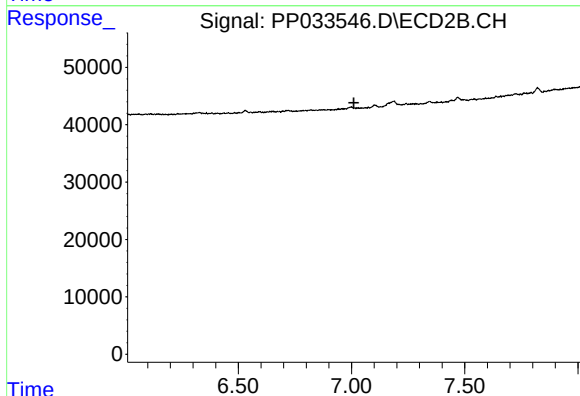


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.010 min
Response: 0
Conc: N.D.

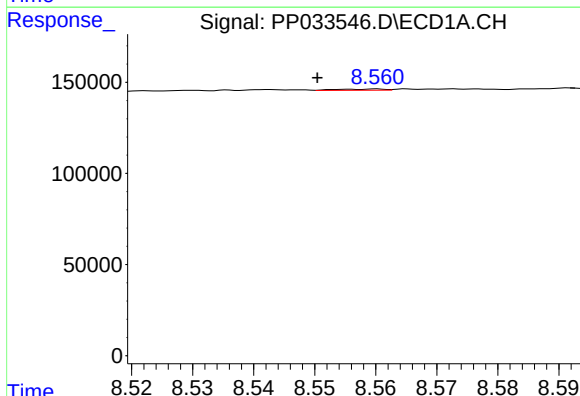


#34 AR-1260-4

R.T.: 8.560 min
Delta R.T.: 0.010 min
Response: 3481
Conc: 1.33 ng/ml

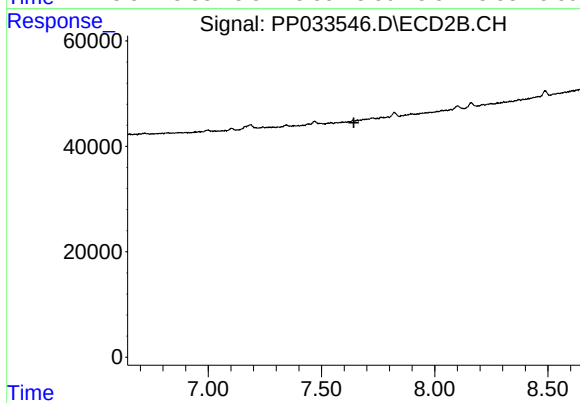

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.643 min
Response: 0
Conc: N.D.

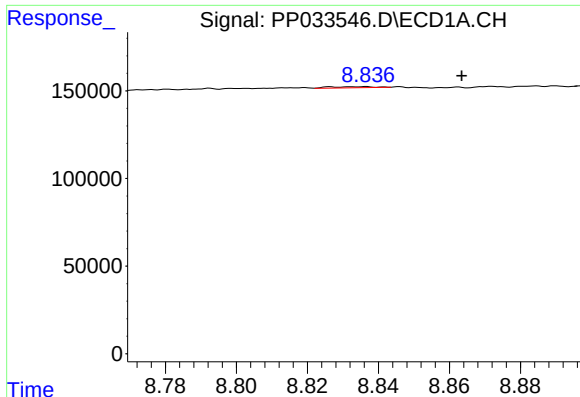

#35 AR-1260-5


R.T.: 8.837 min
Delta R.T.: -0.027 min
Response: 5620
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
CBH-591

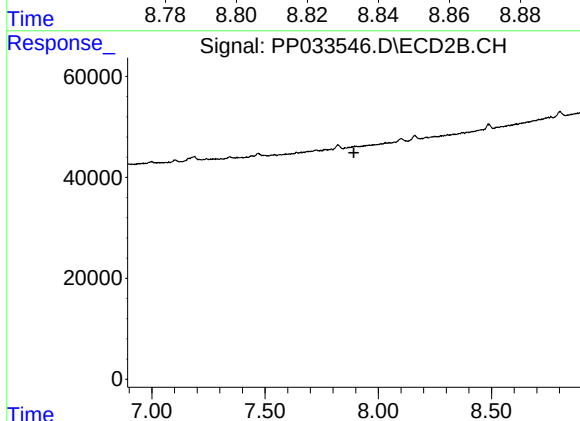


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.

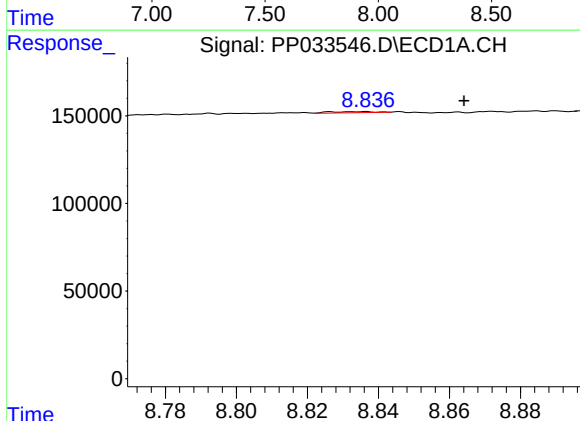


#37 AR-1262-2

R.T.: 8.837 min
Delta R.T.: -0.027 min
Response: 5620
Conc: 0.92 ng/ml

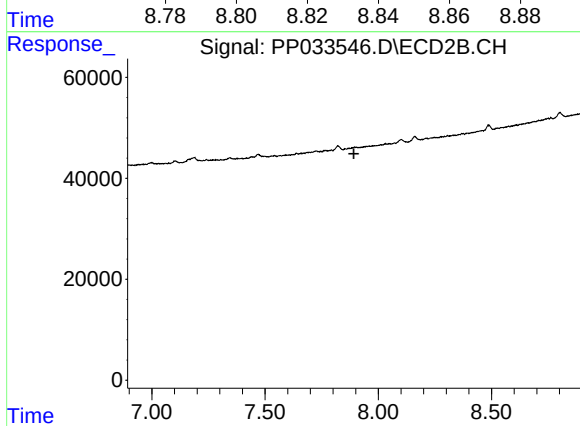

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.

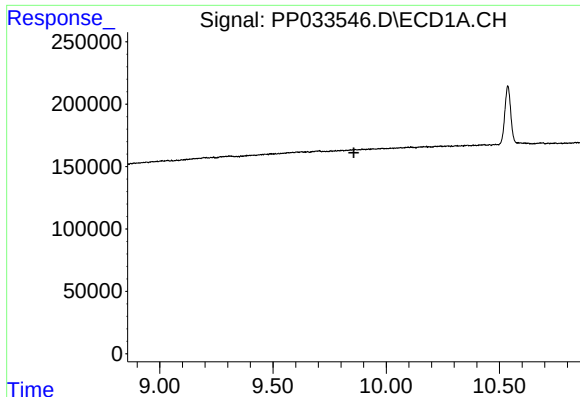

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.857 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CBH-591

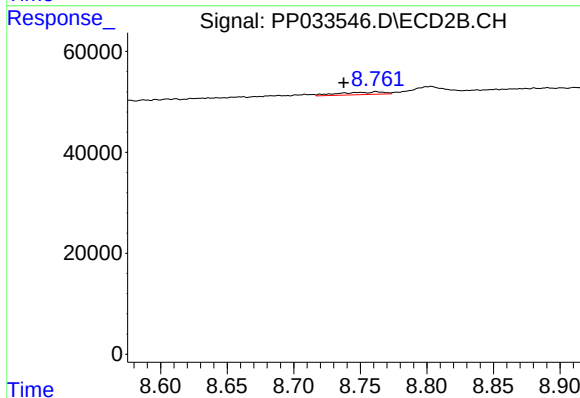


#40 AR-1262-5

R.T.: 8.762 min
Delta R.T.: 0.024 min
Response: 11857
Conc: 9.90 ng/ml

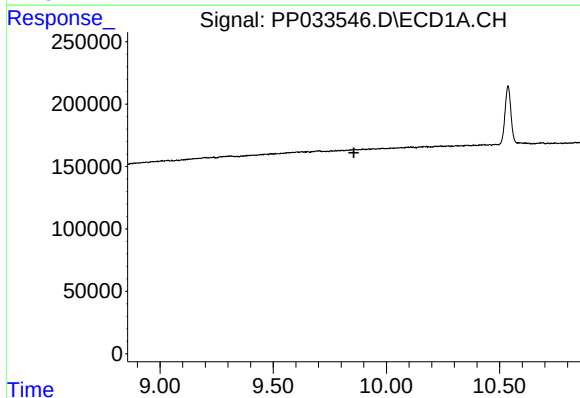

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.856 min
Response: 0
Conc: N.D.

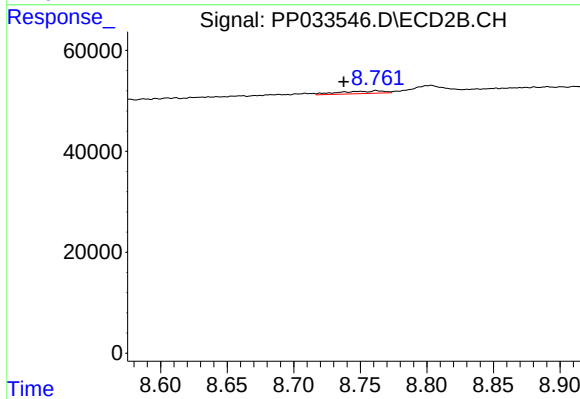

#44 AR-1268-4

R.T.: 8.762 min
Delta R.T.: 0.024 min
Response: 11857
Conc: 8.60 ng/ml