

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022422\
 Data File : PP043984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 21:59
 Operator : YP\AJ
 Sample : N1642-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 31453-58

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/25/2022
 Supervised By :Ankita Jodhani 02/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:44:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.917	3.173	31161011	29753788	14.093	15.841m
2) SA Decachlor...	10.058	8.543	17777785	22750723	14.966	14.023

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022422\
Data File : PP043984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 21:59
Operator : YP\AJ
Sample : N1642-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
31453-58


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/25/2022
Supervised By :Ankita Jodhani 02/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:44:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

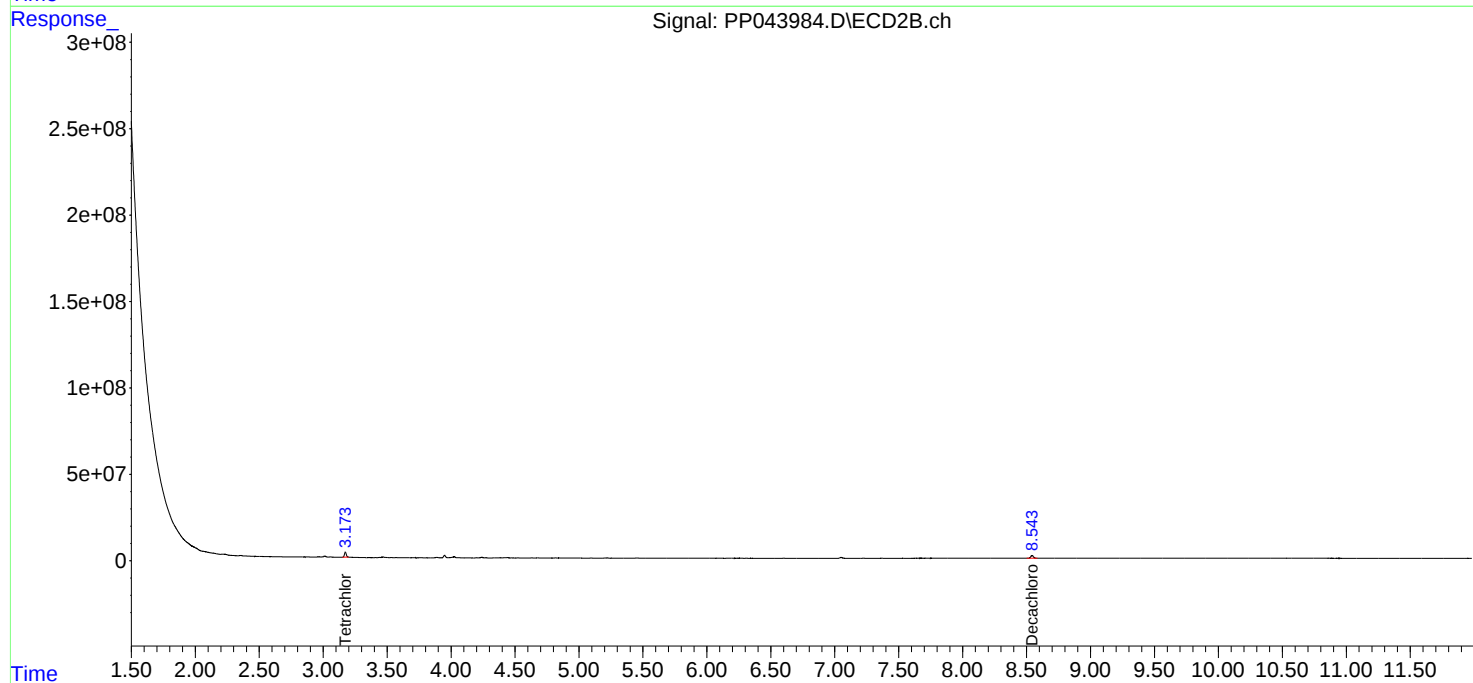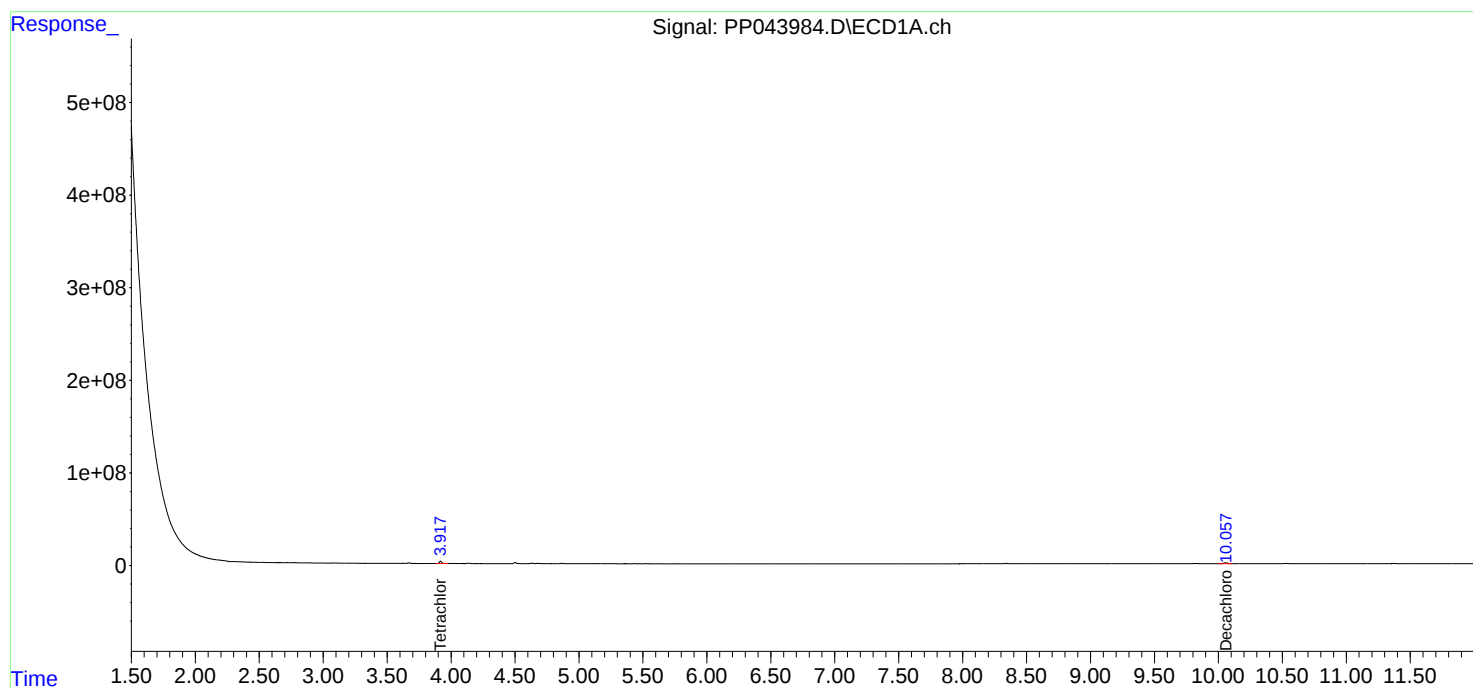

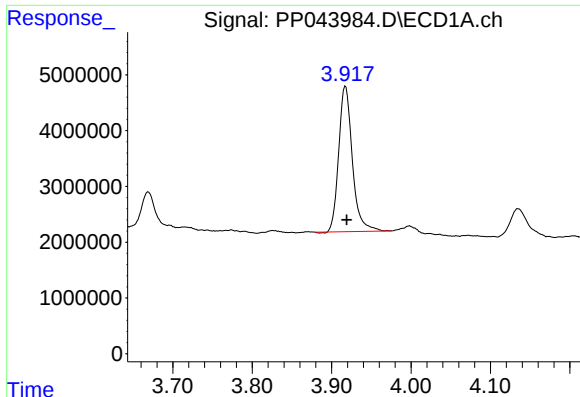


#1 Tetrachloro-m-xylene

R.T.: 3.917 min
Delta R.T.: -0.002 min
Response: 31161011
Conc: 14.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
31453-58


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/25/2022
Supervised By :Ankita Jodhani 02/25/2022

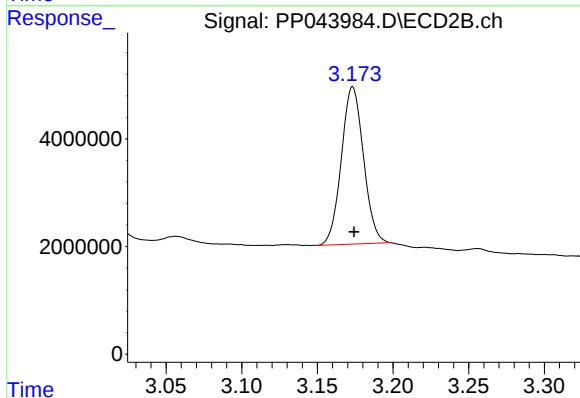


#1 Tetrachloro-m-xylene

R.T.: 3.173 min
Delta R.T.: -0.001 min
Response: 29753788
Conc: 15.84 ng/ml m

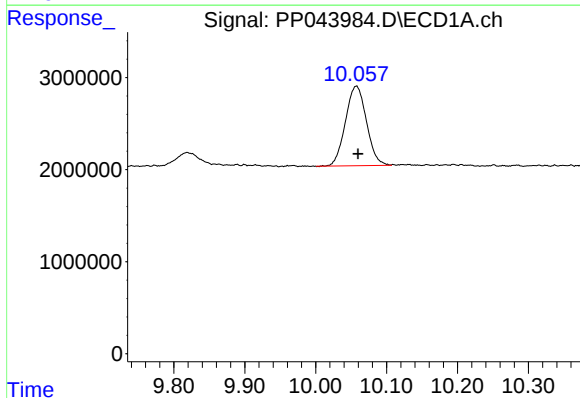

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: -0.002 min
Response: 17777785
Conc: 14.97 ng/ml

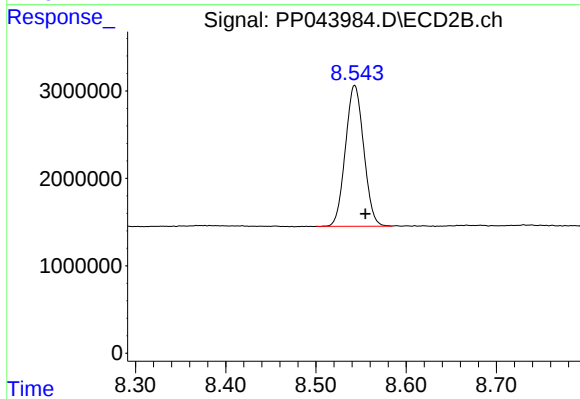

#2 Decachlorobiphenyl

R.T.: 8.543 min
Delta R.T.: -0.012 min
Response: 22750723
Conc: 14.02 ng/ml