

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022423\
 Data File : PP055981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2023 05:49
 Operator : YP\AJ
 Sample : 01670-03 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZZ207Y-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/27/2023
 Supervised By :Ankita Jodhani 02/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 08:02:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.564	2078594	1655611	1.290	1.134
2) SA Decachlor...	10.061	8.564	3530614	1708201	1.731m	1.506

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022423\
Data File : PP055981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2023 05:49
Operator : YP\AJ
Sample : 01670-03 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZZ207Y-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2023
Supervised By :Ankita Jodhani 02/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 08:02:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

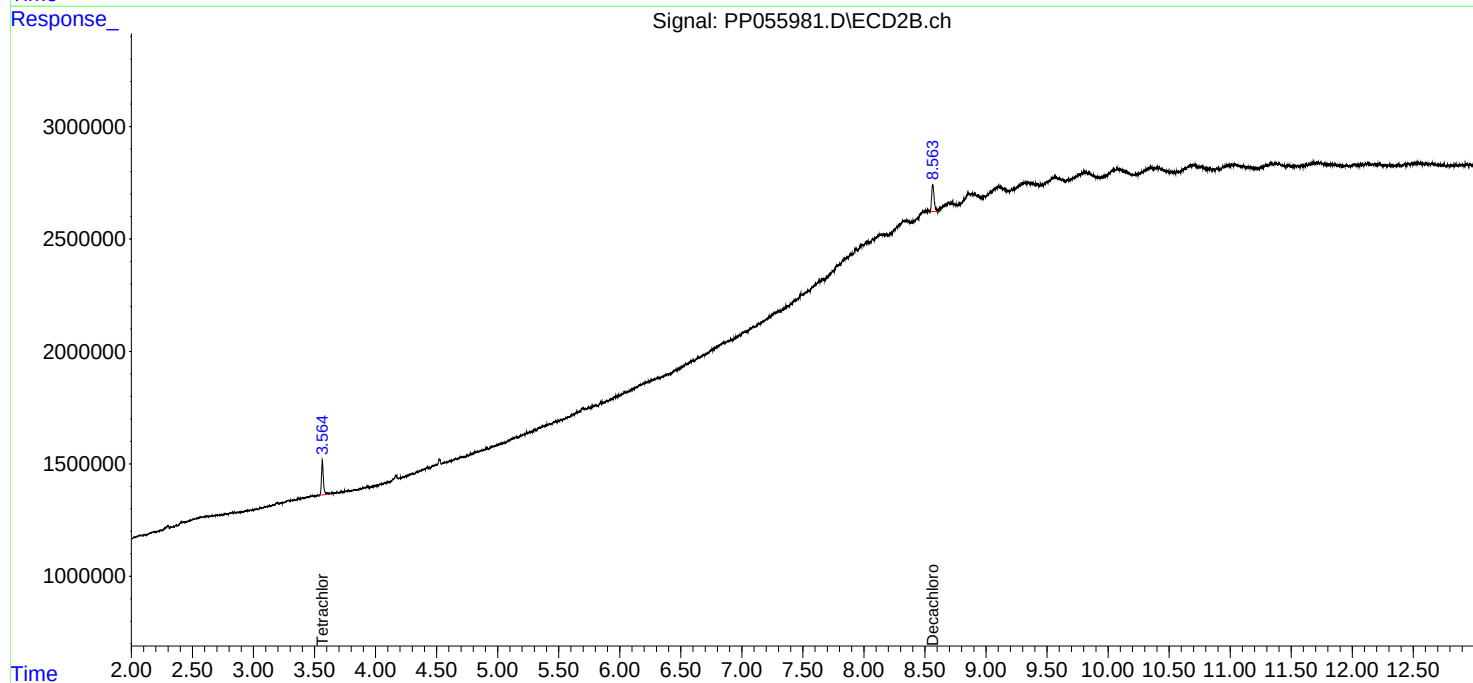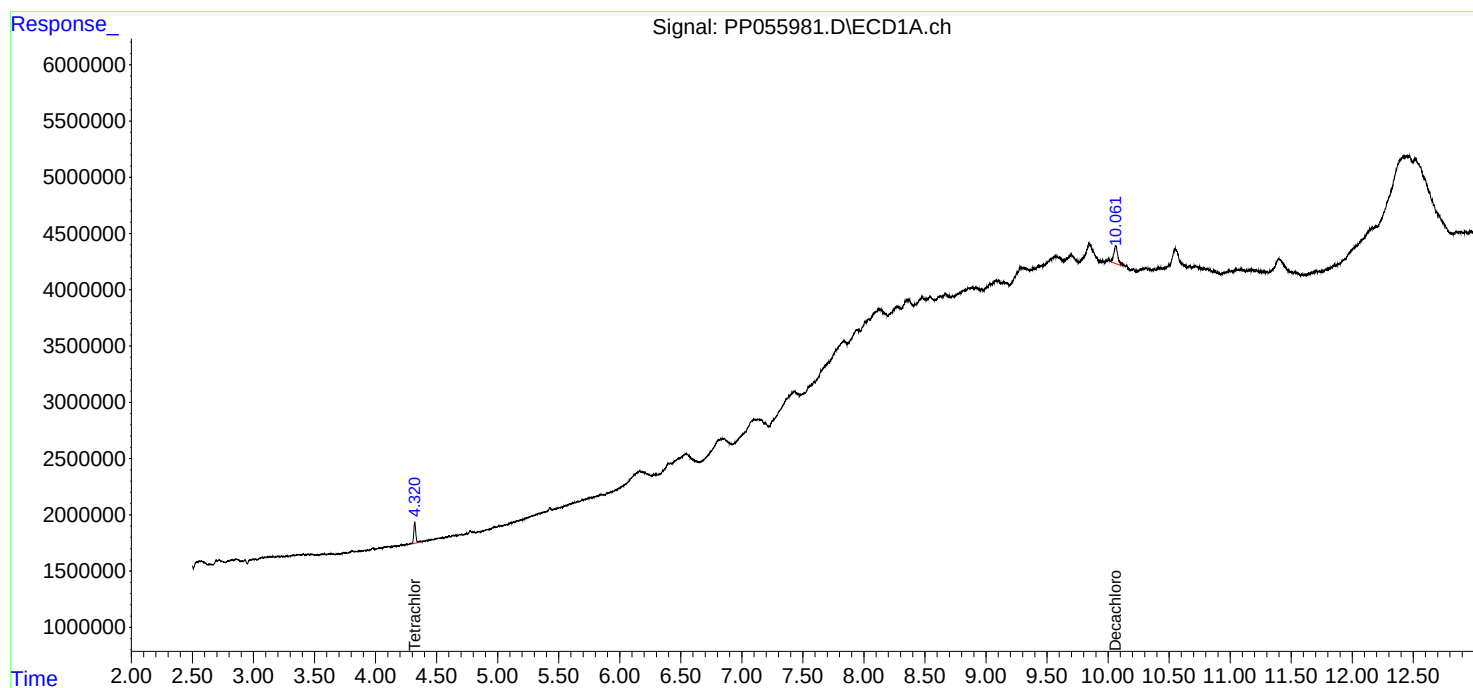

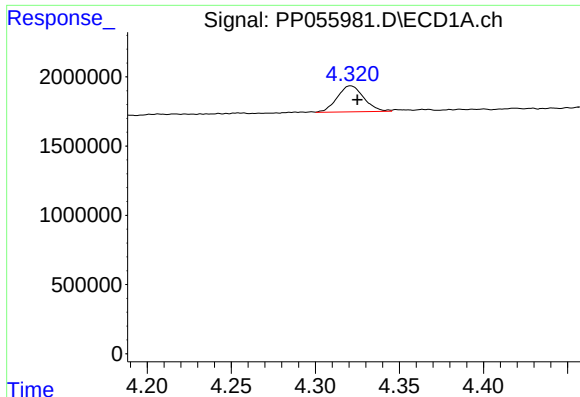


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: -0.004 min
Response: 2078594
Conc: 1.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ207Y-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2023
Supervised By :Ankita Jodhani 02/27/2023

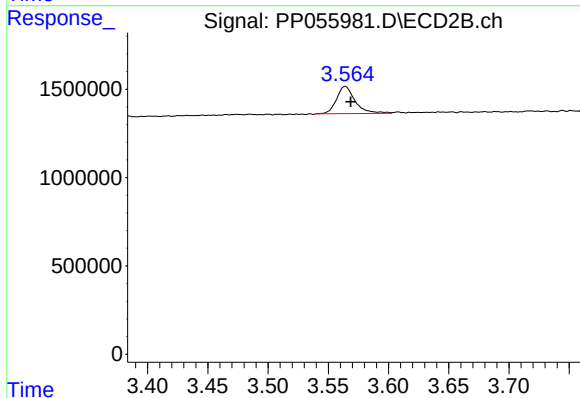


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.005 min
Response: 1655611
Conc: 1.13 ng/ml

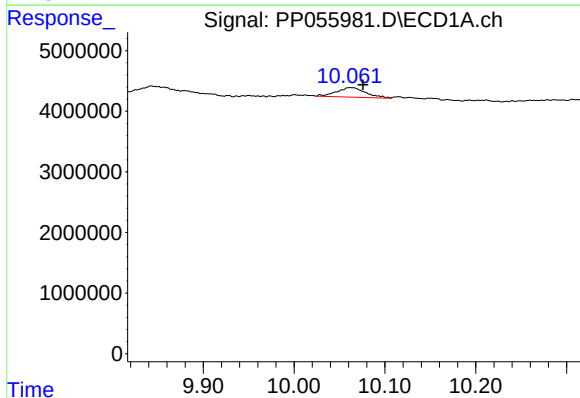

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: -0.015 min
Response: 3530614
Conc: 1.73 ng/ml m

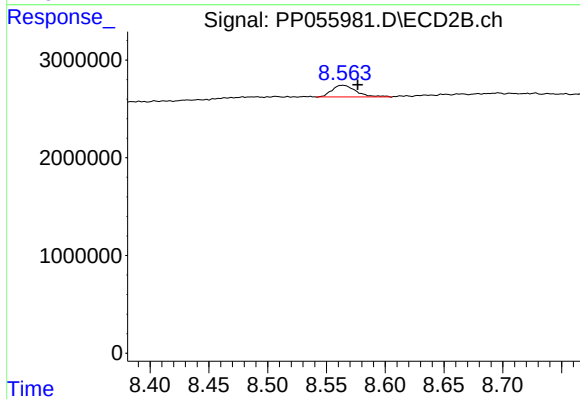

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.013 min
Response: 1708201
Conc: 1.51 ng/ml