

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 12:47
 Operator : DD\AJ
 Sample : PB134812BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 13:19:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.719	3.990	1556508	865641	21.148	19.656
2)	SA Decachlor...	10.531	9.245	1045185	732805	22.472	23.192
Target Compounds							
9)	L2 AR-1221-2	5.065	0.000	19671	0	38.670	N.D. #
32)	L7 AR-1260-2	7.932f	0.000	3588	0	1.127	N.D. #
34)	L7 AR-1260-4	8.574f	0.000	4579	0	1.755	N.D. #
35)	L7 AR-1260-5	8.862	0.000	25366	0	4.295	N.D. #
37)	L8 AR-1262-2	8.862	0.000	25366	0	4.130	N.D. #
38)	L8 AR-1262-3	0.000	8.155f	0	19847	N.D.	11.589 #
41)	L9 AR-1268-1	0.000	8.155f	0	19847	N.D.	4.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 12:47
Operator : DD\AJ
Sample : PB134812BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 13:19:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

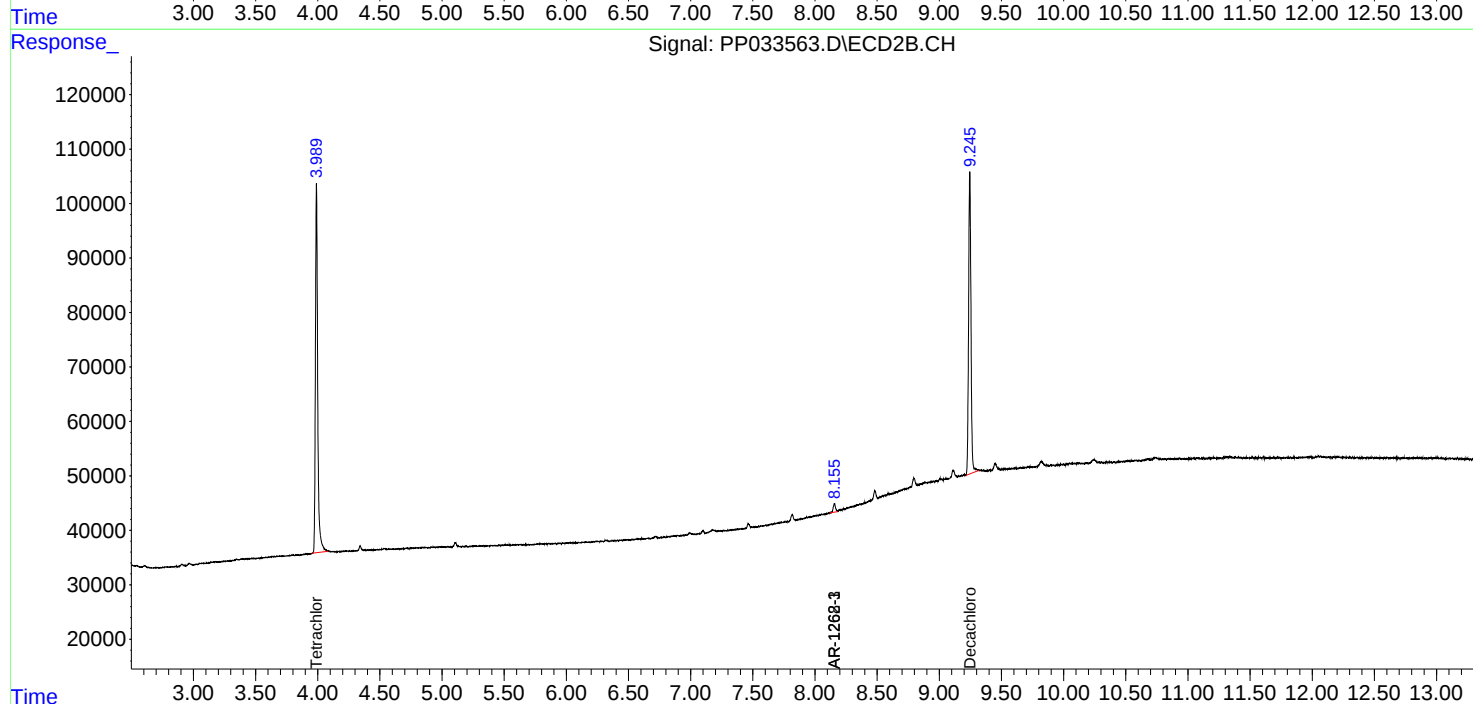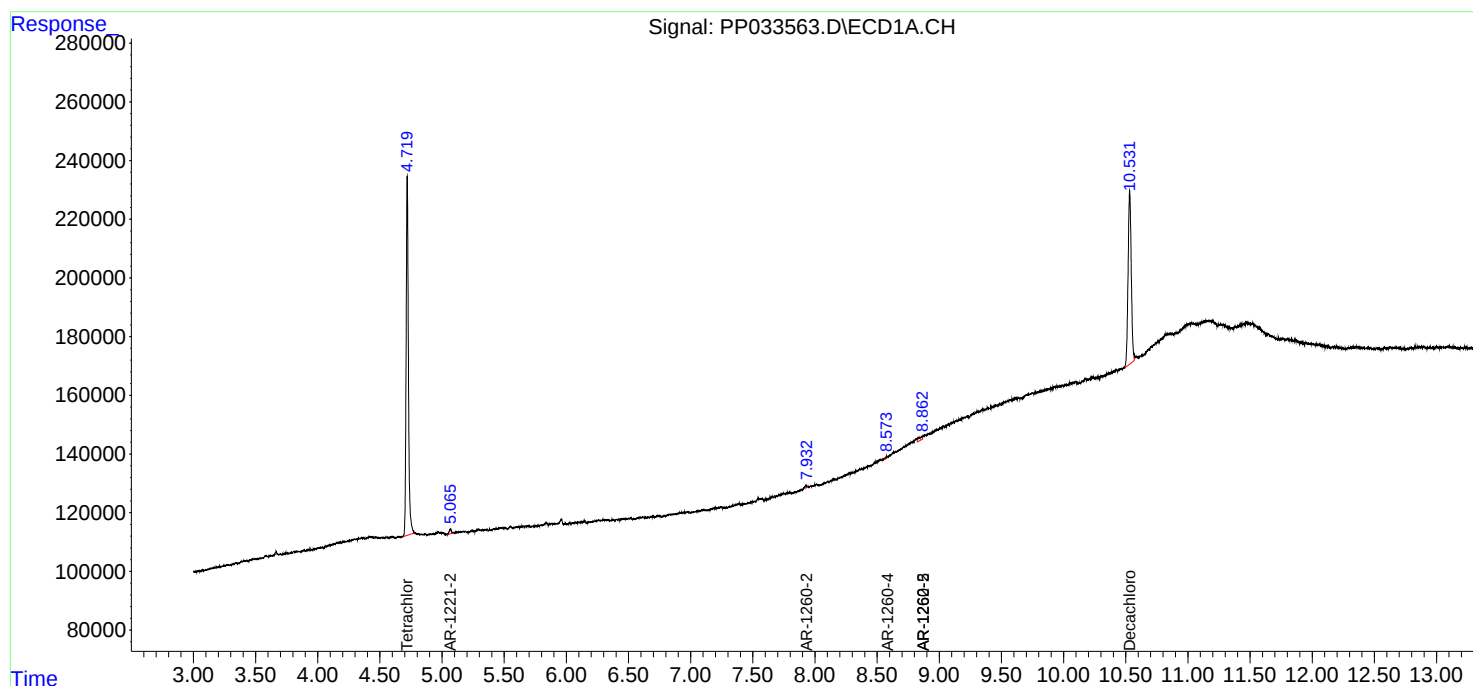


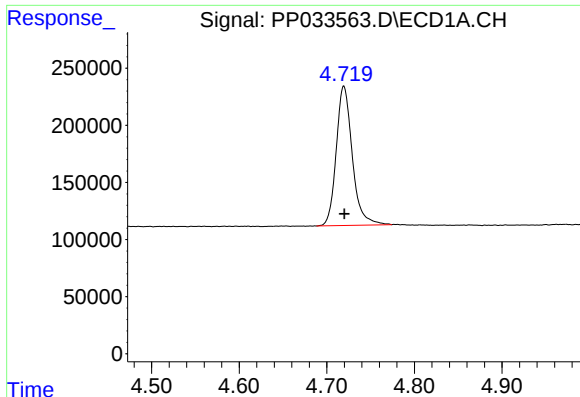

#1 Tetrachloro-m-xylene


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 1556508
Conc: 21.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

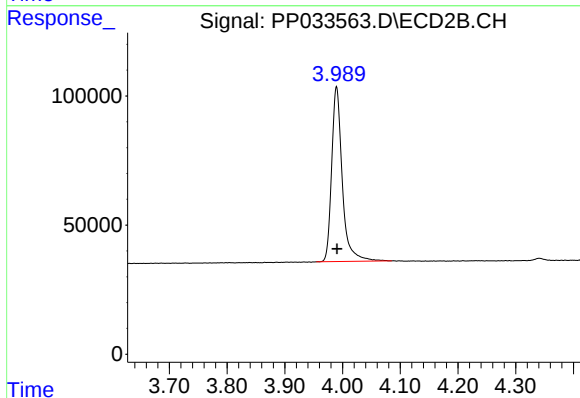


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 865641
Conc: 19.66 ng/ml

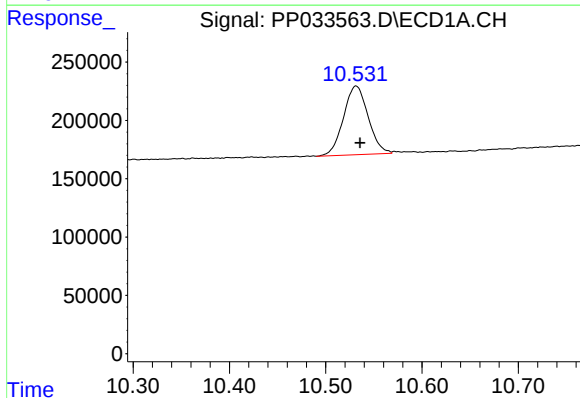


#2 Decachlorobiphenyl

R.T.: 10.531 min
Delta R.T.: -0.004 min
Response: 1045185
Conc: 22.47 ng/ml

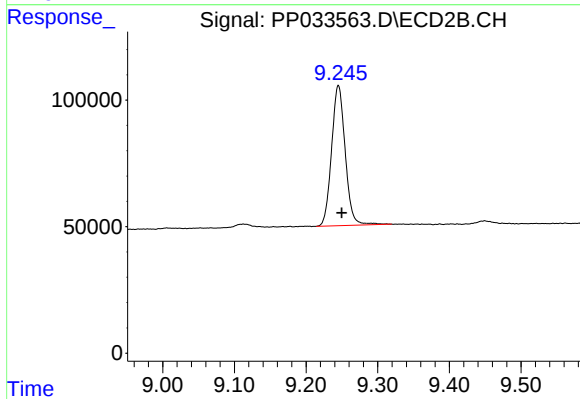

#2 Decachlorobiphenyl


R.T.: 9.245 min
Delta R.T.: -0.005 min
Response: 732805
Conc: 23.19 ng/ml

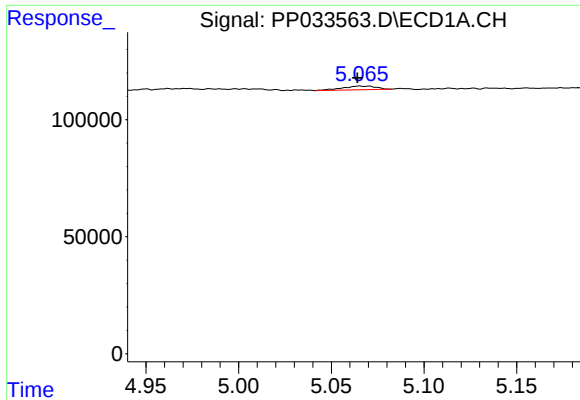

#9 AR-1221-2


R.T.: 5.065 min
Delta R.T.: 0.001 min
Response: 19671
Conc: 38.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

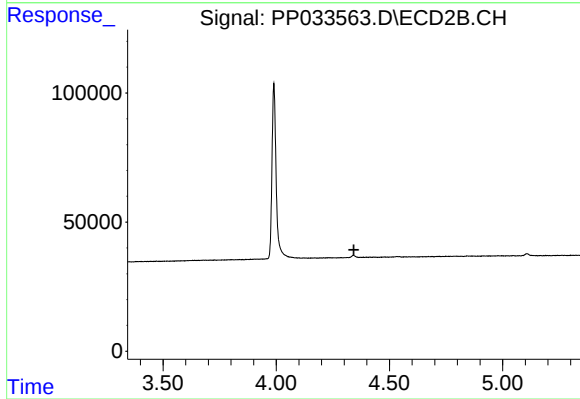


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

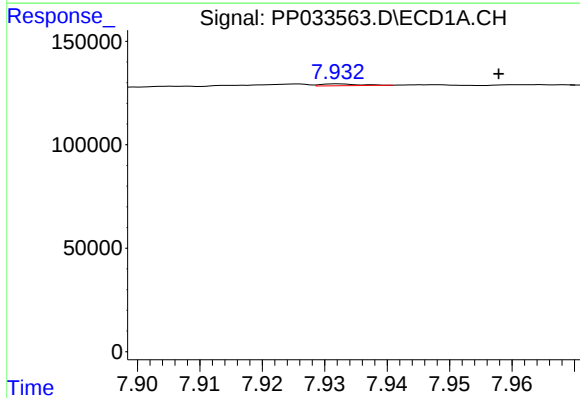


#32 AR-1260-2

R.T.: 7.932 min
Delta R.T.: -0.026 min
Response: 3588
Conc: 1.13 ng/ml

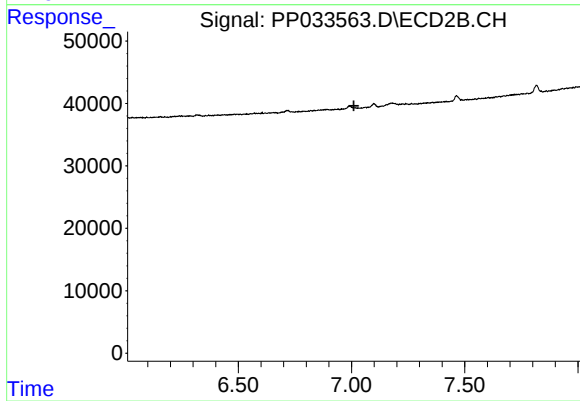

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.010 min
Response: 0
Conc: N.D.

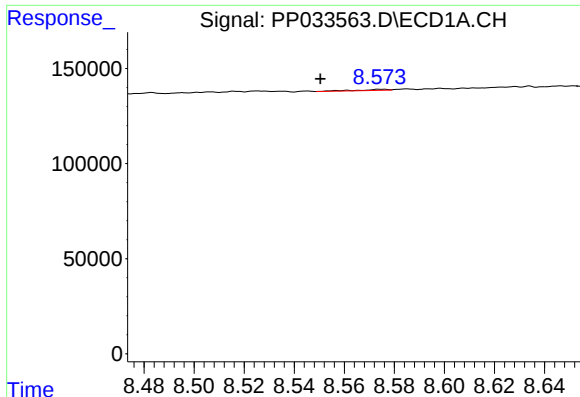

#34 AR-1260-4


R.T.: 8.574 min
Delta R.T.: 0.023 min
Response: 4579
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

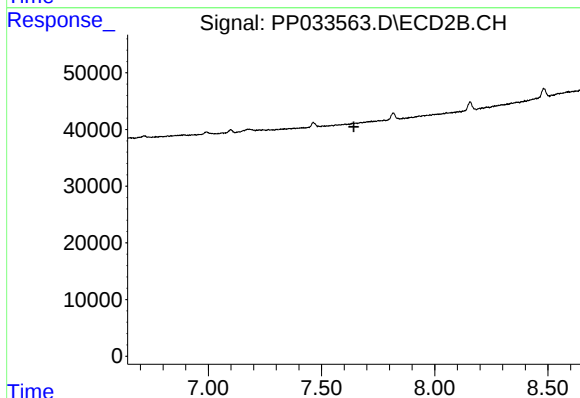


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.643 min
Response: 0
Conc: N.D.

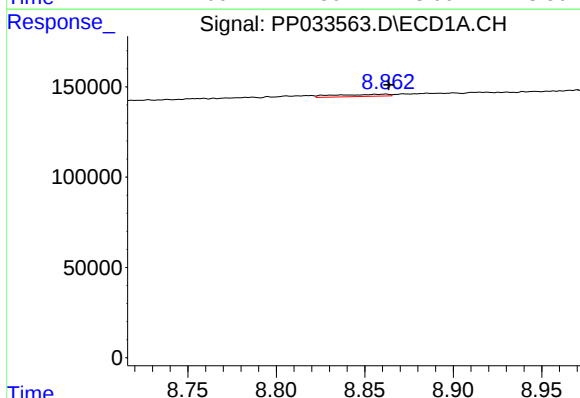


#35 AR-1260-5

R.T.: 8.862 min
Delta R.T.: -0.001 min
Response: 25366
Conc: 4.29 ng/ml

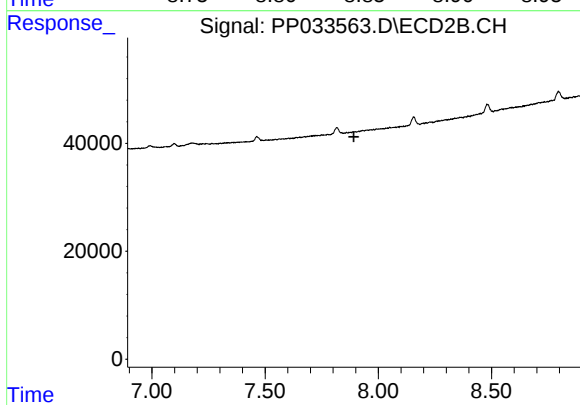

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.

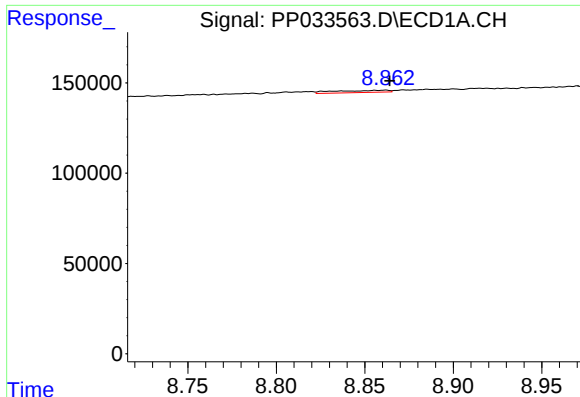

#37 AR-1262-2


R.T.: 8.862 min
Delta R.T.: -0.002 min
Response: 25366
Conc: 4.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

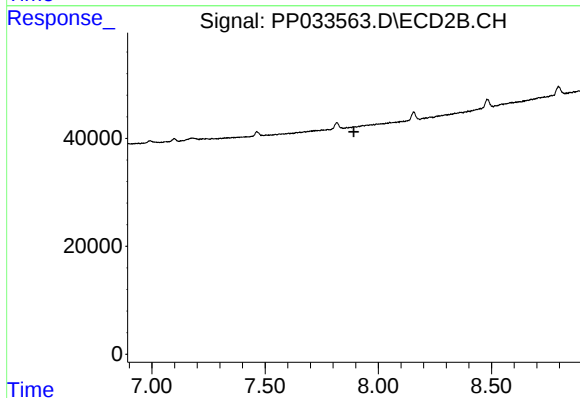


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.

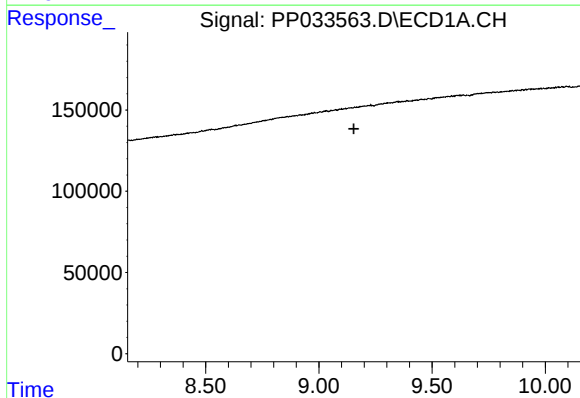


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.154 min
Response: 0
Conc: N.D.

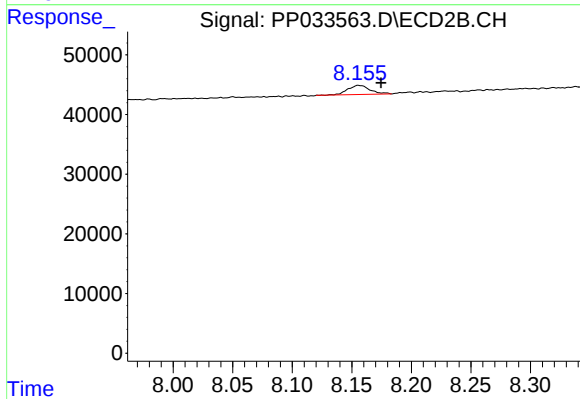

#38 AR-1262-3


R.T.: 8.155 min
Delta R.T.: -0.019 min
Response: 19847
Conc: 11.59 ng/ml

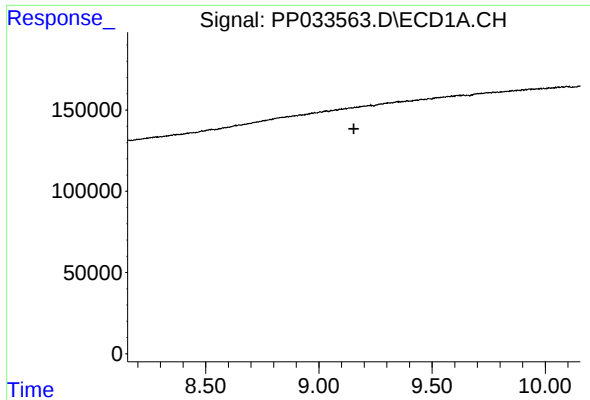

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

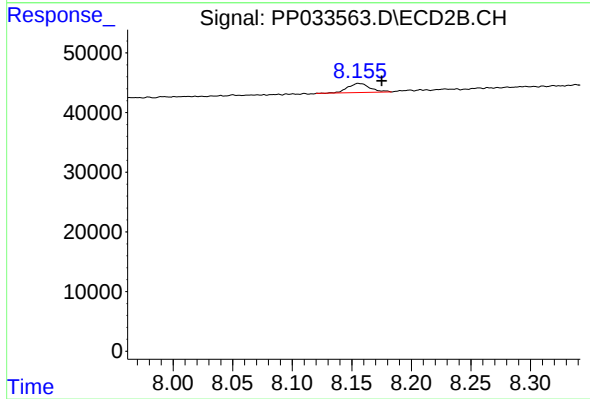

#41 AR-1268-1

R.T.: 8.155 min
Delta R.T.: -0.020 min
Response: 19847
Conc: 4.20 ng/ml