

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 19:11
 Operator : DD\AJ
 Sample : M1480-13 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:23:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.721	3.990	116549	108979	1.584	2.475 #
2)	SA Decachlor...	10.534	9.248	111664	94577	2.401	2.993
Target Compounds							
30)	L6 AR-1254-5	8.244	0.000	6858	0	2.924	N.D. #
32)	L7 AR-1260-2	7.958	0.000	20366	0	6.397	N.D. #
35)	L7 AR-1260-5	8.863	7.891	36295	14589	6.145	4.051 #
37)	L8 AR-1262-2	8.863	7.891	36295	14589	5.909	3.933 #
39)	L8 AR-1262-4	9.219f	0.000	4677	0	1.408	N.D. #
42)	L9 AR-1268-2	9.219f	0.000	4677	0	0.711	N.D. #
43)	L9 AR-1268-3	9.480f	0.000	176844	0	27.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 19:11
Operator : DD\AJ
Sample : M1480-13 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:23:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

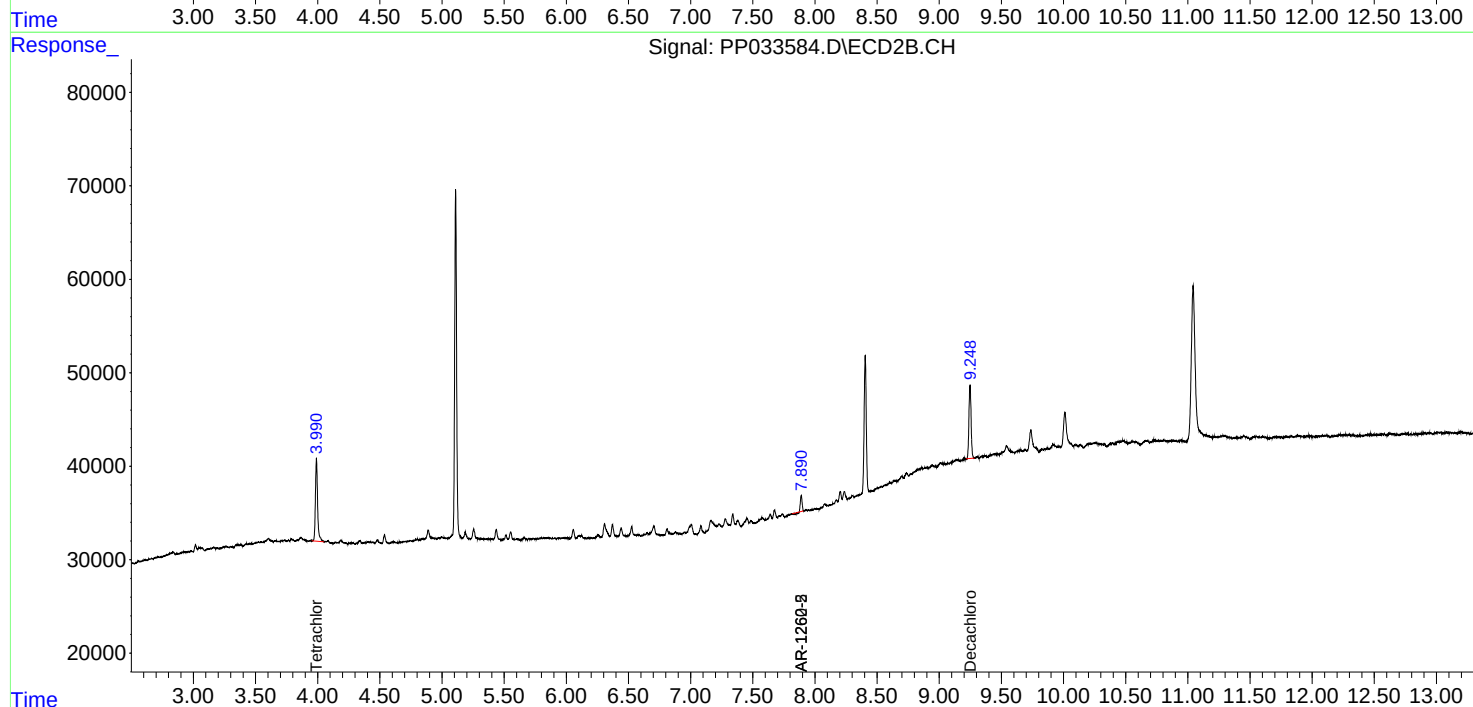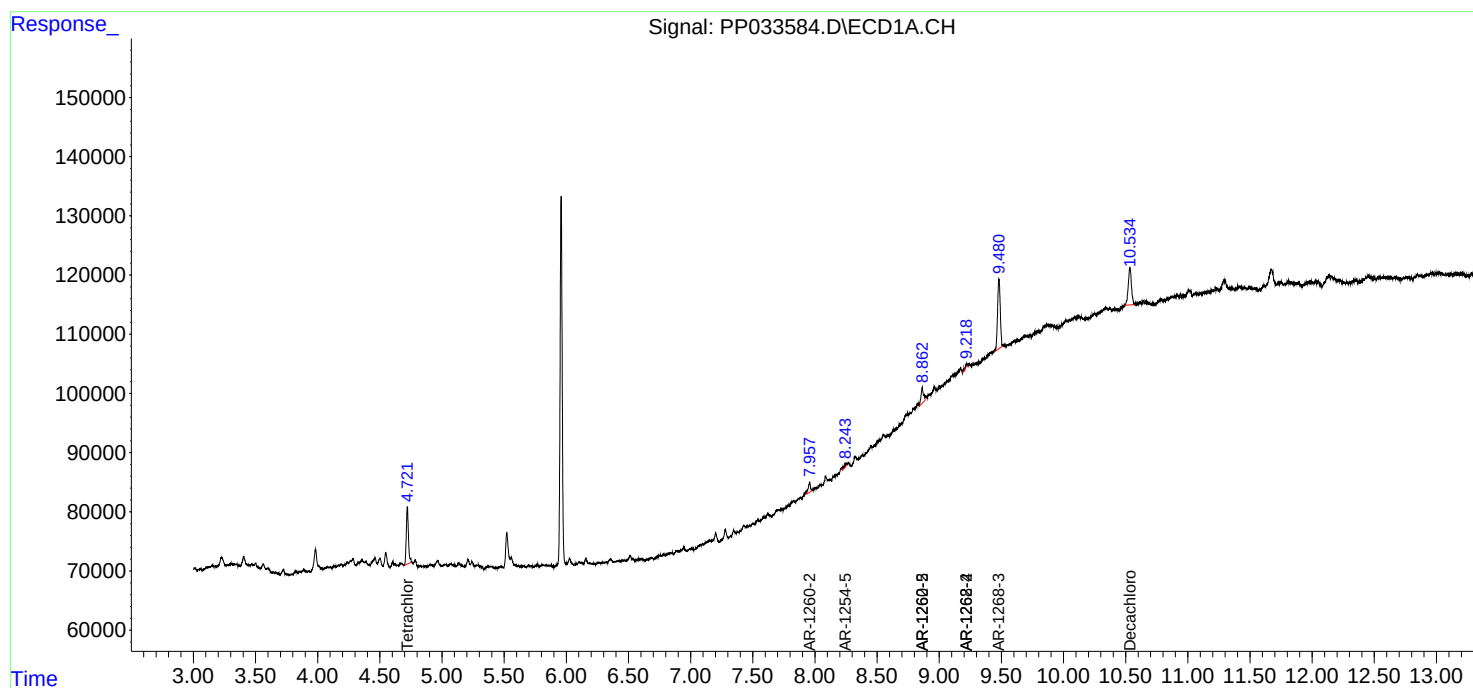


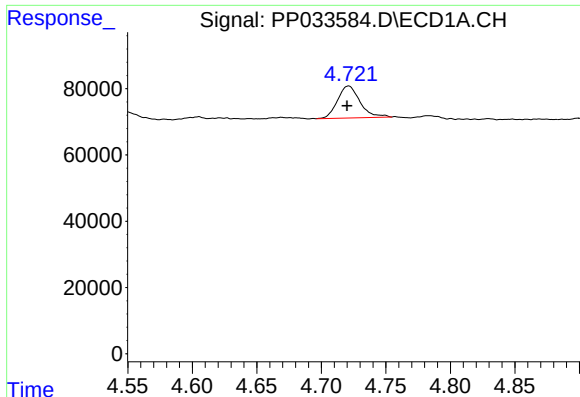

#1 Tetrachloro-m-xylene


R.T.: 4.721 min
Delta R.T.: 0.001 min
Response: 116549
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

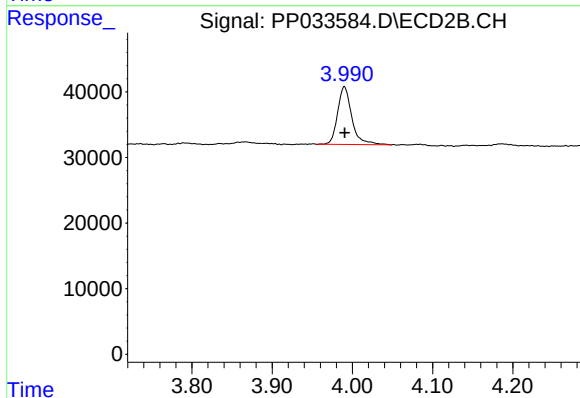


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 108979
Conc: 2.47 ng/ml

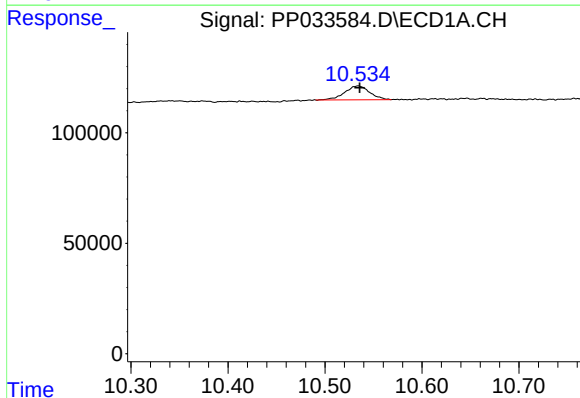


#2 Decachlorobiphenyl

R.T.: 10.534 min
Delta R.T.: -0.001 min
Response: 111664
Conc: 2.40 ng/ml

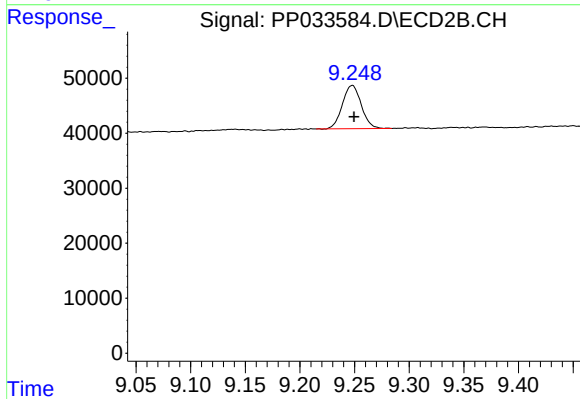

#2 Decachlorobiphenyl


R.T.: 9.248 min
Delta R.T.: -0.002 min
Response: 94577
Conc: 2.99 ng/ml

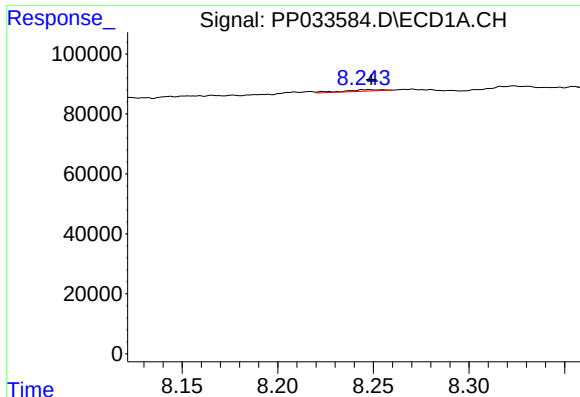

#30 AR-1254-5


R.T.: 8.244 min
Delta R.T.: -0.005 min
Response: 6858
Conc: 2.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

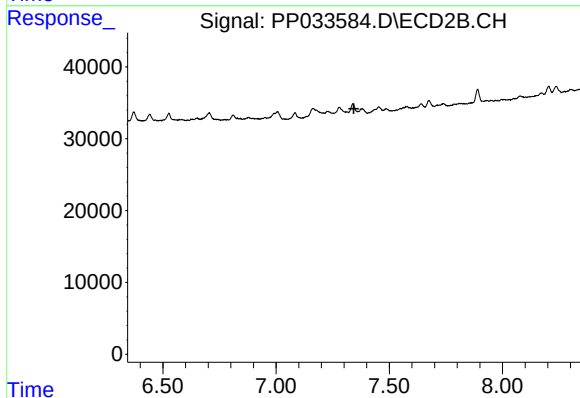


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

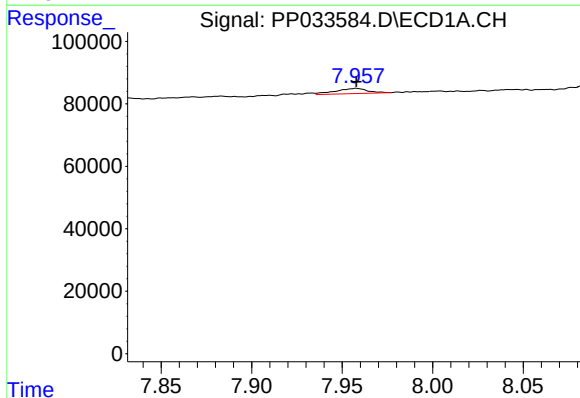


#32 AR-1260-2

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 20366
Conc: 6.40 ng/ml

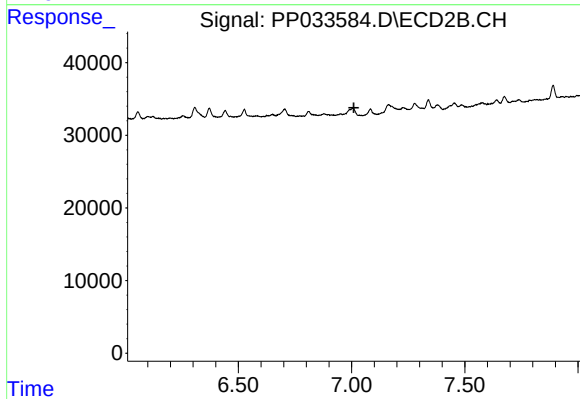

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.010 min
Response: 0
Conc: N.D.

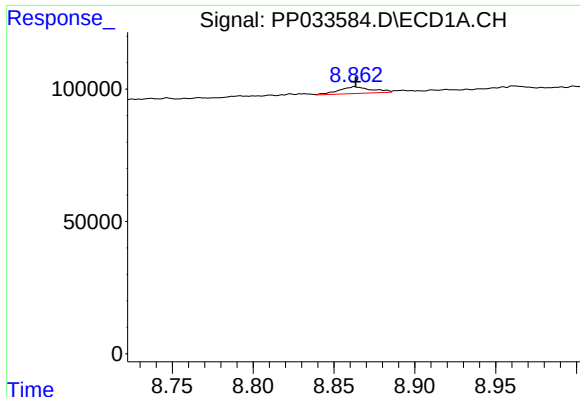

#35 AR-1260-5


R.T.: 8.863 min
Delta R.T.: 0.000 min
Response: 36295
Conc: 6.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

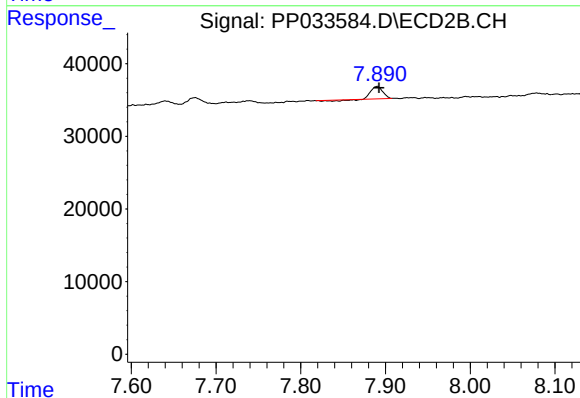


#35 AR-1260-5

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 14589
Conc: 4.05 ng/ml

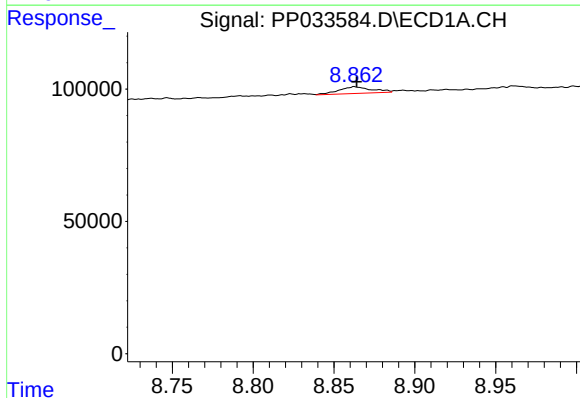


#37 AR-1262-2

R.T.: 8.863 min
Delta R.T.: -0.002 min
Response: 36295
Conc: 5.91 ng/ml

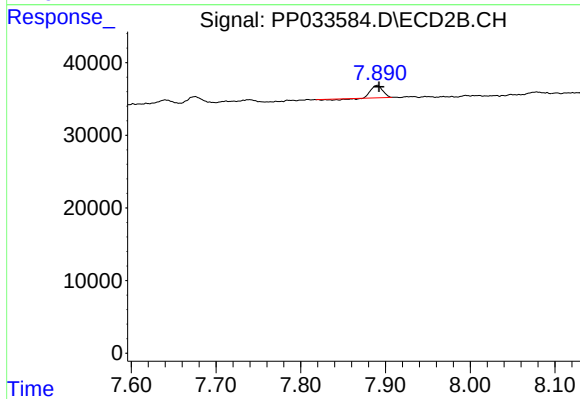

#37 AR-1262-2


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 14589
Conc: 3.93 ng/ml

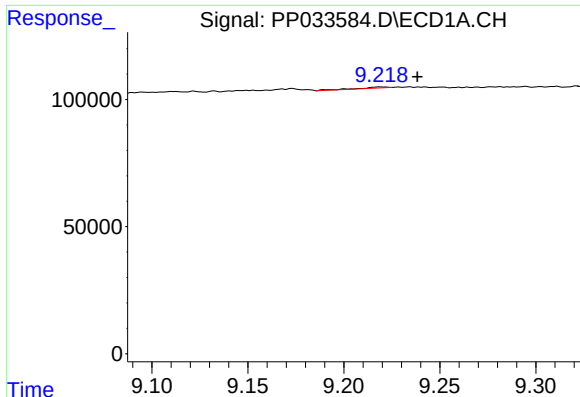

#39 AR-1262-4


R.T.: 9.219 min
Delta R.T.: -0.020 min
Response: 4677
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

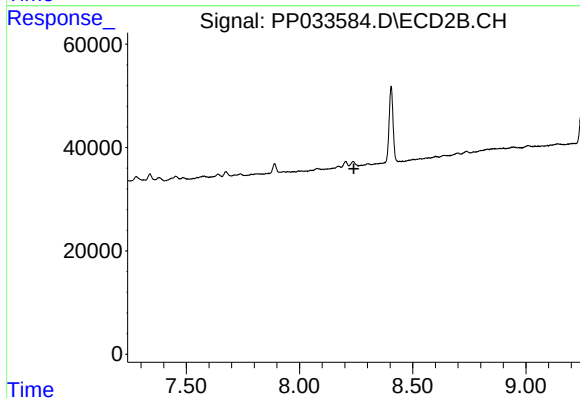


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.240 min
Response: 0
Conc: N.D.

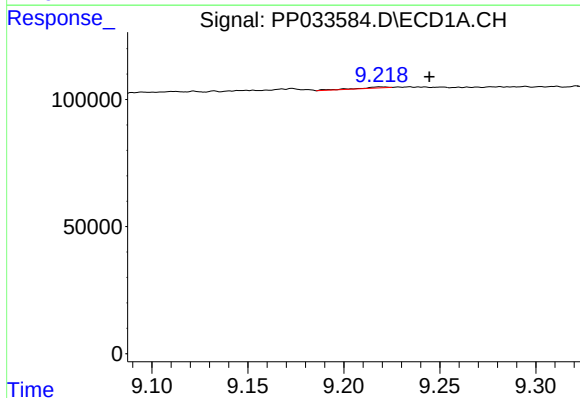


#42 AR-1268-2

R.T.: 9.219 min
Delta R.T.: -0.026 min
Response: 4677
Conc: 0.71 ng/ml

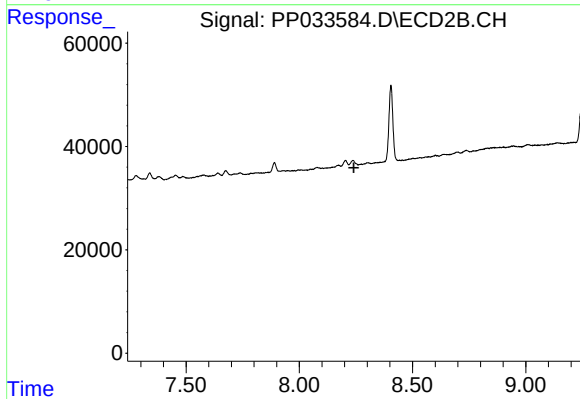

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.241 min
Response: 0
Conc: N.D.

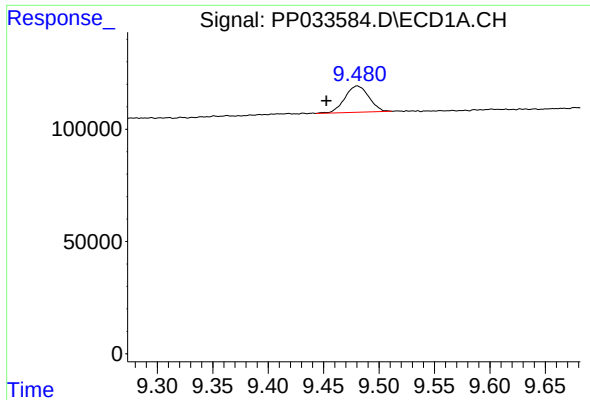

#43 AR-1268-3

R.T.: 9.480 min
Delta R.T.: 0.028 min
Response: 176844
Conc: 27.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

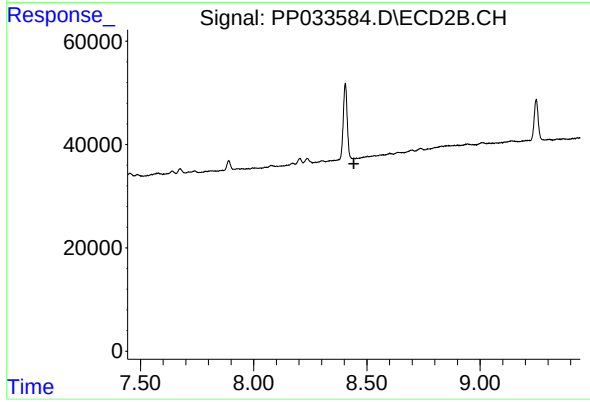

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.443 min
Response: 0
Conc: N.D.