

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 22:16
 Operator : DD\AJ
 Sample : M1480-05 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:28:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.718	3.988	106723	109351	1.450	2.483 #
2)	SA Decachlor...	10.531	9.244	87904	101502	1.890	3.212 #
Target Compounds							
8)	L2 AR-1221-1	4.950f	0.000	60	0	0.090	N.D. #
32)	L7 AR-1260-2	7.955	0.000	21821	0	6.854	N.D. #
33)	L7 AR-1260-3	0.000	7.181f	0	25618	N.D.	12.714 #
35)	L7 AR-1260-5	8.842f	7.881	1177	27702	0.199	7.693 #
37)	L8 AR-1262-2	8.842f	7.881	1177	27702	0.192	7.468 #
39)	L8 AR-1262-4	9.255f	0.000	9335	0	2.810	N.D. #
42)	L9 AR-1268-2	9.255	0.000	9335	0	1.418	N.D. #
45)	L9 AR-1268-5	10.213f	0.000	257	0	0.015	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 22:16
Operator : DD\AJ
Sample : M1480-05 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:28:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

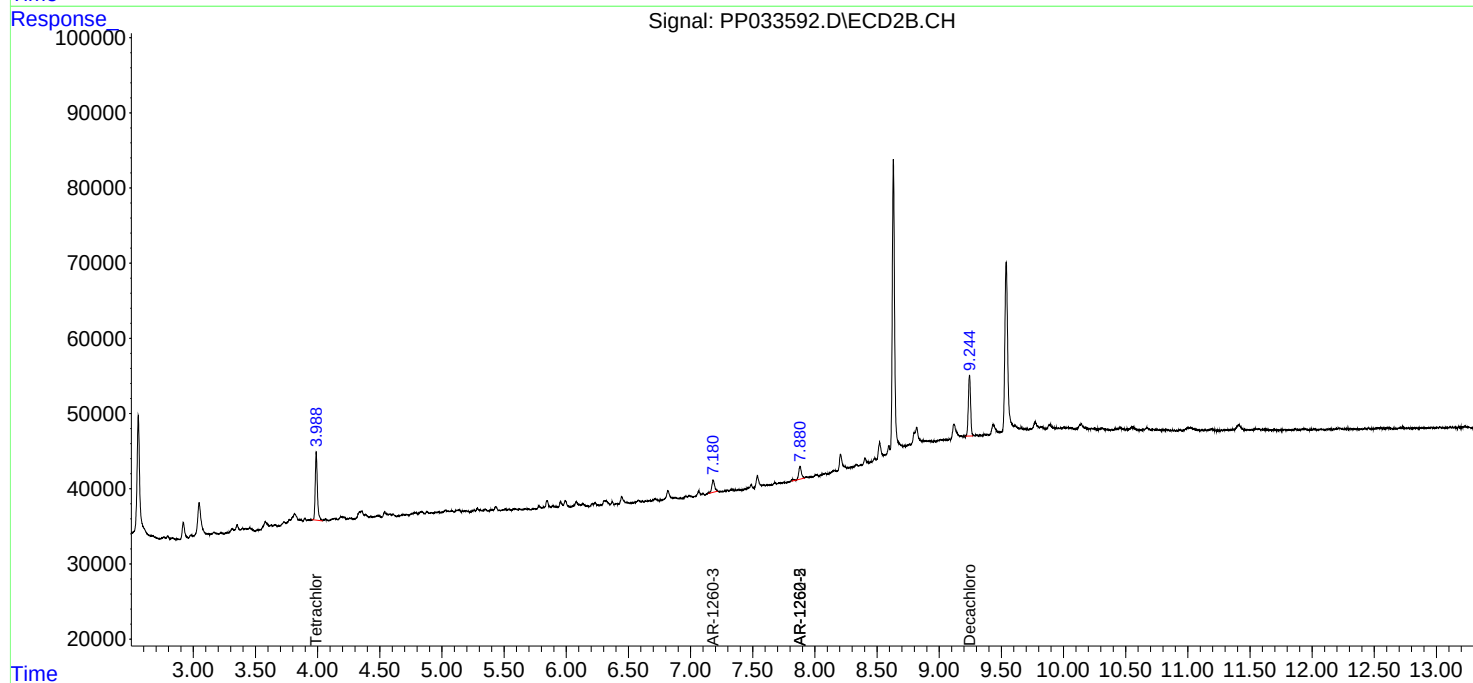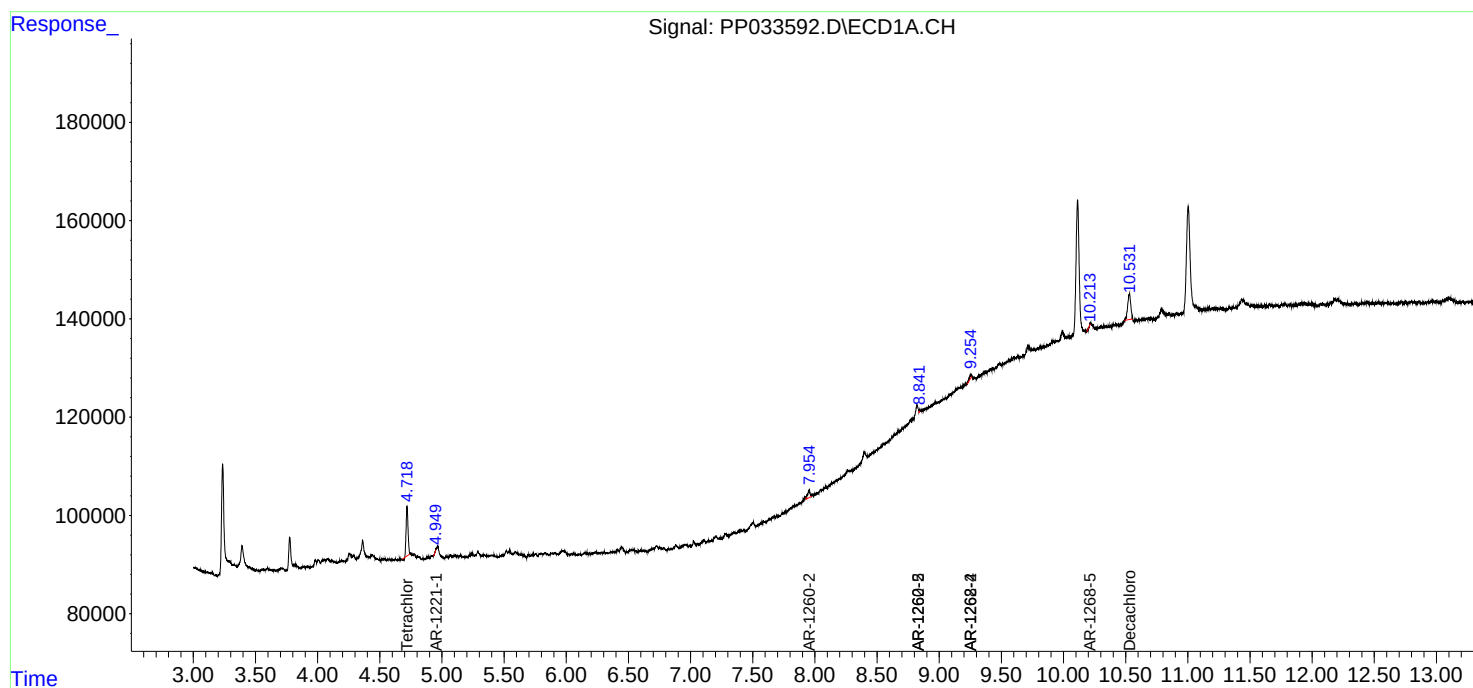


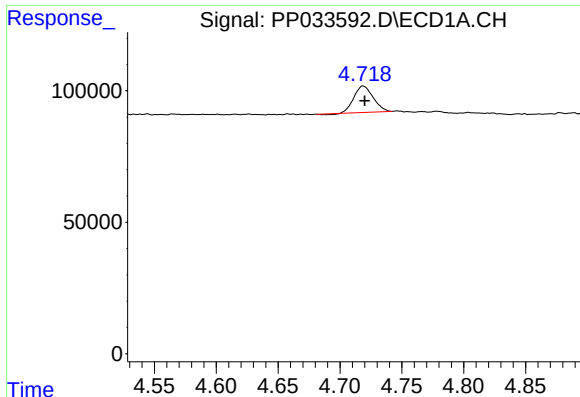

#1 Tetrachloro-m-xylene


R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 106723
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

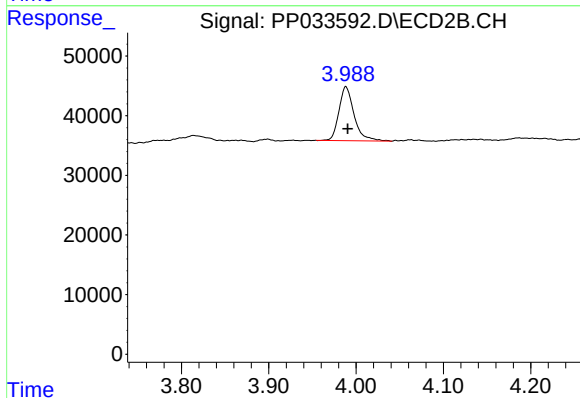


#1 Tetrachloro-m-xylene

R.T.: 3.988 min
Delta R.T.: -0.002 min
Response: 109351
Conc: 2.48 ng/ml

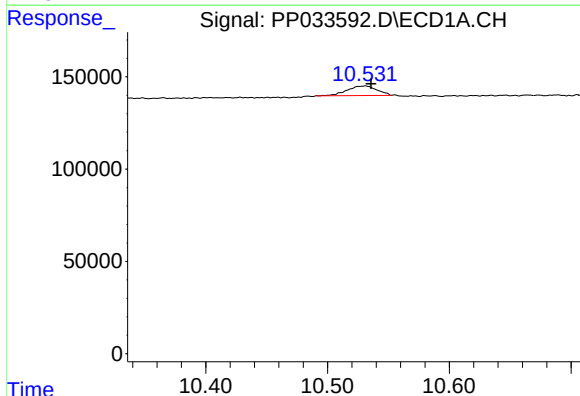


#2 Decachlorobiphenyl

R.T.: 10.531 min
Delta R.T.: -0.004 min
Response: 87904
Conc: 1.89 ng/ml

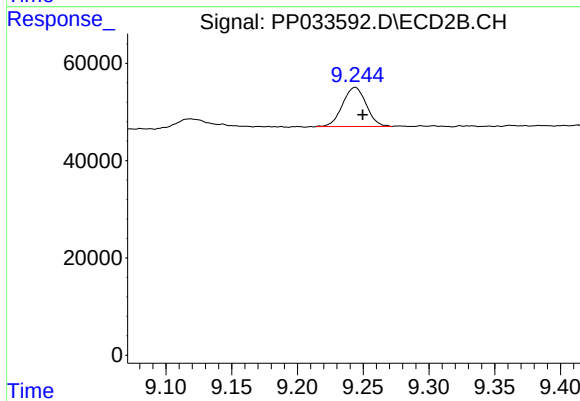

#2 Decachlorobiphenyl


R.T.: 9.244 min
Delta R.T.: -0.006 min
Response: 101502
Conc: 3.21 ng/ml

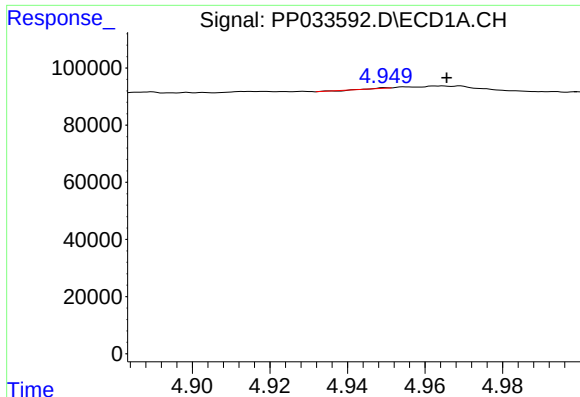

#8 AR-1221-1


R.T.: 4.950 min
Delta R.T.: -0.016 min
Response: 60
Conc: 0.09 ng/ml

Instrument :
ECD_P
ClientSampleId :

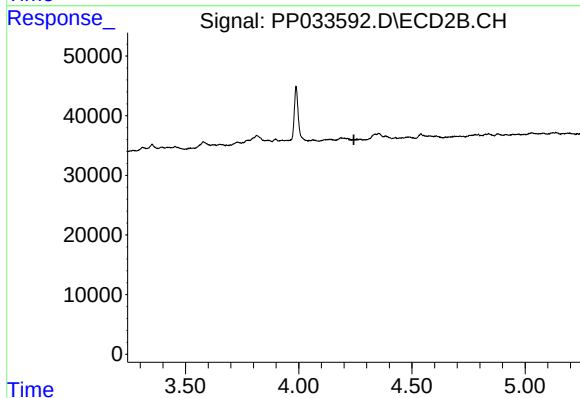


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.244 min
Response: 0
Conc: N.D.

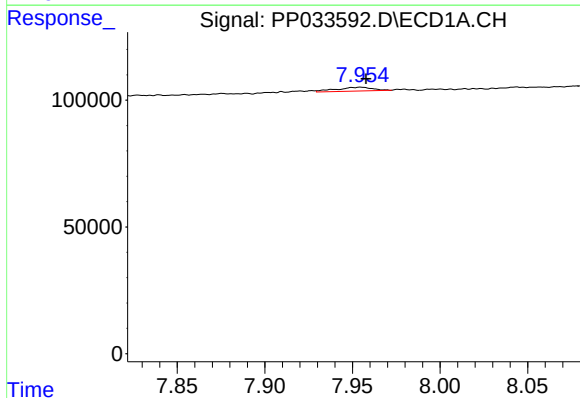


#32 AR-1260-2

R.T.: 7.955 min
Delta R.T.: -0.003 min
Response: 21821
Conc: 6.85 ng/ml

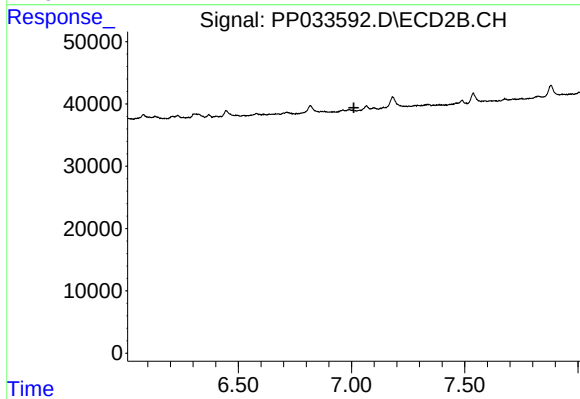

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.010 min
Response: 0
Conc: N.D.

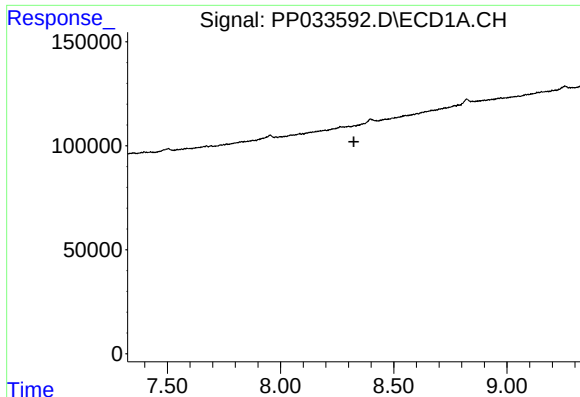

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

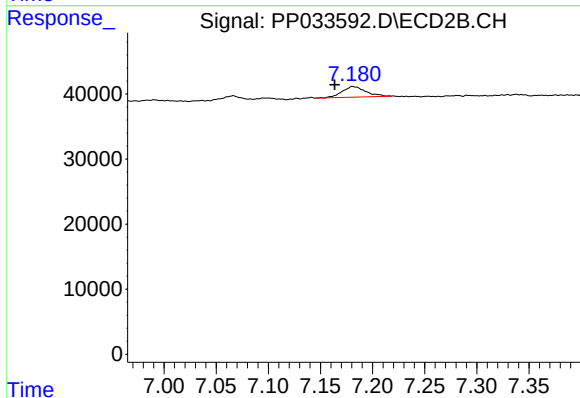


#33 AR-1260-3

R.T.: 7.181 min
Delta R.T.: 0.017 min
Response: 25618
Conc: 12.71 ng/ml

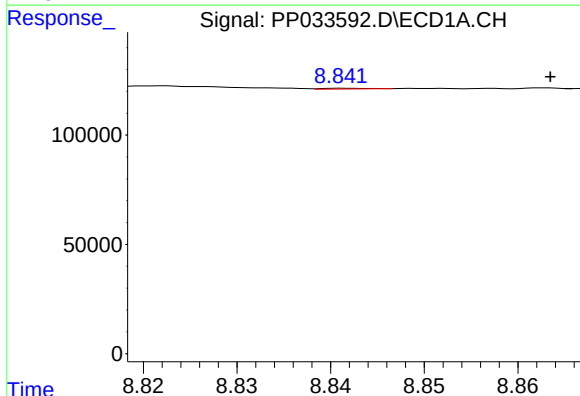


#35 AR-1260-5

R.T.: 8.842 min
Delta R.T.: -0.022 min
Response: 1177
Conc: 0.20 ng/ml

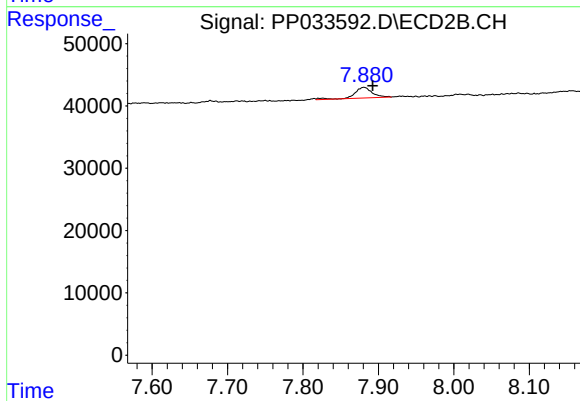

#35 AR-1260-5


R.T.: 7.881 min
Delta R.T.: -0.012 min
Response: 27702
Conc: 7.69 ng/ml

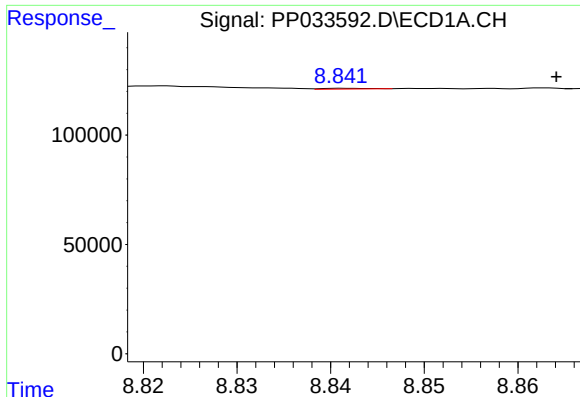

#37 AR-1262-2


R.T.: 8.842 min
Delta R.T.: -0.022 min
Response: 1177
Conc: 0.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

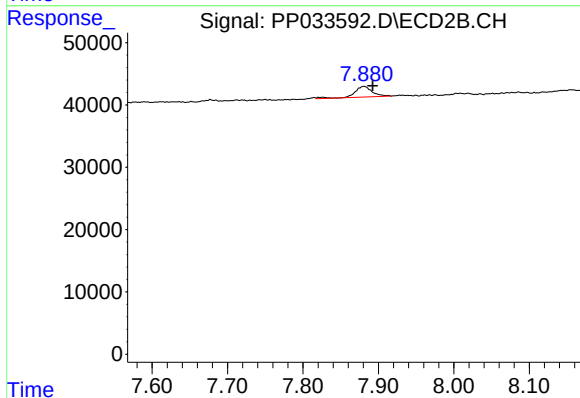


#37 AR-1262-2

R.T.: 7.881 min
Delta R.T.: -0.012 min
Response: 27702
Conc: 7.47 ng/ml

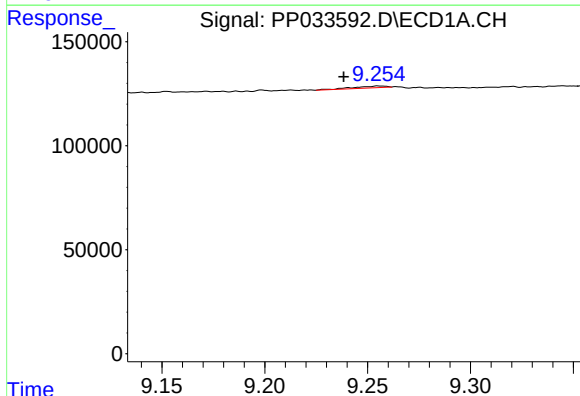


#39 AR-1262-4

R.T.: 9.255 min
Delta R.T.: 0.017 min
Response: 9335
Conc: 2.81 ng/ml

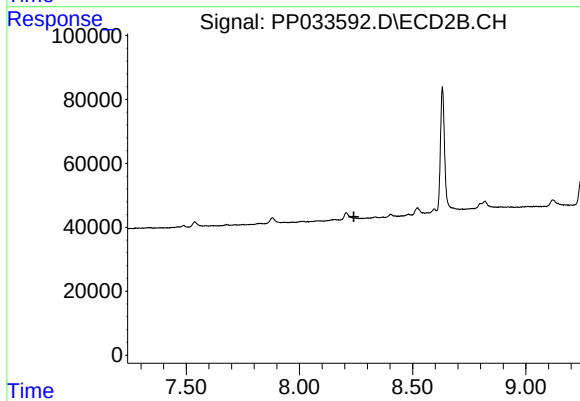

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.240 min
Response: 0
Conc: N.D.

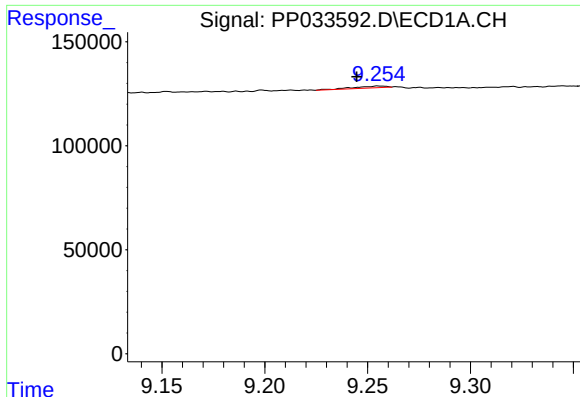

#42 AR-1268-2


R.T.: 9.255 min
Delta R.T.: 0.010 min
Response: 9335
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :

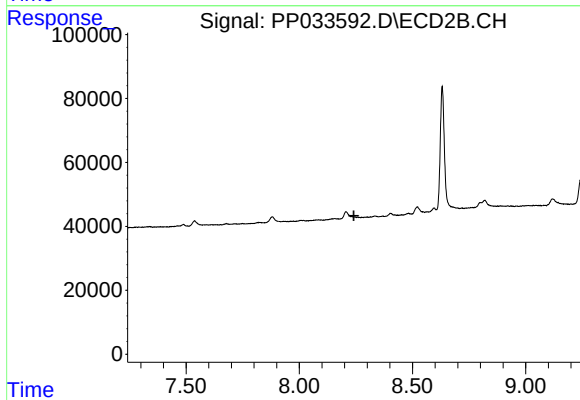


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.241 min
Response: 0
Conc: N.D.

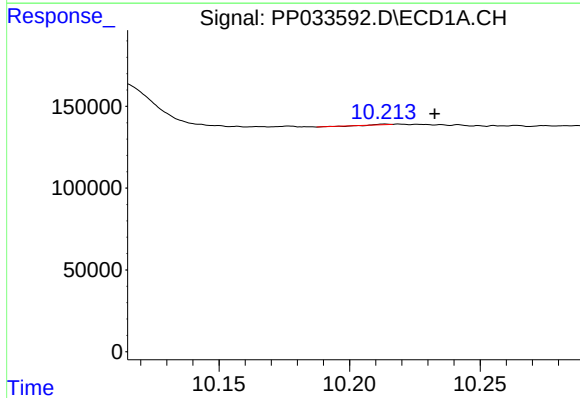

#45 AR-1268-5

R.T.: 10.213 min
Delta R.T.: -0.019 min
Response: 257
Conc: 0.02 ng/ml

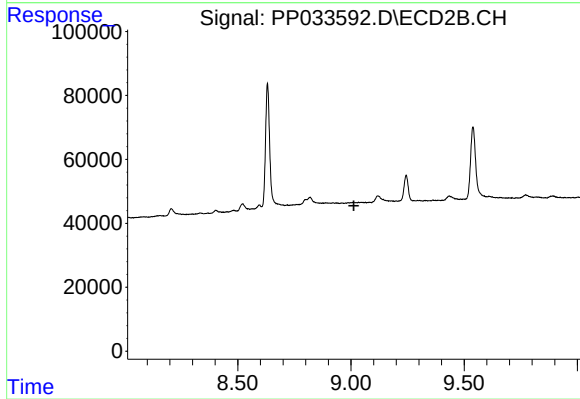

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.013 min
Response: 0
Conc: N.D.