

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033567.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 13:55
 Operator : DD\AJ
 Sample : M1469-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-08-022321

Manual Integrations
 APPROVED

Ankita
 2/26/2021 10:31:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 07:06:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.723	3.992	959367	769780	13.035	17.480 #
2) SA Decachlor...	10.536	9.248	702162	596455	15.097	18.877 #
Target Compounds						
31) L7 AR-1260-1	7.694	6.813	36809	49753	16.067m	28.817 #
32) L7 AR-1260-2	7.958	7.010	133434	54584	41.913	27.743 #
33) L7 AR-1260-3	8.322	7.161	33756	45128	11.633	22.397m#
34) L7 AR-1260-4	8.549	7.643	66634	26400	25.534	16.296 #
35) L7 AR-1260-5	8.865	7.891	94654	49525	16.026	13.753m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 13:55
Operator : DD\AJ
Sample : M1469-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TR-08-022321


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 07:06:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

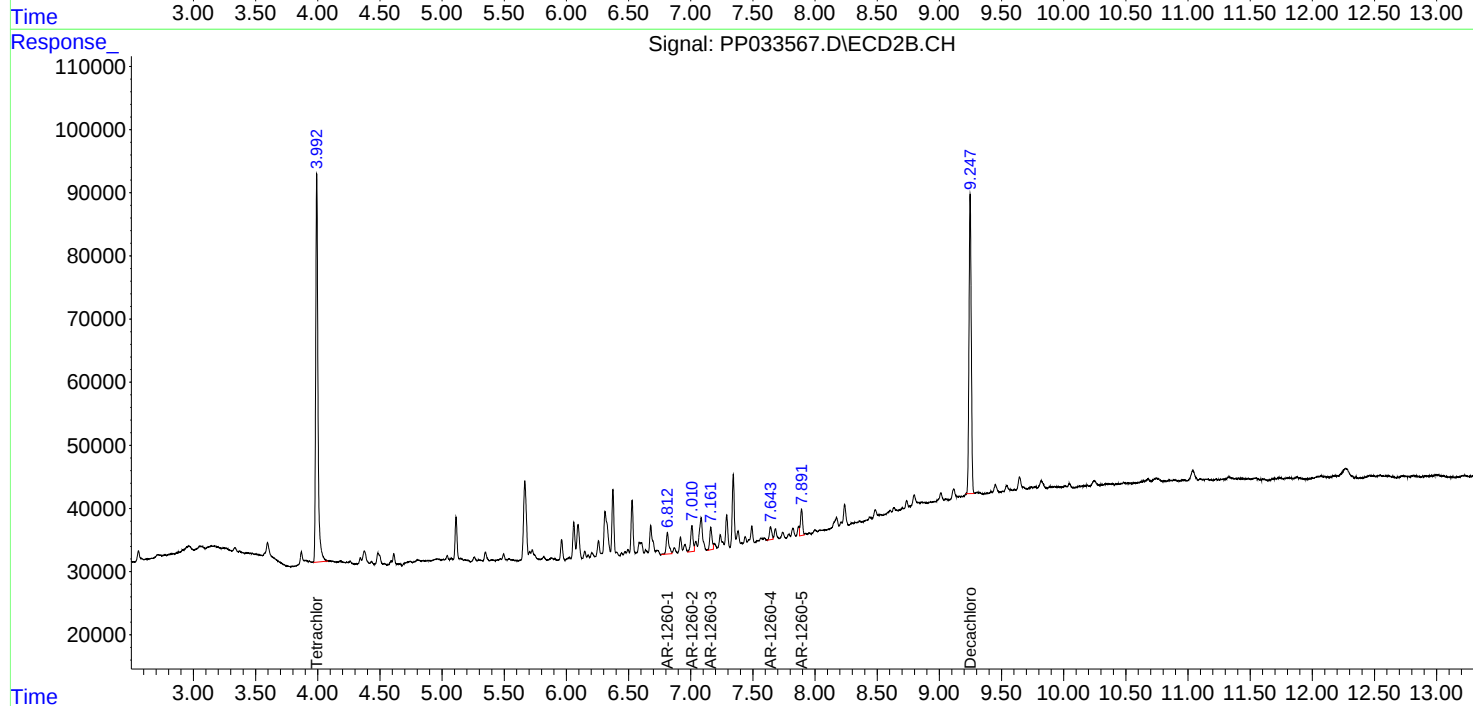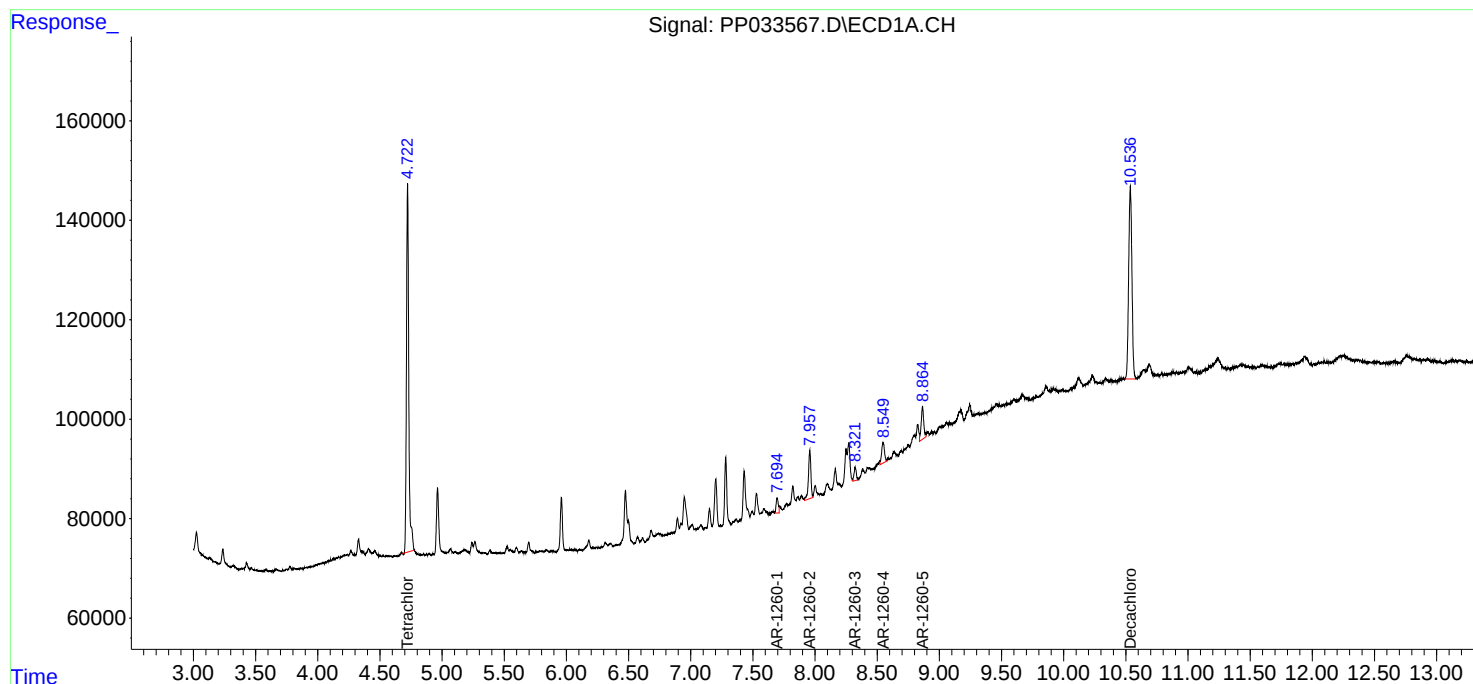

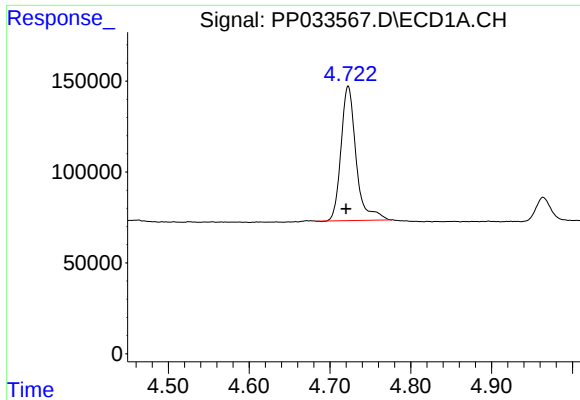


#1 Tetrachloro-m-xylene

R.T.: 4.723 min
Delta R.T.: 0.003 min
Response: 959367
Conc: 13.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-08-022321


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:17 AM

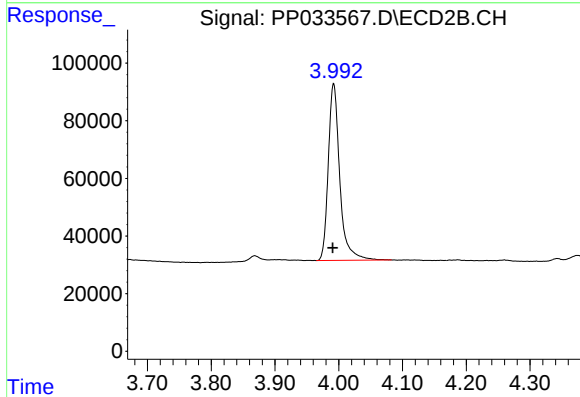


#1 Tetrachloro-m-xylene

R.T.: 3.992 min
Delta R.T.: 0.002 min
Response: 769780
Conc: 17.48 ng/ml

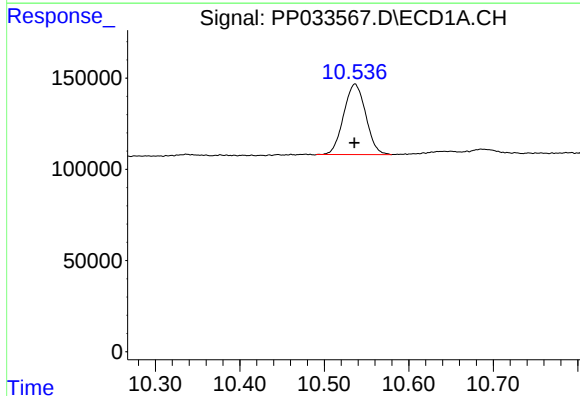


#2 Decachlorobiphenyl

R.T.: 10.536 min
Delta R.T.: 0.000 min
Response: 702162
Conc: 15.10 ng/ml

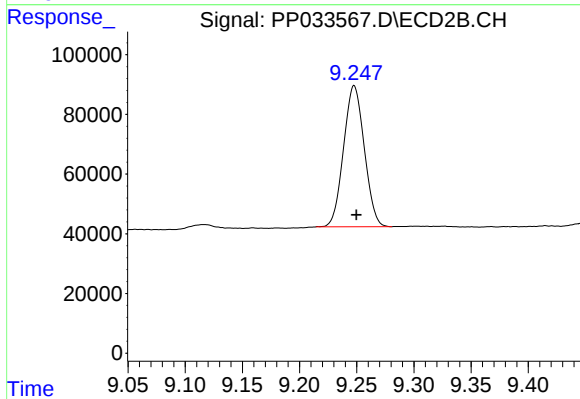

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.002 min
Response: 596455
Conc: 18.88 ng/ml

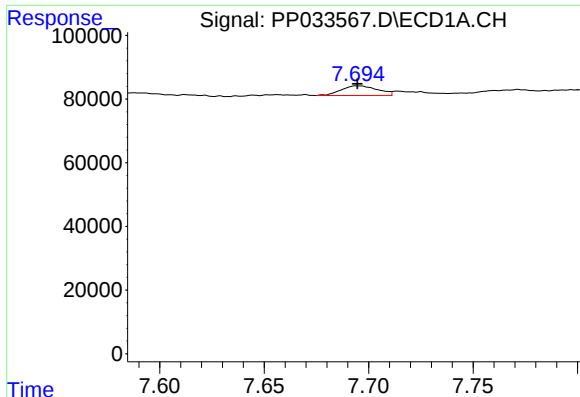


#31 AR-1260-1

R.T.: 7.694 min
Delta R.T.: 0.000 min
Response: 36809
Conc: 16.07 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TR-08-022321


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:17 AM

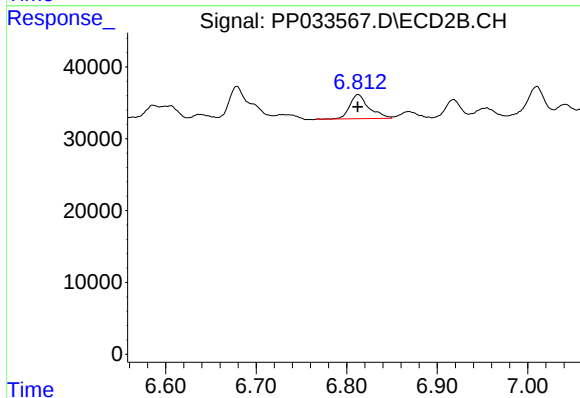


#31 AR-1260-1

R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 49753
Conc: 28.82 ng/ml

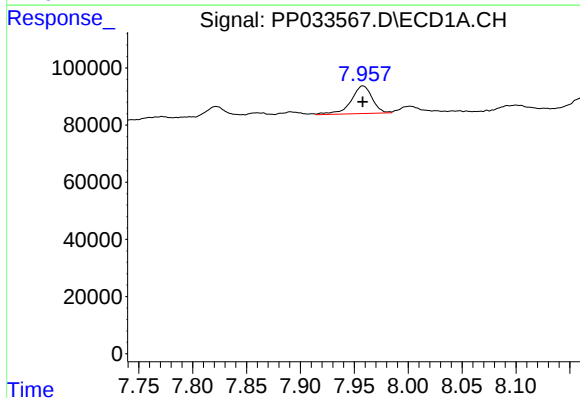


#32 AR-1260-2

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 133434
Conc: 41.91 ng/ml

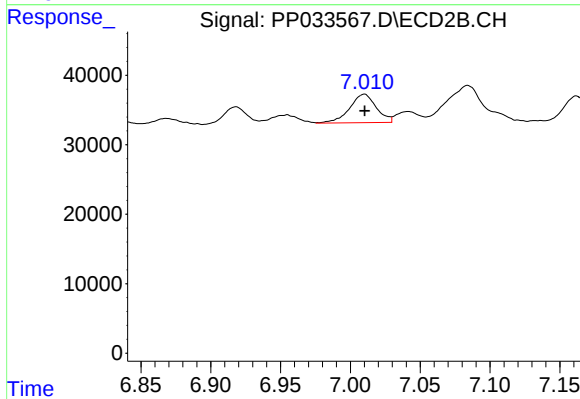

#32 AR-1260-2

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 54584
Conc: 27.74 ng/ml

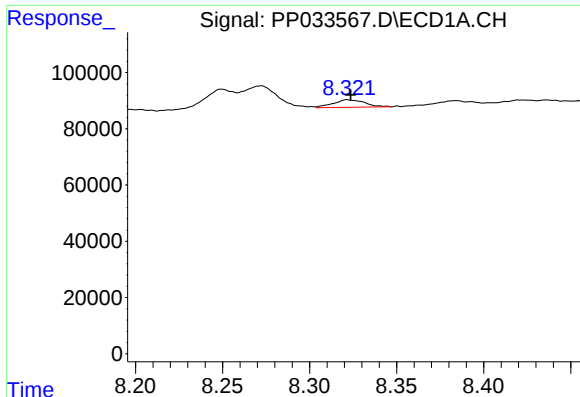


#33 AR-1260-3

R.T.: 8.322 min
Delta R.T.: -0.002 min
Response: 33756
Conc: 11.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-08-022321


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:17 AM

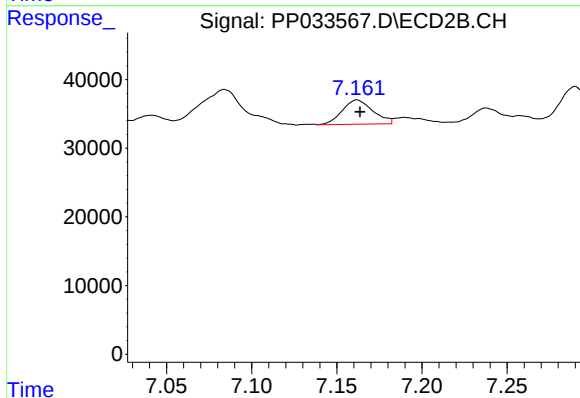


#33 AR-1260-3

R.T.: 7.161 min
Delta R.T.: -0.002 min
Response: 45128
Conc: 22.40 ng/ml m

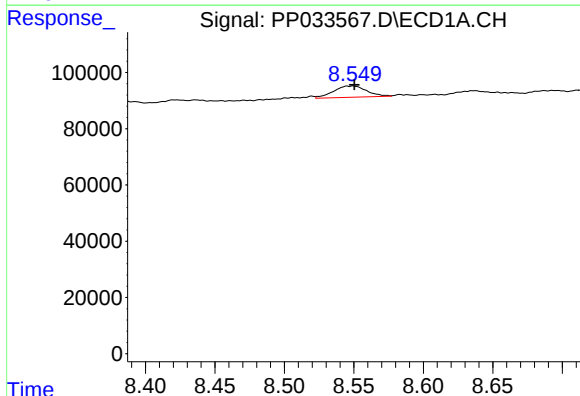


#34 AR-1260-4

R.T.: 8.549 min
Delta R.T.: 0.000 min
Response: 66634
Conc: 25.53 ng/ml

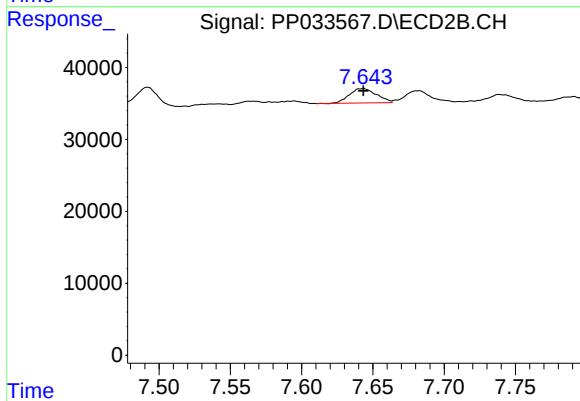

#34 AR-1260-4

R.T.: 7.643 min
Delta R.T.: 0.000 min
Response: 26400
Conc: 16.30 ng/ml

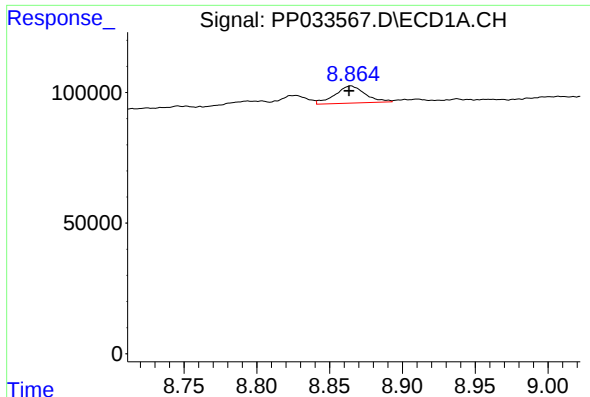


#35 AR-1260-5

R.T.: 8.865 min
Delta R.T.: 0.001 min
Response: 94654
Conc: 16.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-08-022321

Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:17 AM

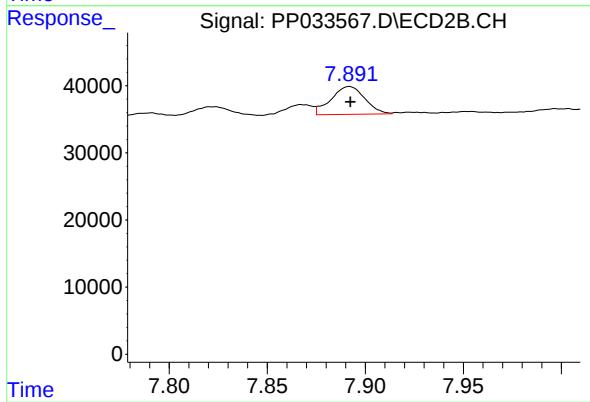

#35 AR-1260-5

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 49525
Conc: 13.75 ng/ml m