

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033570.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 14:45
 Operator : DD\AJ
 Sample : M1472-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMPOSITE-01(TP2-TP1)

Manual Integrations
 APPROVED

Ankita
 2/26/2021 10:31:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 15:21:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.723	3.994	1312783	797890	17.836m	18.118
2) SA Decachlor...	10.533	9.247	927355	878065	19.939	27.789 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 14:45
Operator : DD\AJ
Sample : M1472-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMPOSITE-01(TP2-TP1)


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 15:21:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

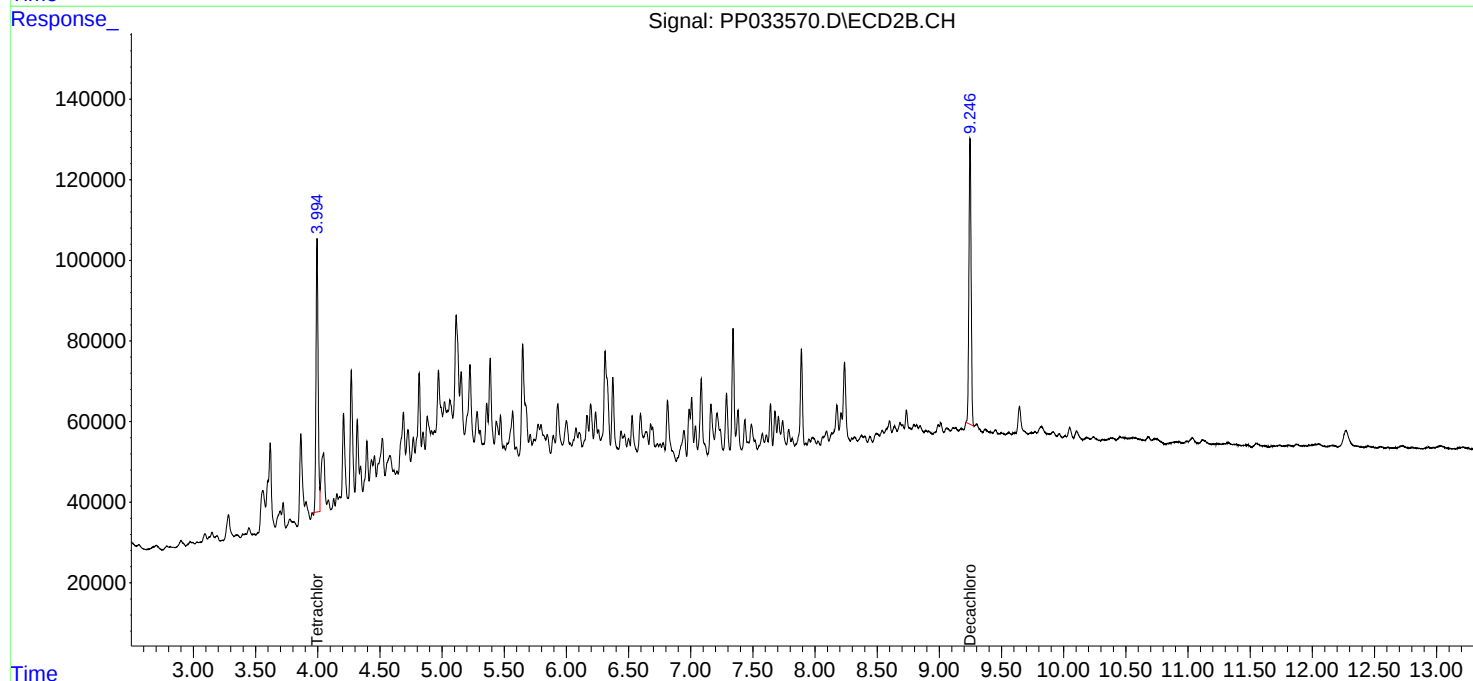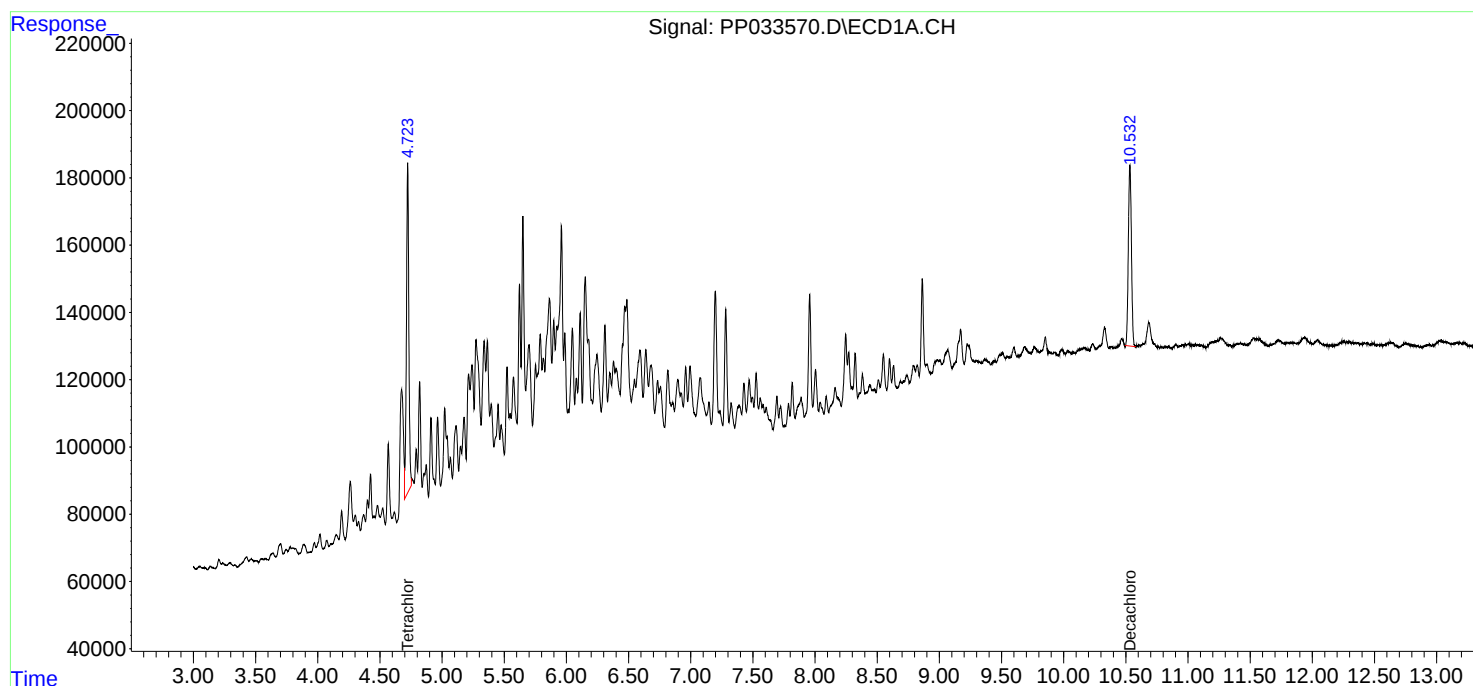

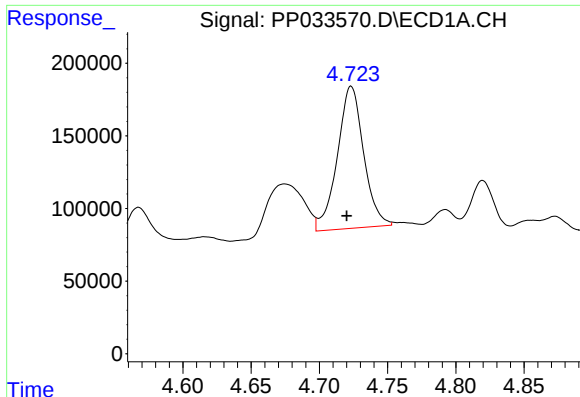


#1 Tetrachloro-m-xylene

R.T.: 4.723 min
Delta R.T.: 0.003 min
Response: 1312783
Conc: 17.84 ng/ml m

Instrument :
ECD_P
ClientSampleId :
COMPOSITE-01(TP2-TP1)


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:21 AM

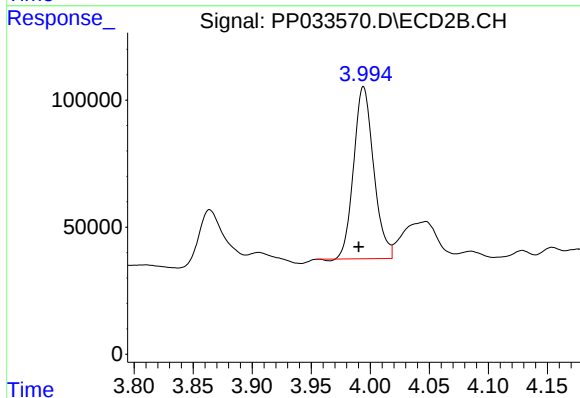


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: 0.004 min
Response: 797890
Conc: 18.12 ng/ml

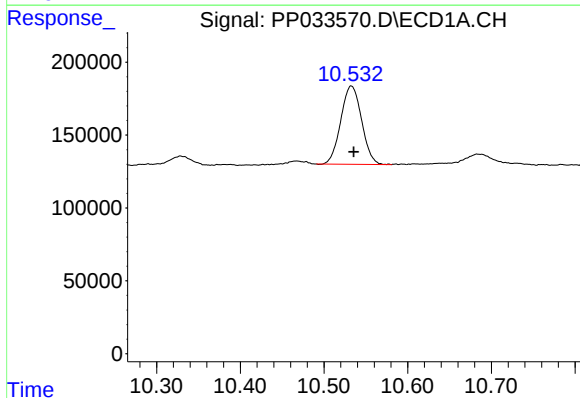

#2 Decachlorobiphenyl

R.T.: 10.533 min
Delta R.T.: -0.003 min
Response: 927355
Conc: 19.94 ng/ml

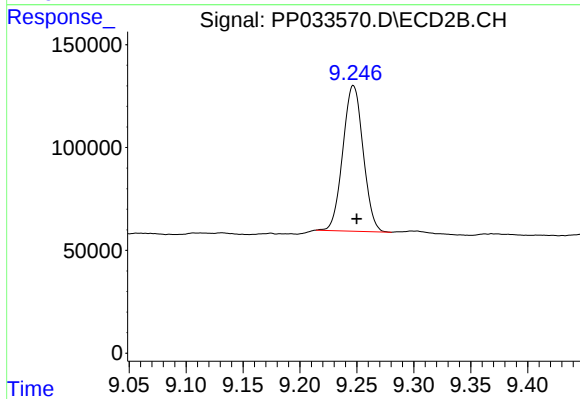

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.003 min
Response: 878065
Conc: 27.79 ng/ml