

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
 Data File : PP033574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2021 16:22
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 2/26/2021 10:31:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 17:34:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.720	3.991	3125746	2291498	42.468	52.034
2)	SA Decachlor...	10.531	9.246	2305182	1882137	49.562	59.566m
Target Compounds							
21)	L5 AR-1248-1	6.017	5.233	493960	387979	447.004	563.887 #
22)	L5 AR-1248-2	6.309	5.494	673263	539865	440.994	545.122
23)	L5 AR-1248-3	6.523	5.537	816476	575542	452.377	546.488
24)	L5 AR-1248-4	6.948	5.722	875820	694676	462.606	546.550
25)	L5 AR-1248-5	6.987	6.142	865165	653038	469.308	580.399

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022521\
Data File : PP033574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2021 16:22
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 17:34:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

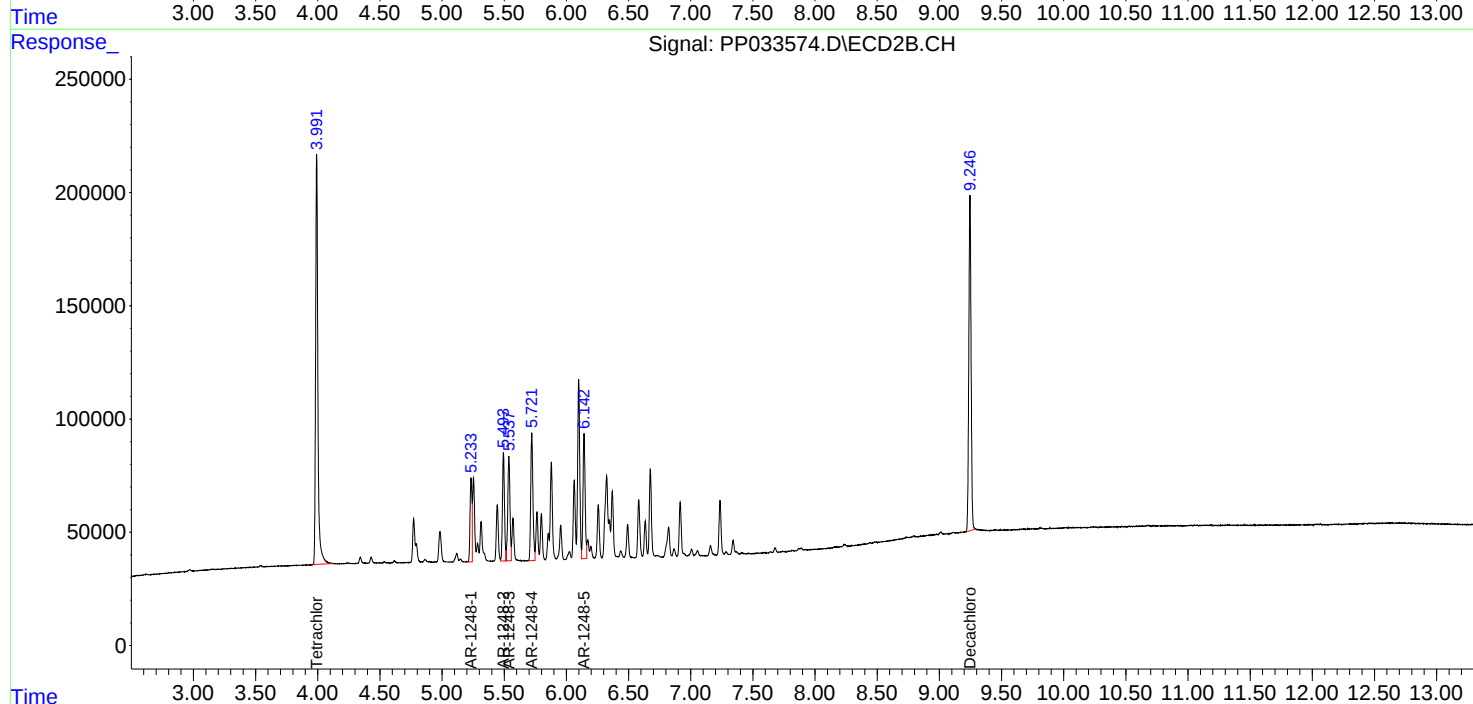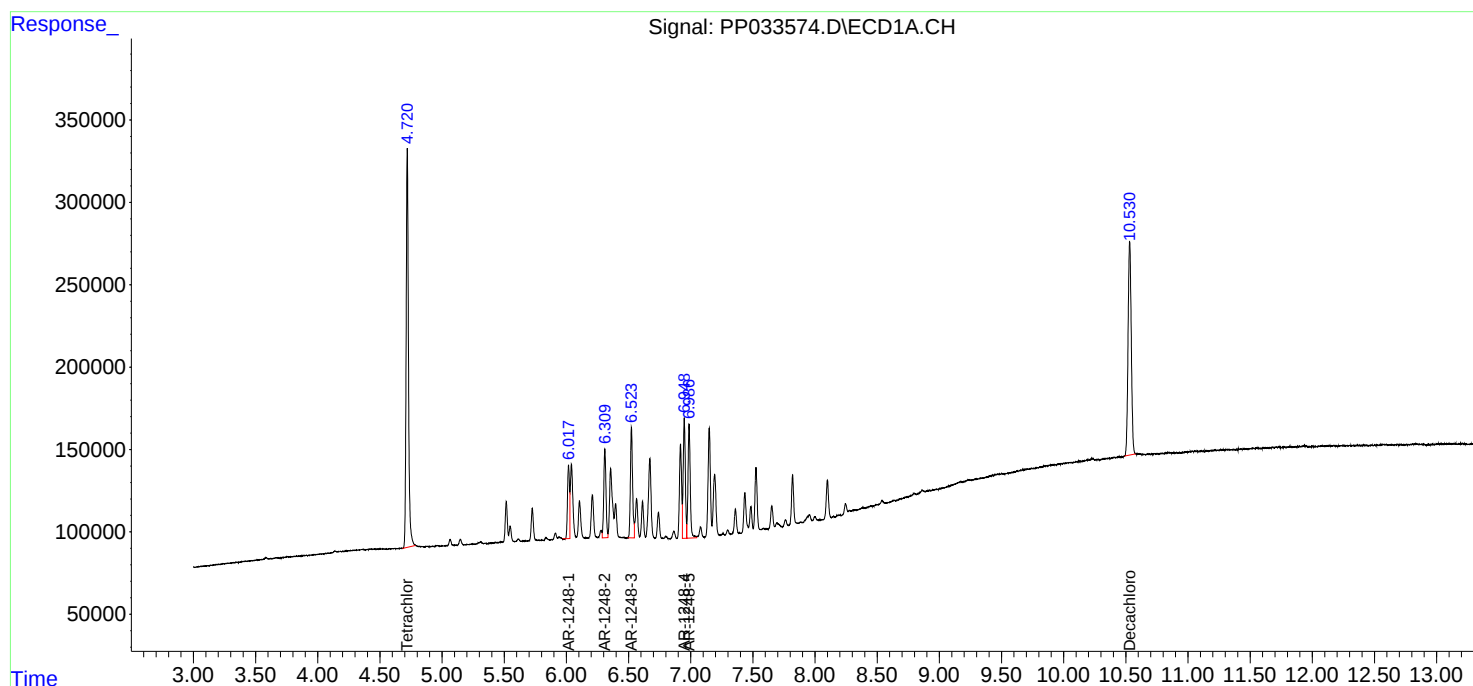

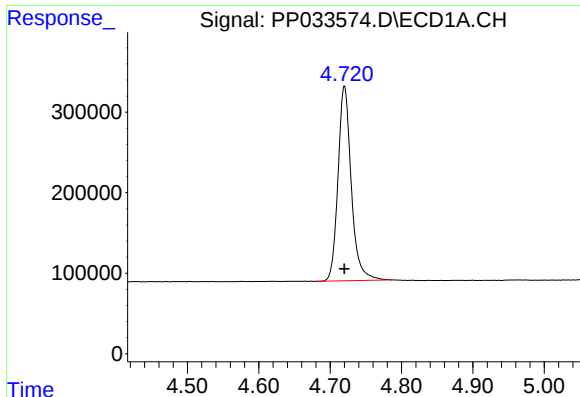


#1 Tetrachloro-m-xylene

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 3125746
Conc: 42.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:23 AM

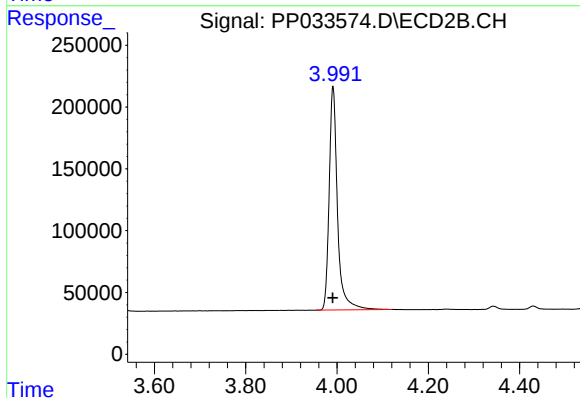


#1 Tetrachloro-m-xylene

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 2291498
Conc: 52.03 ng/ml

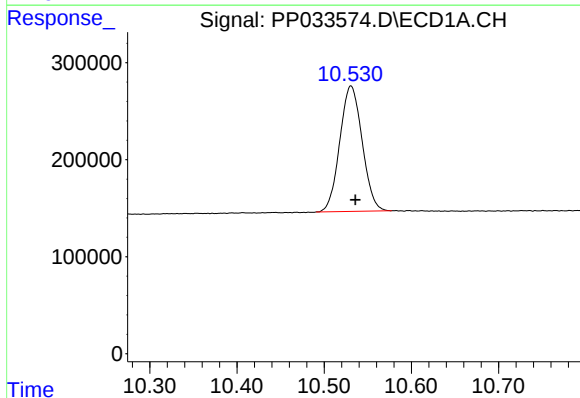


#2 Decachlorobiphenyl

R.T.: 10.531 min
Delta R.T.: -0.005 min
Response: 2305182
Conc: 49.56 ng/ml

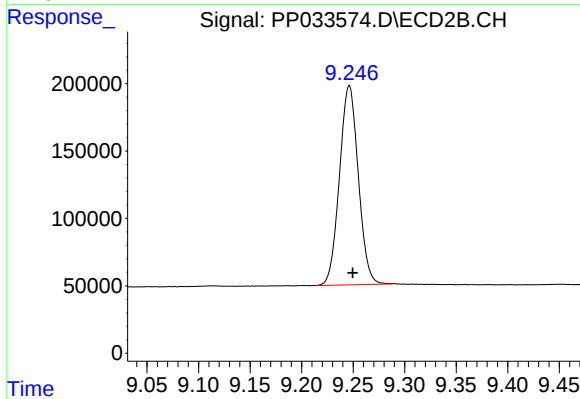

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: -0.004 min
Response: 1882137
Conc: 59.57 ng/ml m

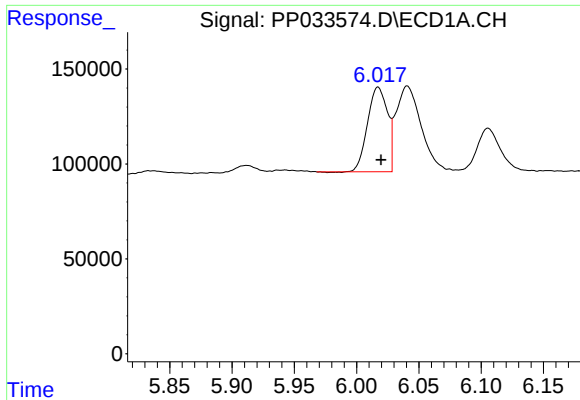


#21 AR-1248-1

R.T.: 6.017 min
Delta R.T.: -0.002 min
Response: 493960
Conc: 447.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:23 AM

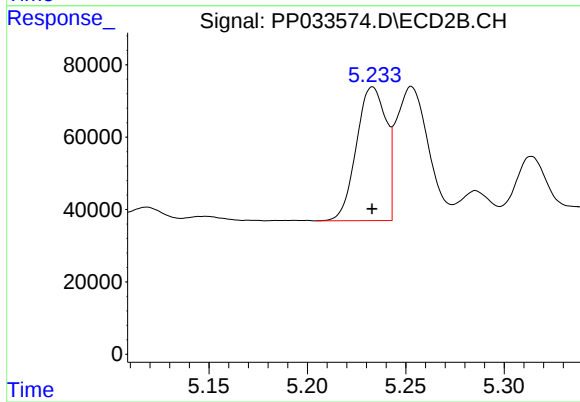


#21 AR-1248-1

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 387979
Conc: 563.89 ng/ml

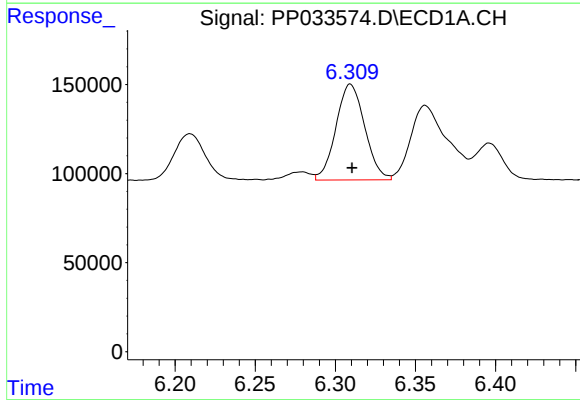


#22 AR-1248-2

R.T.: 6.309 min
Delta R.T.: -0.001 min
Response: 673263
Conc: 440.99 ng/ml

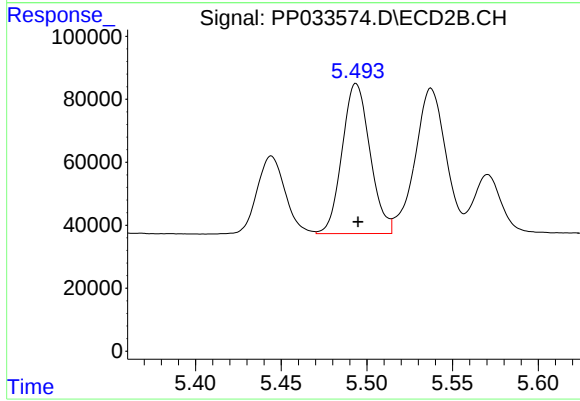

#22 AR-1248-2

R.T.: 5.494 min
Delta R.T.: -0.001 min
Response: 539865
Conc: 545.12 ng/ml

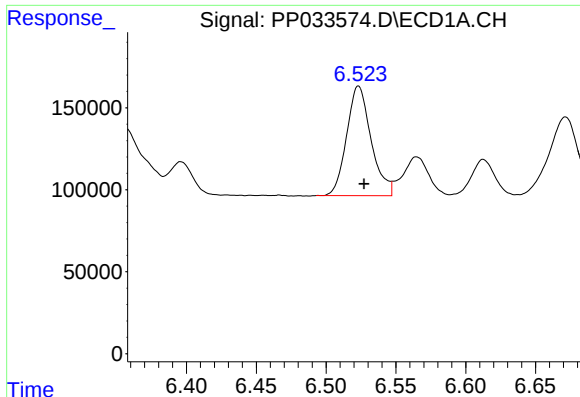


#23 AR-1248-3

R.T.: 6.523 min
Delta R.T.: -0.004 min
Response: 816476
Conc: 452.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:23 AM

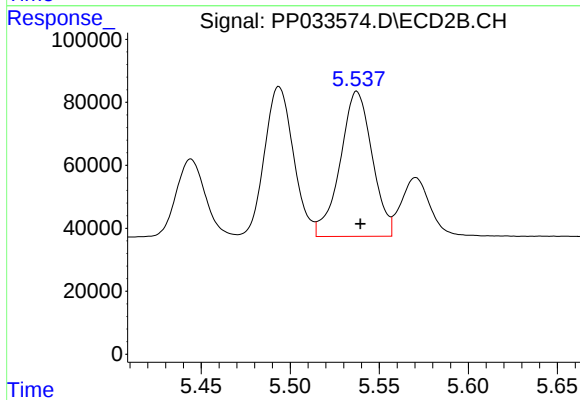


#23 AR-1248-3

R.T.: 5.537 min
Delta R.T.: -0.002 min
Response: 575542
Conc: 546.49 ng/ml

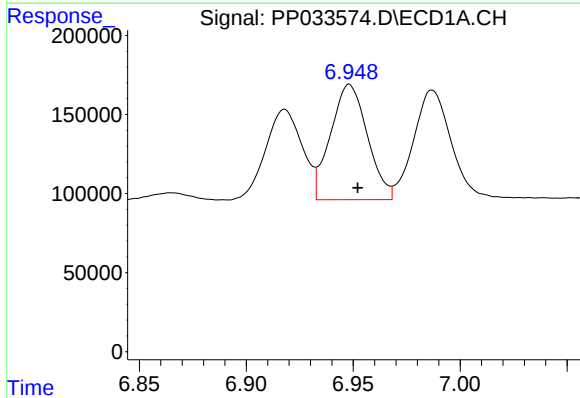


#24 AR-1248-4

R.T.: 6.948 min
Delta R.T.: -0.004 min
Response: 875820
Conc: 462.61 ng/ml

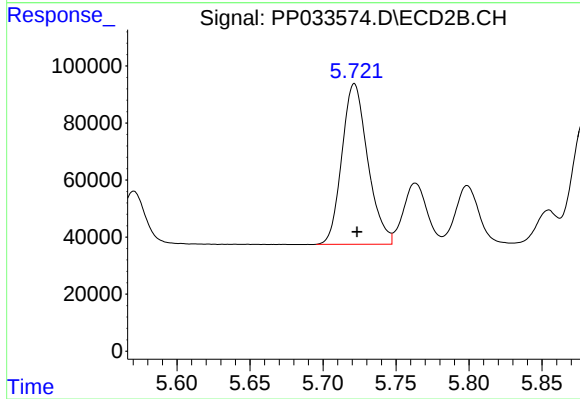

#24 AR-1248-4

R.T.: 5.722 min
Delta R.T.: -0.002 min
Response: 694676
Conc: 546.55 ng/ml

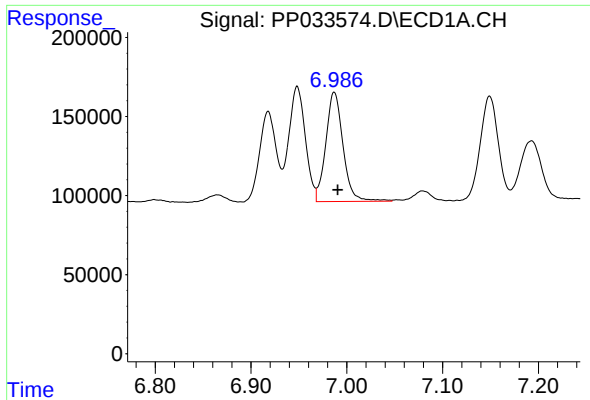


#25 AR-1248-5

R.T.: 6.987 min
Delta R.T.: -0.004 min
Response: 865165
Conc: 469.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
2/26/2021 10:31:23 AM

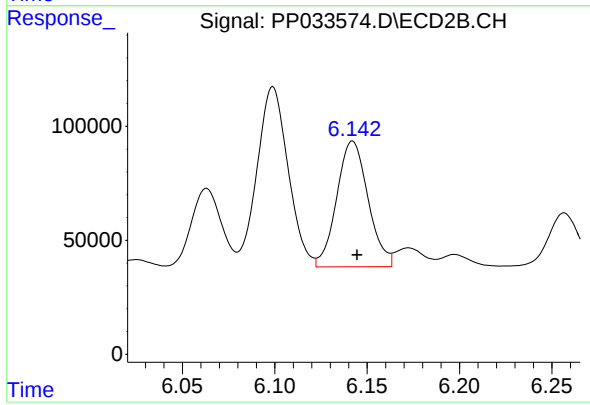

#25 AR-1248-5

R.T.: 6.142 min
Delta R.T.: -0.002 min
Response: 653038
Conc: 580.40 ng/ml