

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022522\
 Data File : PP044054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2022 03:41
 Operator : YP\AJ
 Sample : N1658-01 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1-3-DRUMS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/28/2022
 Supervised By :Ankita Jodhani 02/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 08:04:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.917	3.177	2883645	3243496	1.304m	1.727m#
2) SA Decachlor...	10.054	8.541	3247772	3343229	2.734m	2.061m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022522\
Data File : PP044054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2022 03:41
Operator : YP\AJ
Sample : N1658-01 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1-3-DRUMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/28/2022
Supervised By :Ankita Jodhani 02/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 08:04:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

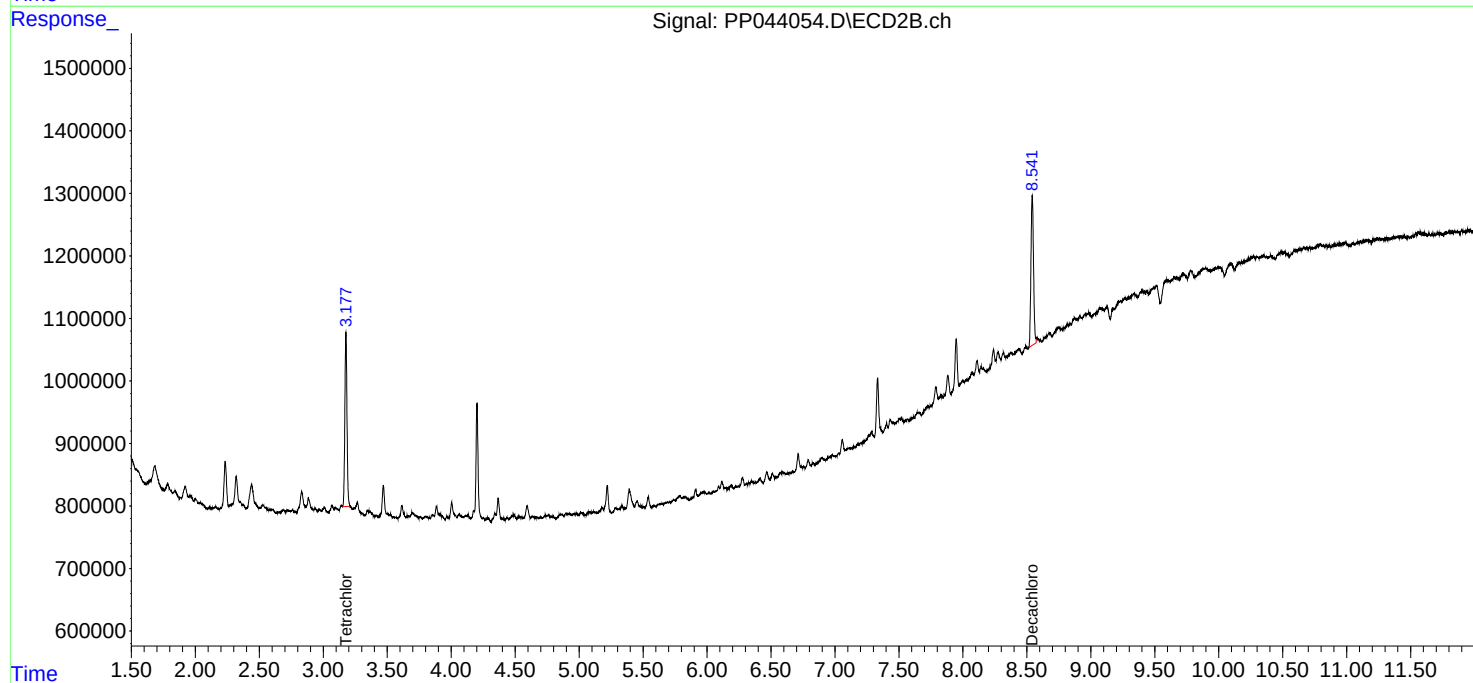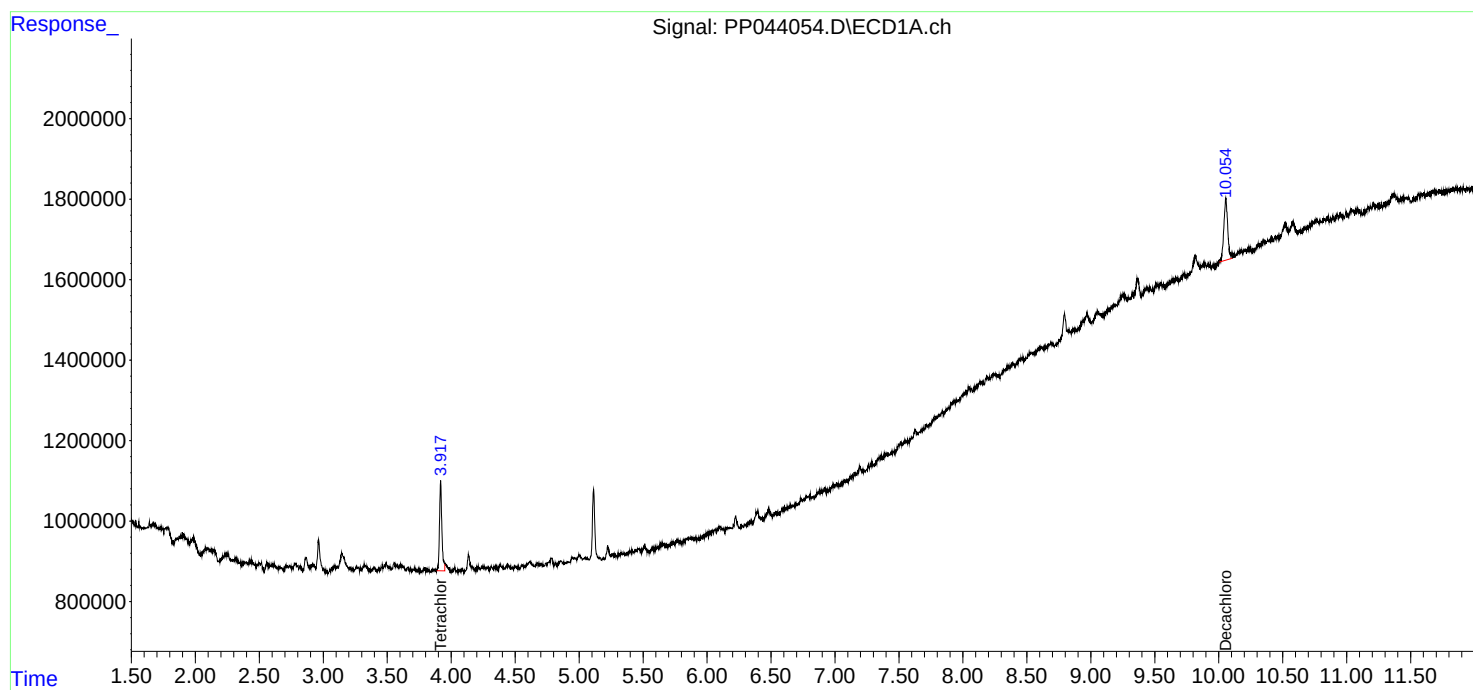

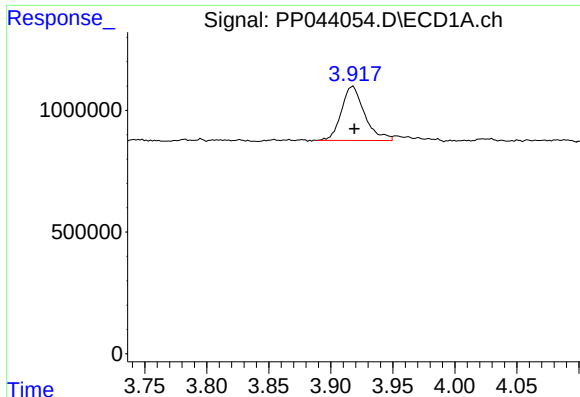


#1 Tetrachloro-m-xylene

R.T.: 3.917 min
Delta R.T.: -0.002 min
Response: 2883645
Conc: 1.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
1-3-DRUMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/28/2022
Supervised By :Ankita Jodhani 02/28/2022

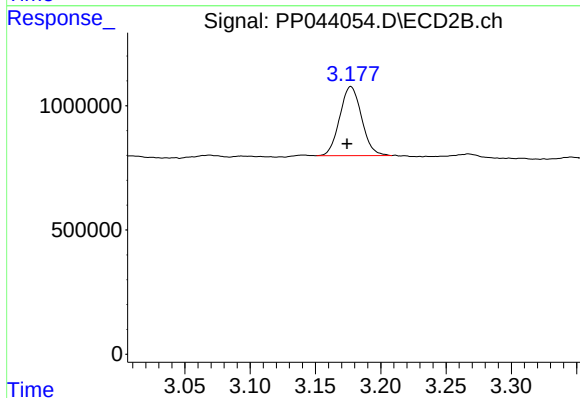


#1 Tetrachloro-m-xylene

R.T.: 3.177 min
Delta R.T.: 0.003 min
Response: 3243496
Conc: 1.73 ng/ml m

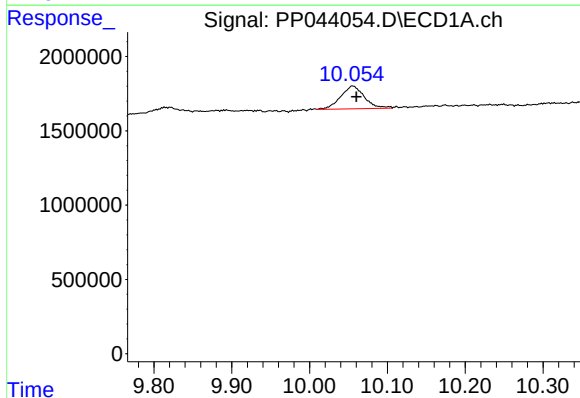

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: -0.006 min
Response: 3247772
Conc: 2.73 ng/ml m

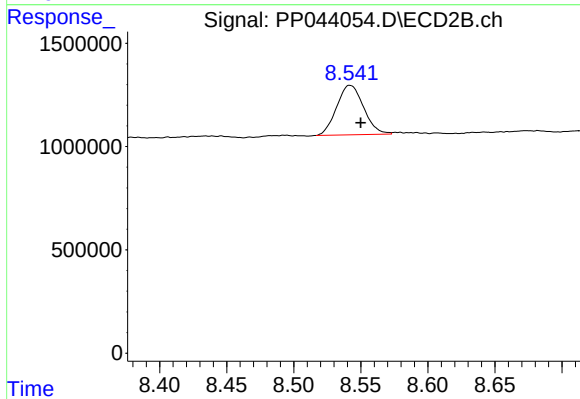

#2 Decachlorobiphenyl

R.T.: 8.541 min
Delta R.T.: -0.009 min
Response: 3343229
Conc: 2.06 ng/ml m