

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022621\
 Data File : PP033602.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Feb 2021 13:58
 Operator : DD\AJ
 Sample : M1480-15 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH384W-END-2-1

Manual Integrations
 APPROVED

Ankita
 3/2/2021 8:41:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 14:24:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.721	3.989	146188	117917	1.986m	2.678 #
2) SA Decachlor...	10.527	9.243	114329	100245	2.458	3.173m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022621\
Data File : PP033602.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2021 13:58
Operator : DD\AJ
Sample : M1480-15 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH384W-END-2-1


Manual Integrations
APPROVED

Ankita
3/2/2021 8:41:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 14:24:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

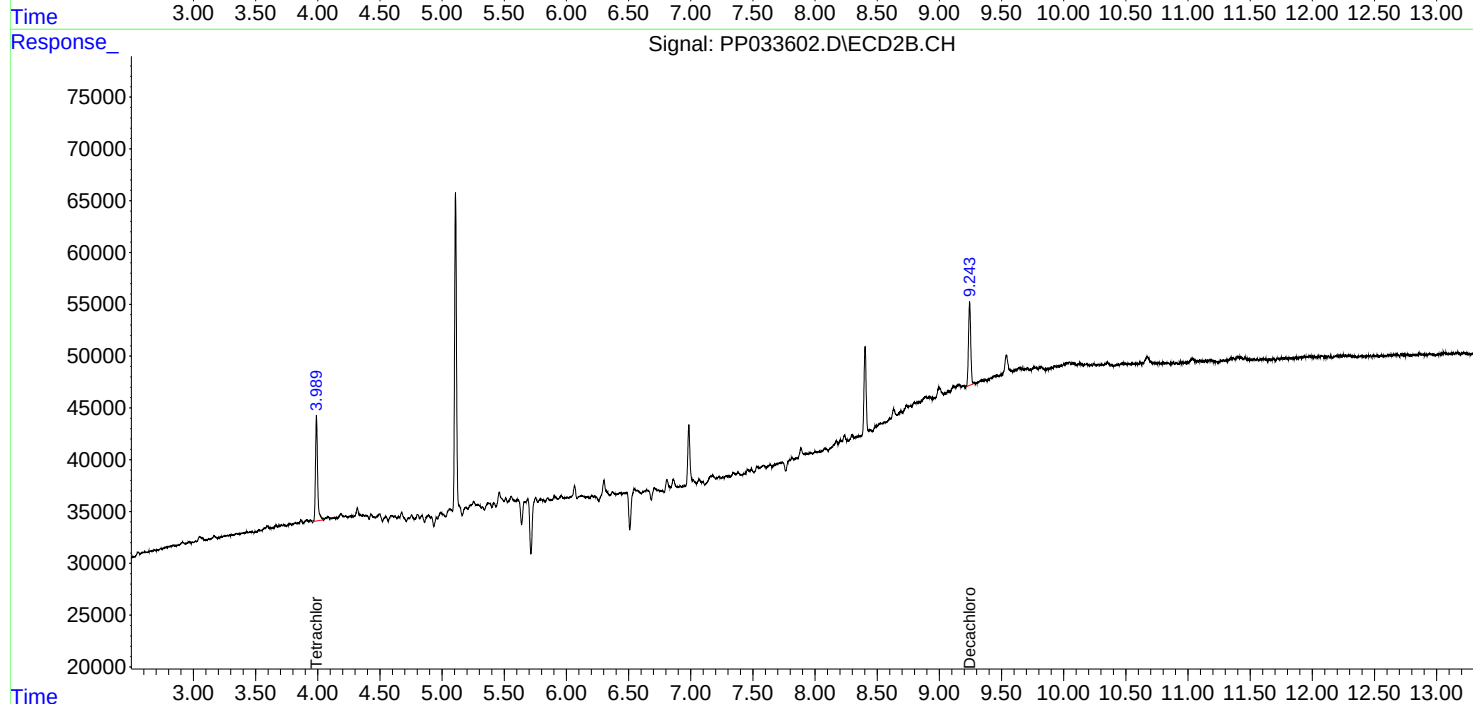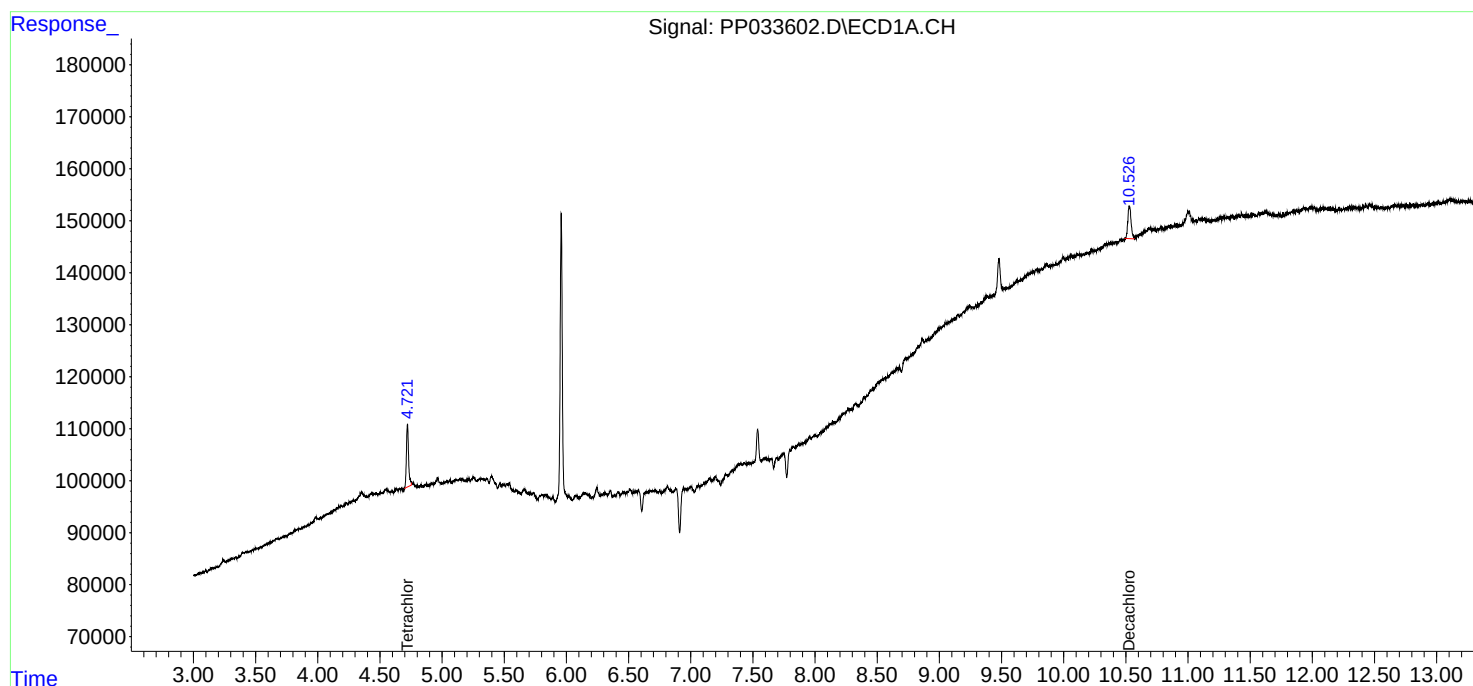

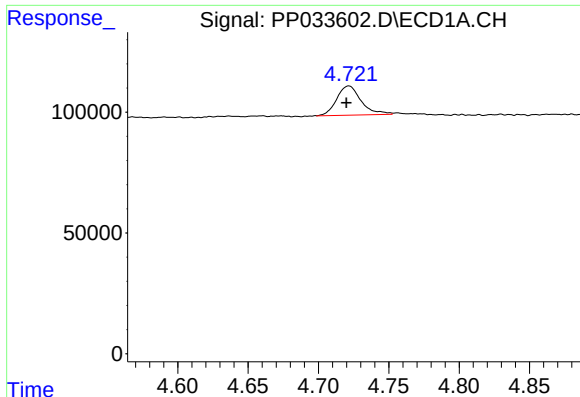


#1 Tetrachloro-m-xylene

R.T.: 4.721 min
Delta R.T.: 0.001 min
Response: 146188
Conc: 1.99 ng/ml m

Instrument :
ECD_P
ClientSampleId :
KMH384W-END-2-1


Manual Integrations
APPROVED

Ankita
3/2/2021 8:41:20 AM

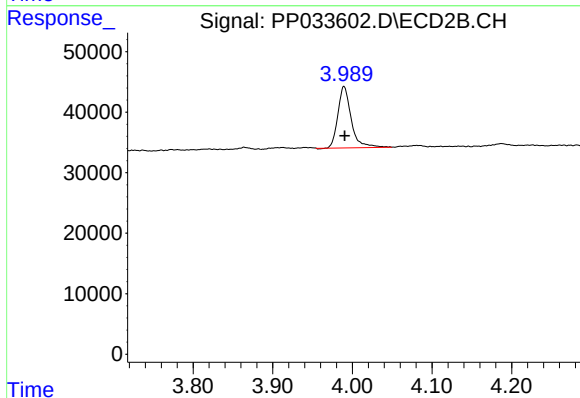


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 117917
Conc: 2.68 ng/ml

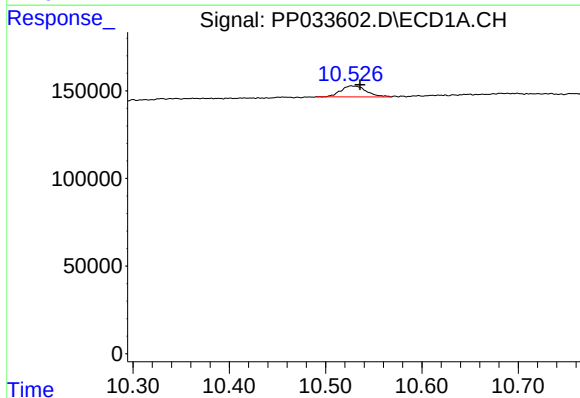

#2 Decachlorobiphenyl

R.T.: 10.527 min
Delta R.T.: -0.009 min
Response: 114329
Conc: 2.46 ng/ml

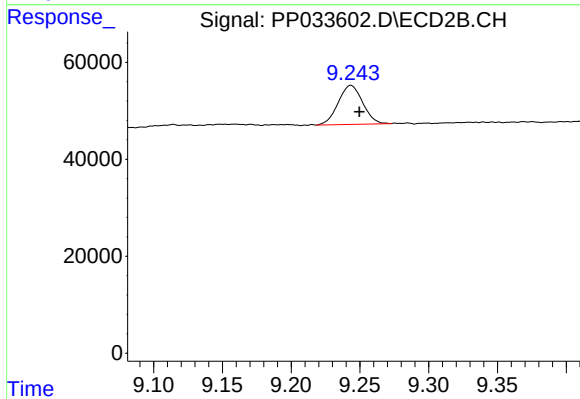

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.007 min
Response: 100245
Conc: 3.17 ng/ml m