

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
Data File : PP063451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 00:30
Operator : YP\AJ
Sample : P1524-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20240766-AMENDED-COMP-39N-N-3-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 01:37:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.641	47074120	47744120	20.948	20.754
2) SA Decachlor...	10.360	8.683	44362316	45699697	22.893	22.400

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
Data File : PP063451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 00:30
Operator : YP\AJ
Sample : P1524-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20240766-AMENDED-COMP-39N-N-3-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 01:37:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

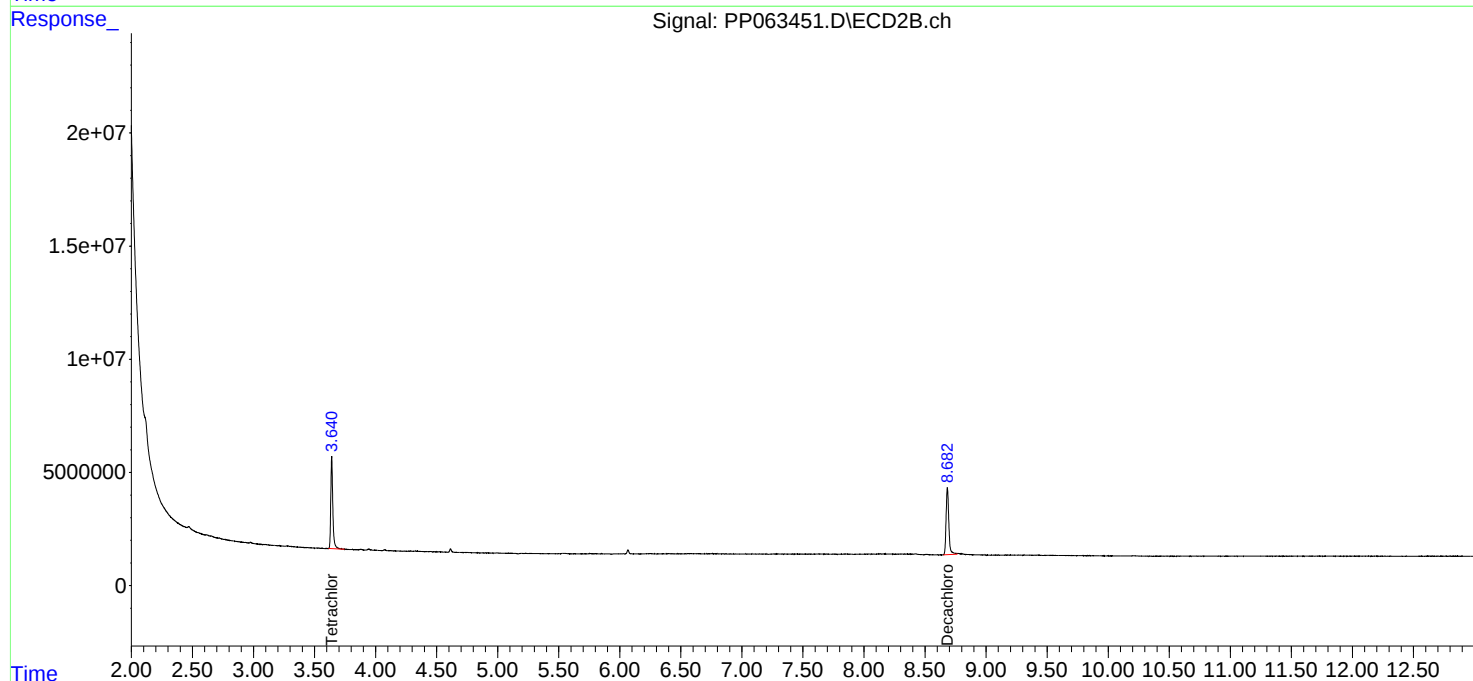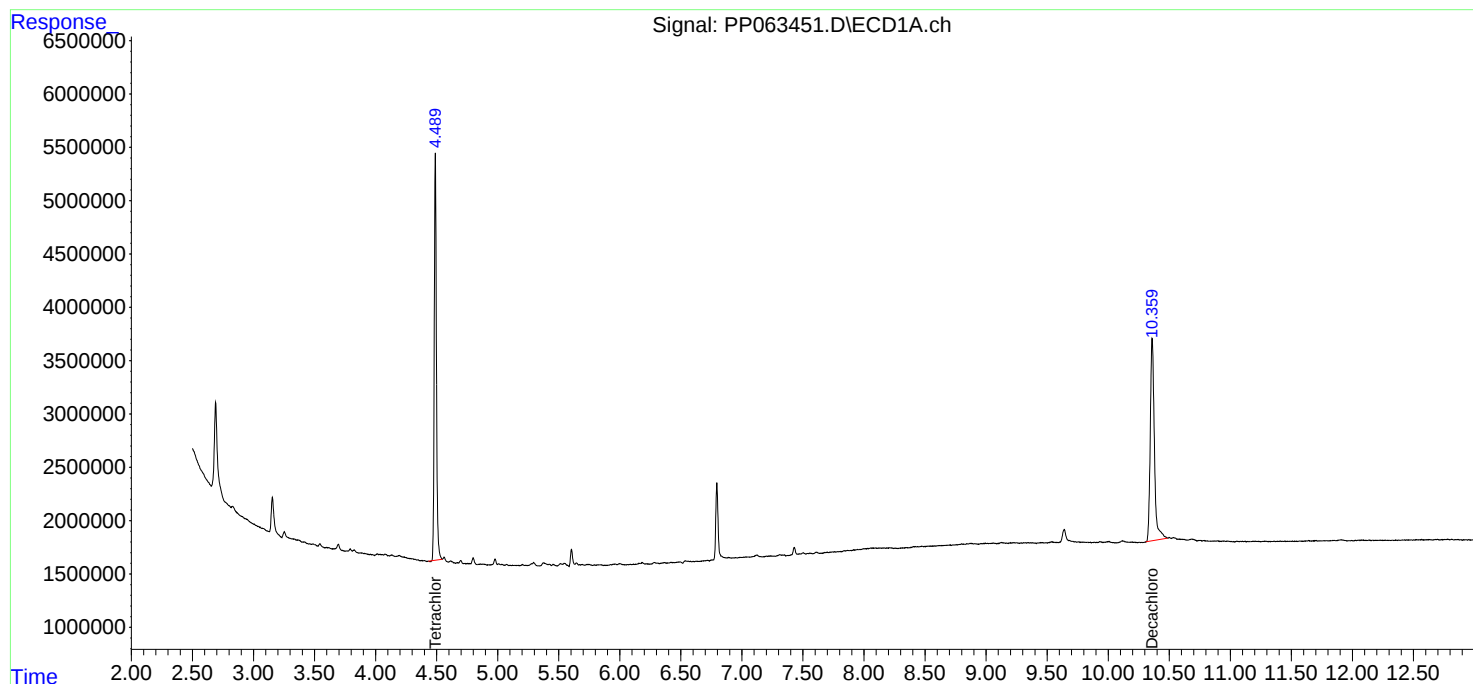


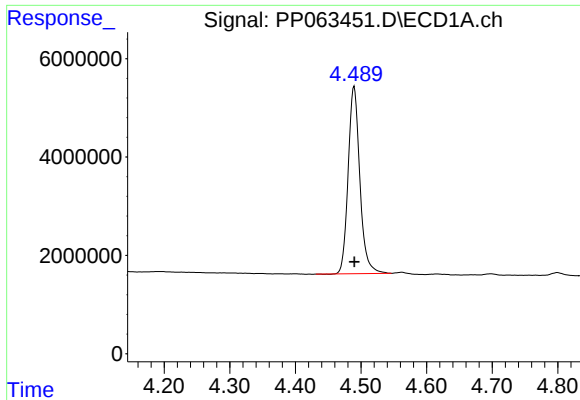

#1 Tetrachloro-m-xylene


R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 47074120
Conc: 20.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
20240766-AMENDED-COMP-39N-N-3-01

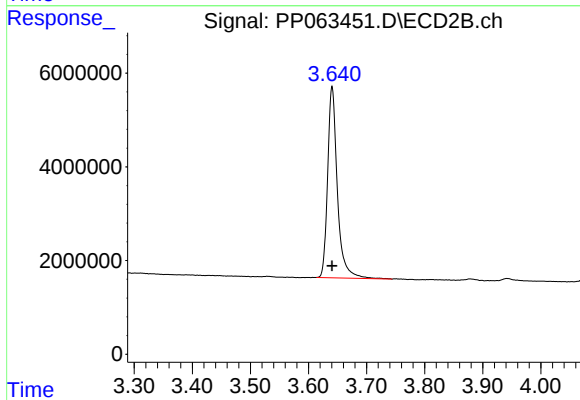


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 47744120
Conc: 20.75 ng/ml

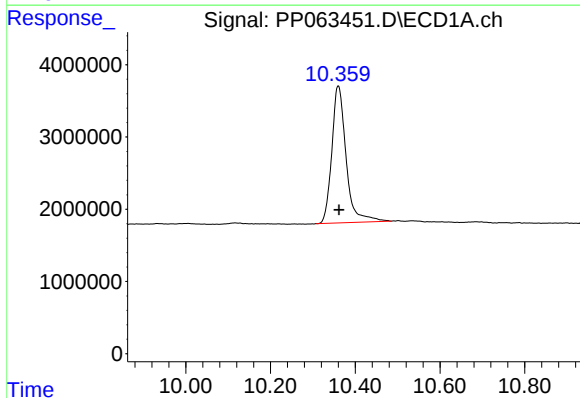

#2 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.002 min
Response: 44362316
Conc: 22.89 ng/ml

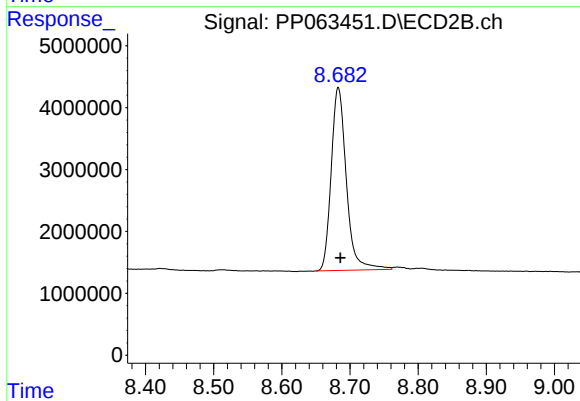

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.003 min
Response: 45699697
Conc: 22.40 ng/ml