

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
 Data File : PP063456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 01:51
 Operator : YP\AJ
 Sample : P1539-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20241102-AMENDED-COMPOSITE-35N-N-4-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/27/2024
 Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 05:07:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.641	44581665	43668059	19.839	18.982m
2) SA Decachlor...	10.361	8.683	45564874	49622569	23.514	24.323

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
Data File : PP063456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 01:51
Operator : YP\AJ
Sample : P1539-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

20241102-AMENDED-COMPOSITE-35N-N-4-01

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 02/27/2024

Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 05:07:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

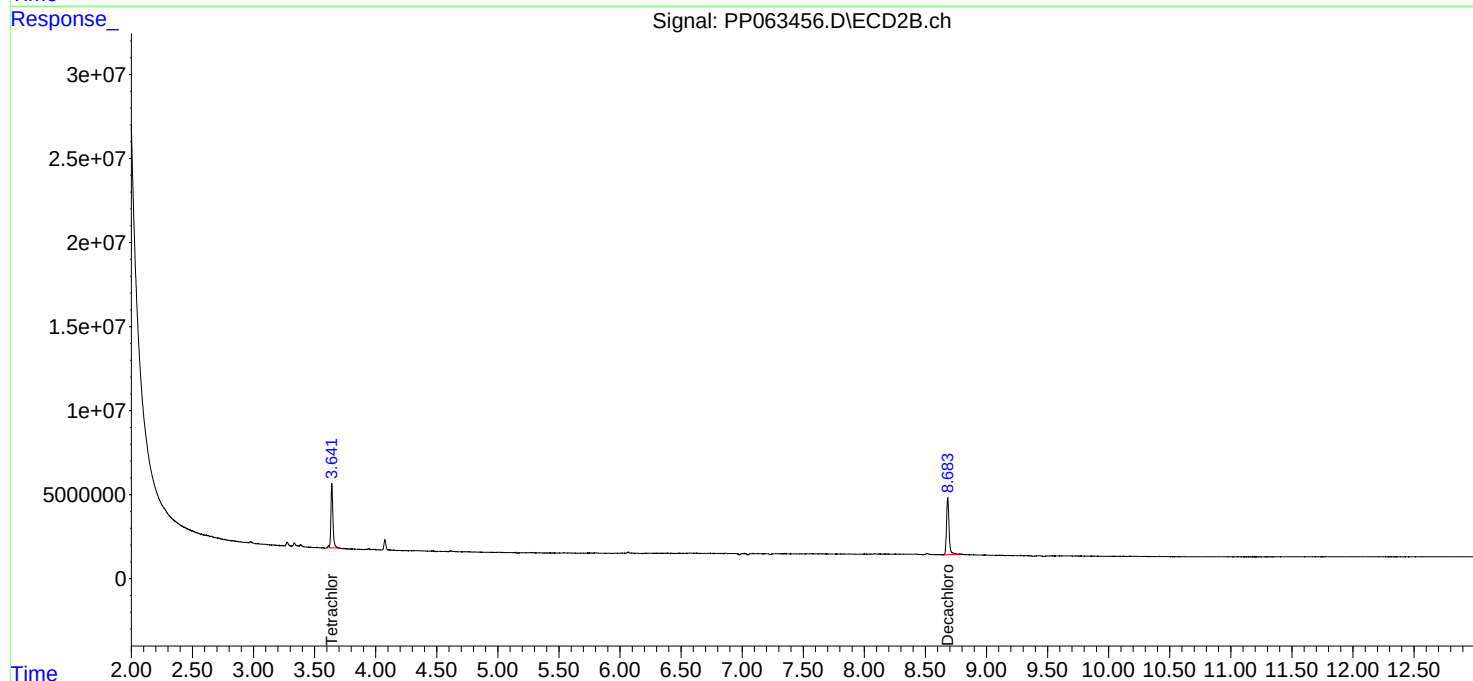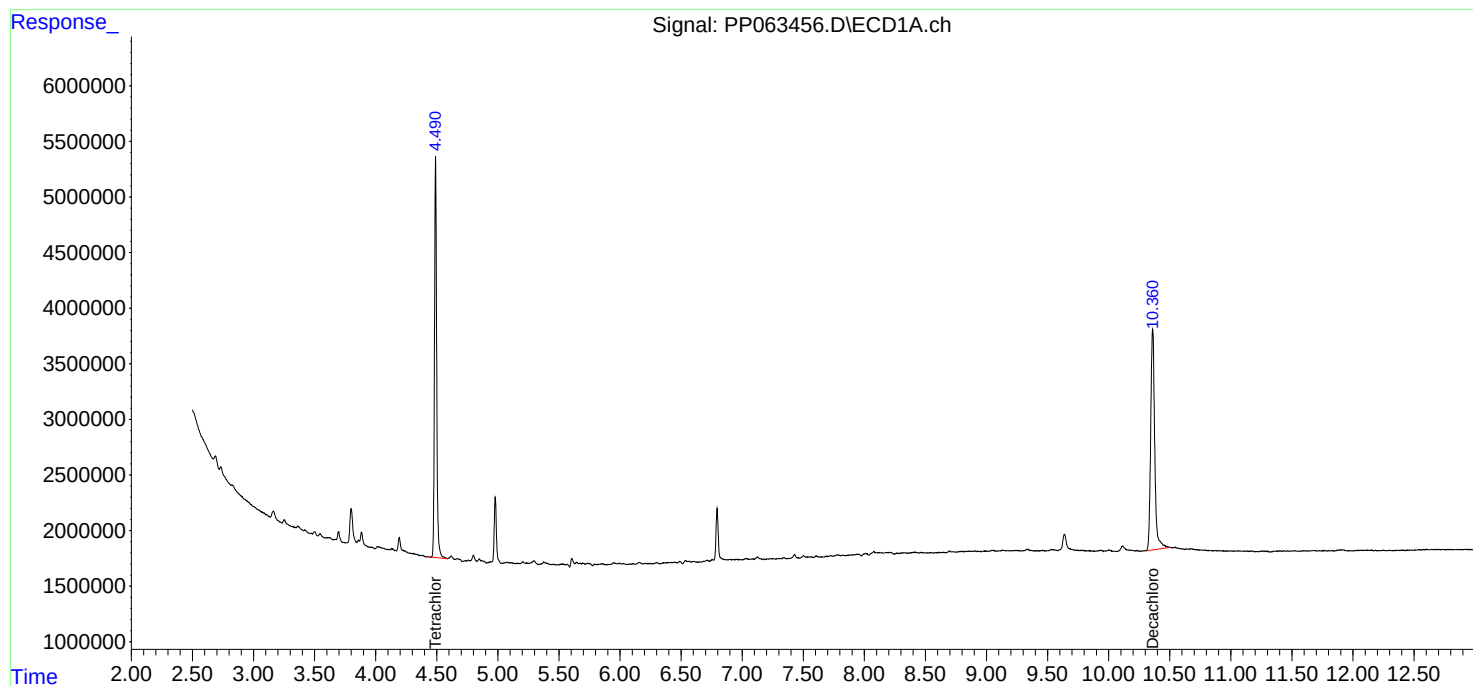

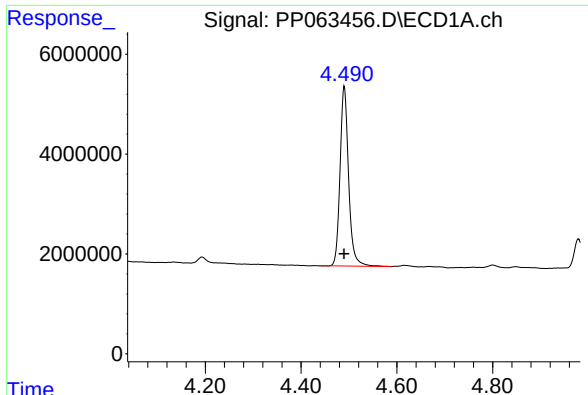

#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 44581665
Conc: 19.84 ng/ml

Instrument :

ECD_P


ClientSampleId :

20241102-AMENDED-COMPOSITE-35N-N-4-01

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 02/27/2024
Supervised By :Ankita Jodhani 02/27/2024

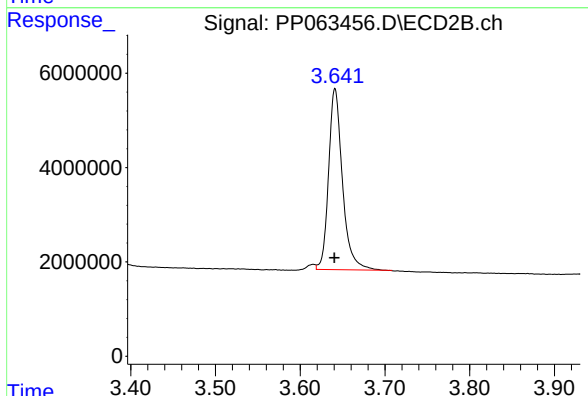


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 43668059
Conc: 18.98 ng/ml m

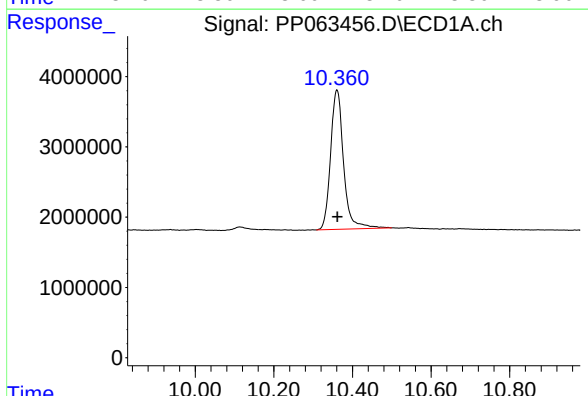

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.001 min
Response: 45564874
Conc: 23.51 ng/ml

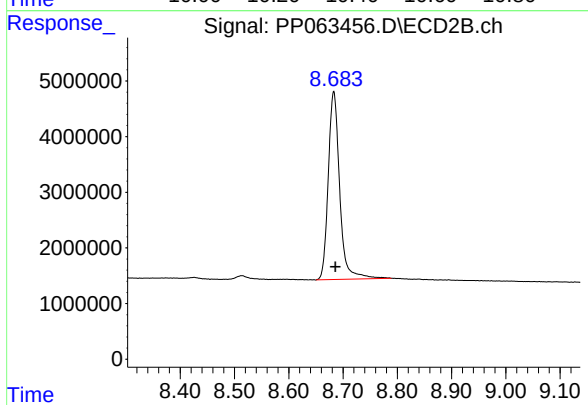

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.003 min
Response: 49622569
Conc: 24.32 ng/ml