

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
 Data File : PP063459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 02:40
 Operator : YP\AJ
 Sample : P1539-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

20241105-AMENDED-COMPOSITE-35N-N-4-04

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 02/27/2024

Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 05:08:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 01:30:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.641	45054522	44805404	20.049m	19.476
2) SA Decachlor...	10.360	8.684	41479822	45319882	21.406	22.214

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022624\
Data File : PP063459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 02:40
Operator : YP\AJ
Sample : P1539-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :

ECD_P

Client Sample ID :

20241105-AMENDED-COMPOSITE-35N-N-4-04

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 02/27/2024

Supervised By :Ankita Jodhani 02/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 05:08:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 01:30:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

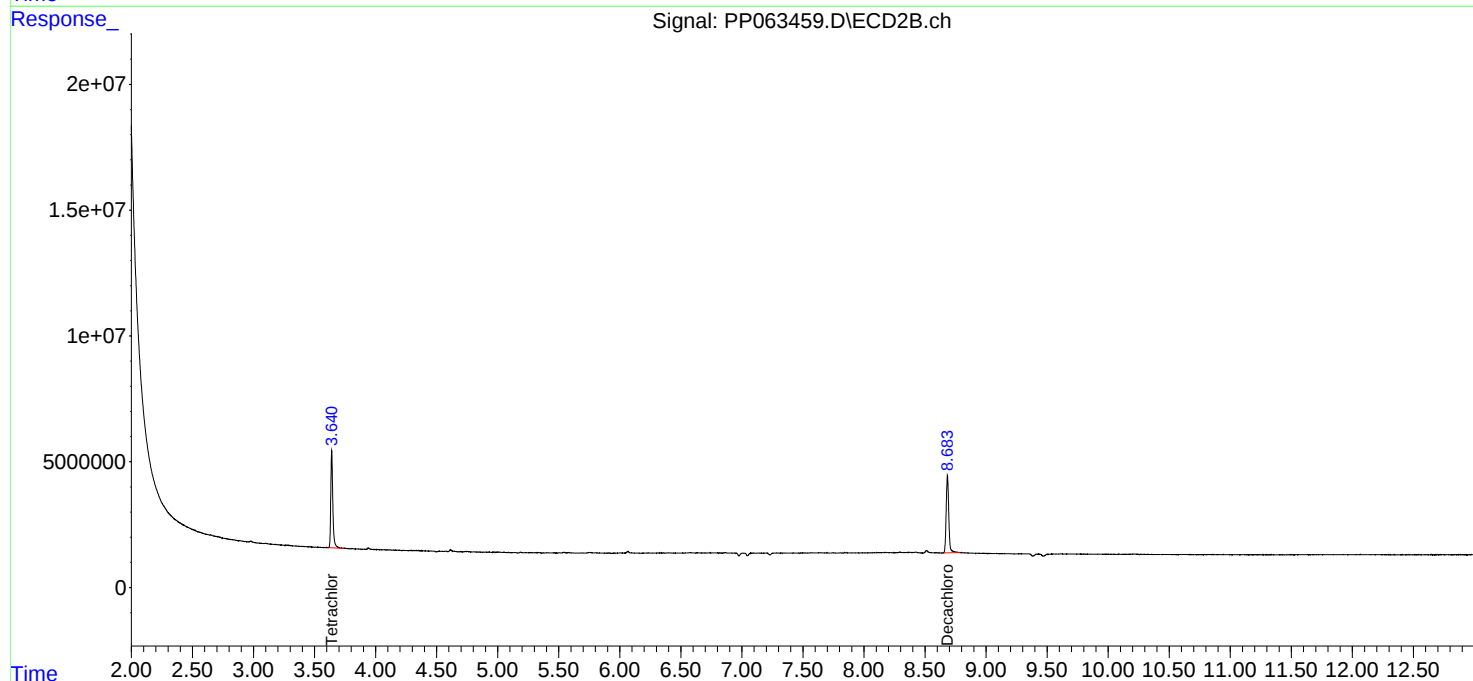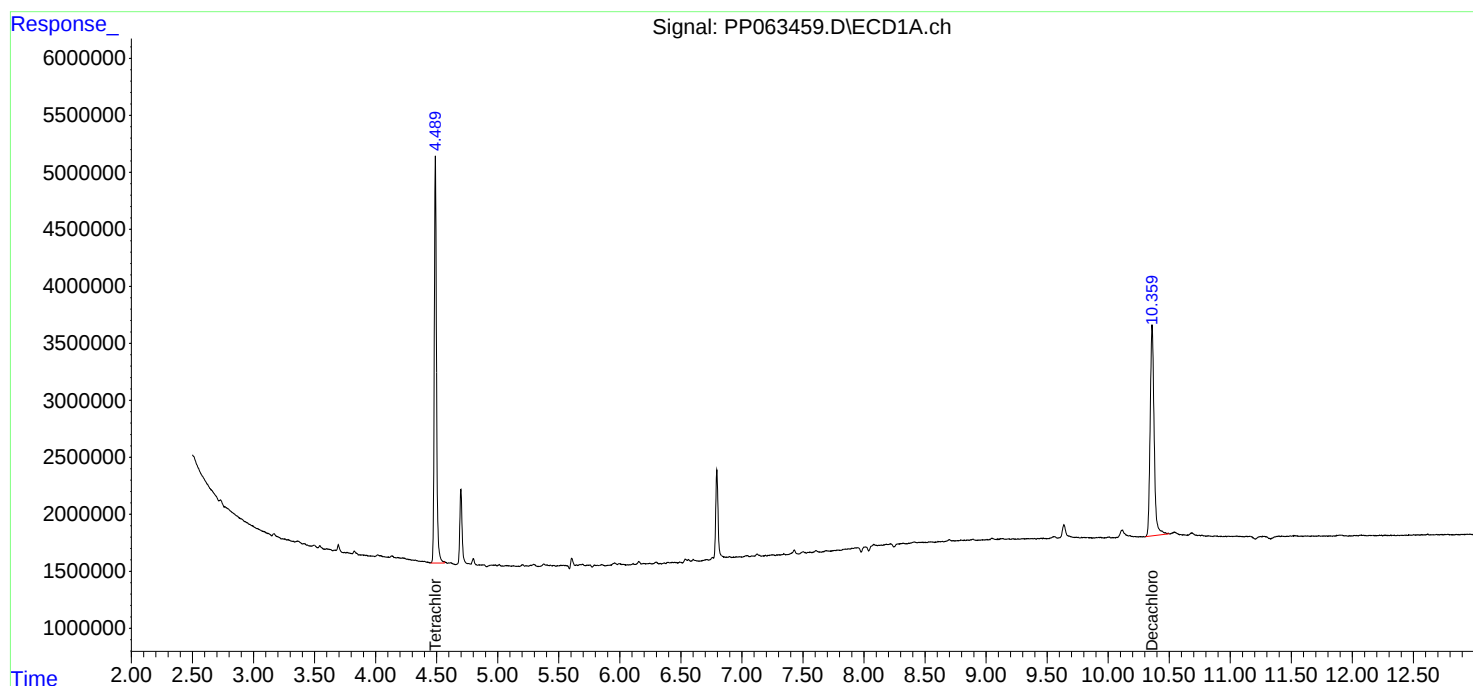

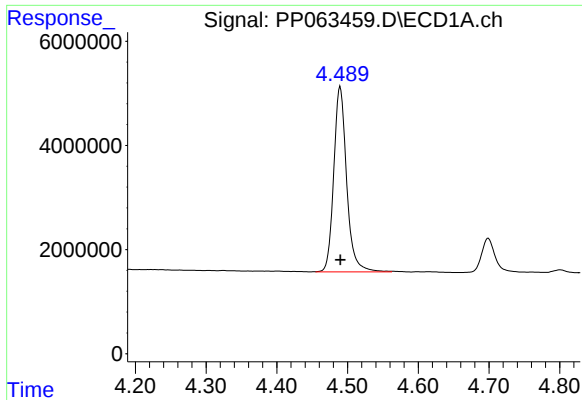


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 45054522
Conc: 20.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
20241105-AMENDED-COMPOSITE-35N-N-4-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2024
Supervised By :Ankita Jodhani 02/27/2024

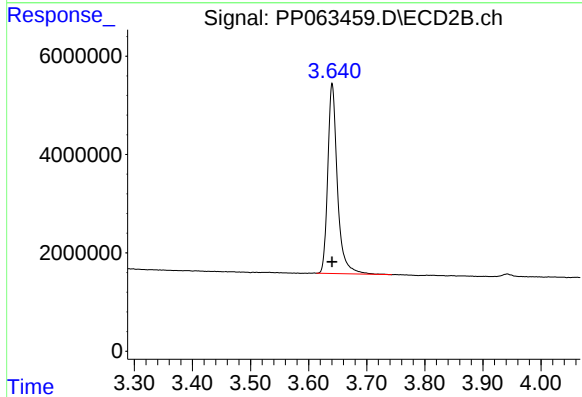


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 44805404
Conc: 19.48 ng/ml

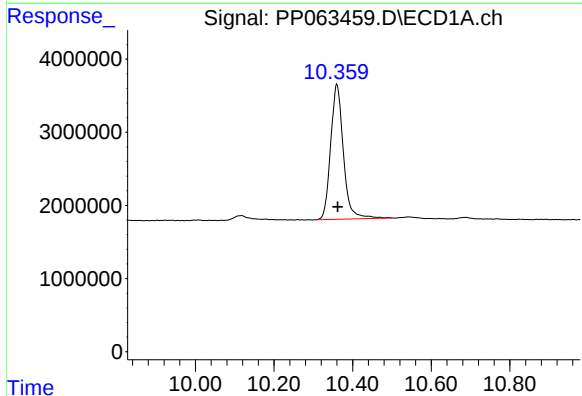

#2 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.002 min
Response: 41479822
Conc: 21.41 ng/ml

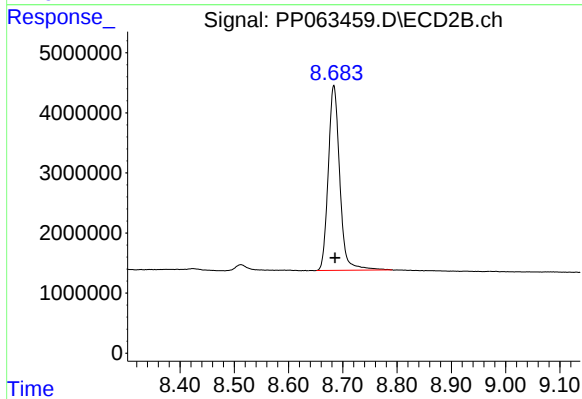

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.002 min
Response: 45319882
Conc: 22.21 ng/ml