

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022625\
 Data File : PP070073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2025 14:39
 Operator : YP\AJ
 Sample : Q1428-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NB-07-022525

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/27/2025
 Supervised By :Ankita Jodhani 02/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 01:47:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.527	3.831	28349482	19663173	19.317m	20.567
2) SA Decachlor...	10.256	8.887	21942838	18813185	19.264	17.354

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022625\
Data File : PP070073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2025 14:39
Operator : YP\AJ
Sample : Q1428-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NB-07-022525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2025
Supervised By :Ankita Jodhani 02/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 01:47:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

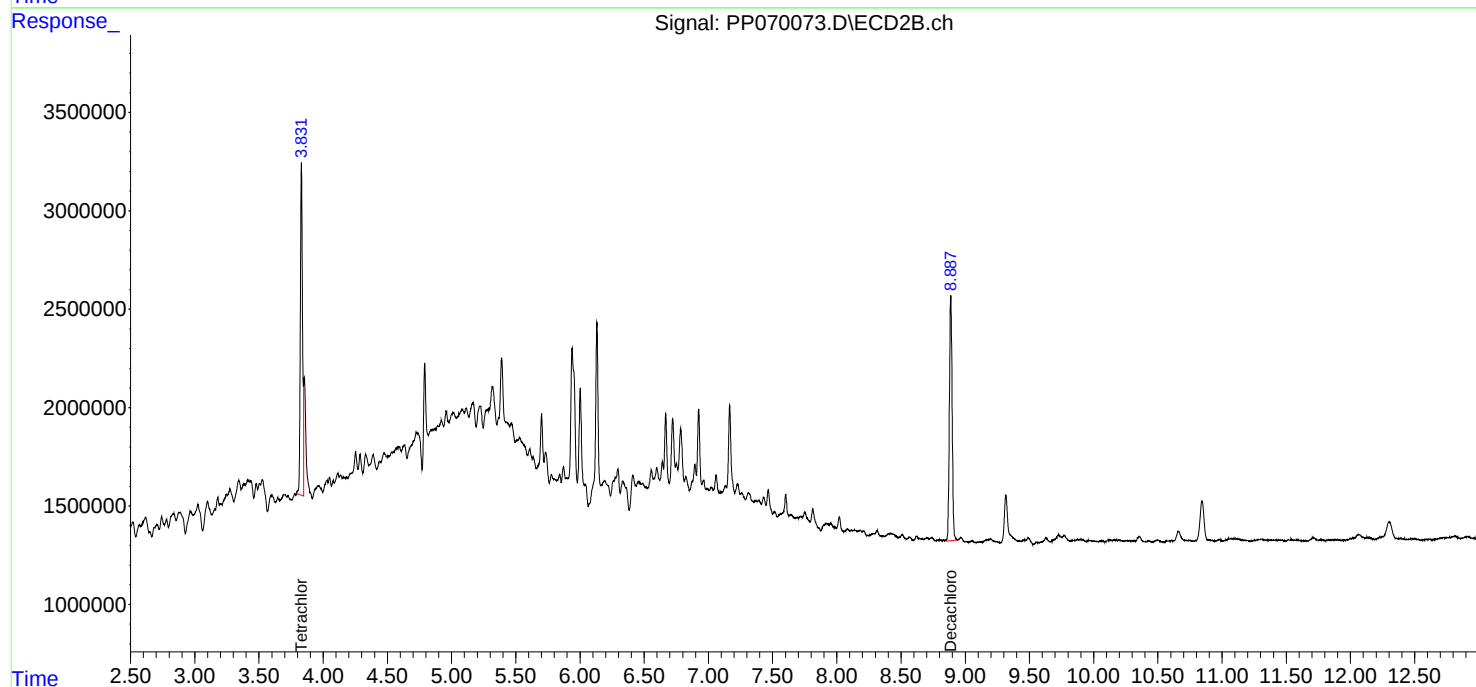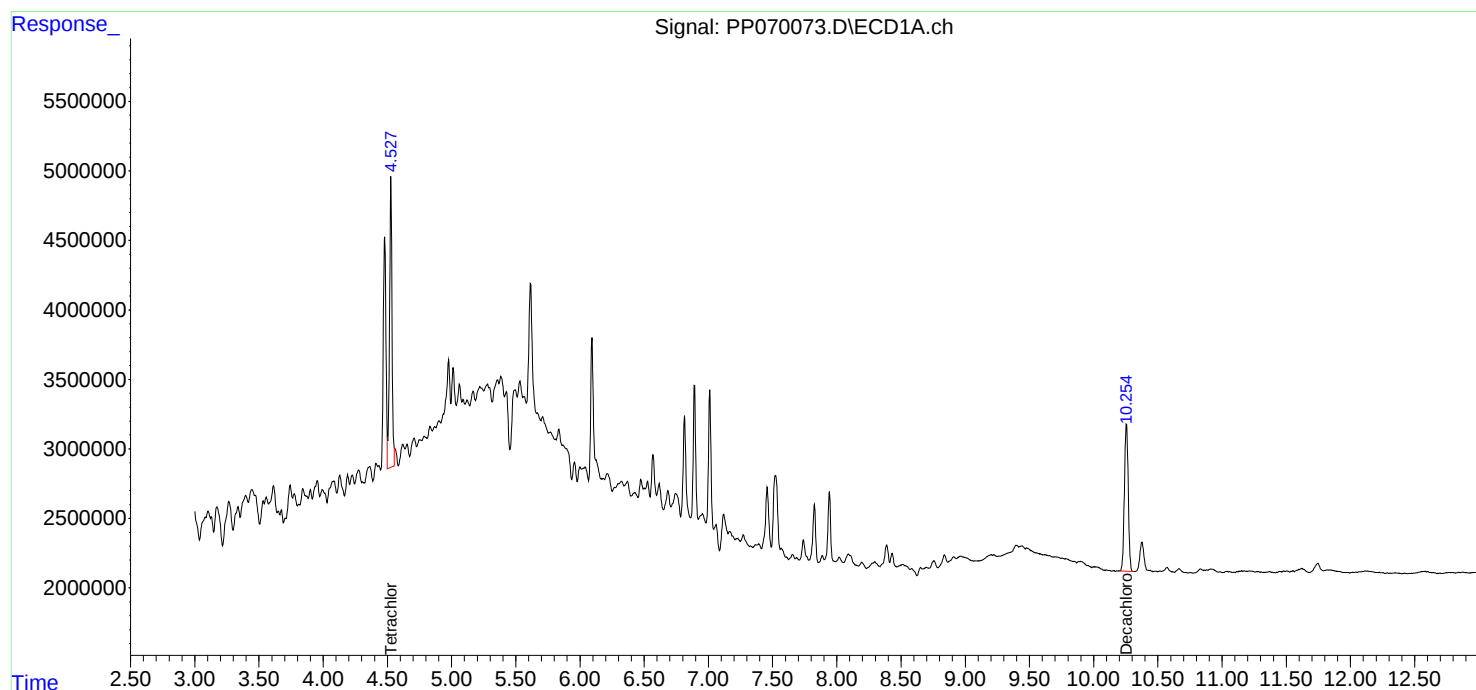

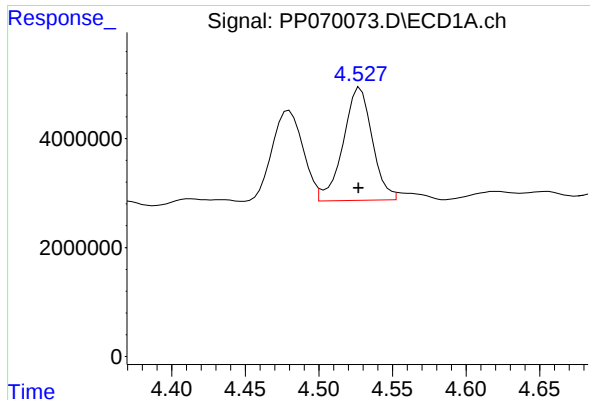


#1 Tetrachloro-m-xylene

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 28349482
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
NB-07-022525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/27/2025
Supervised By :Ankita Jodhani 02/27/2025

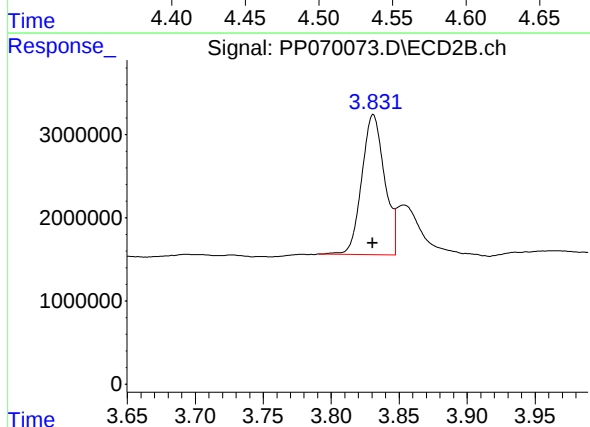


#1 Tetrachloro-m-xylene

R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 19663173
Conc: 20.57 ng/ml

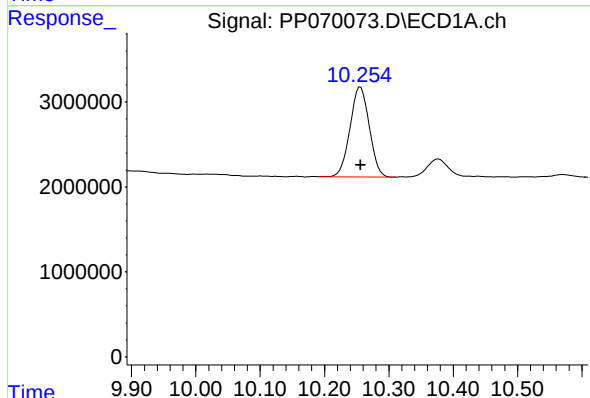

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.000 min
Response: 21942838
Conc: 19.26 ng/ml

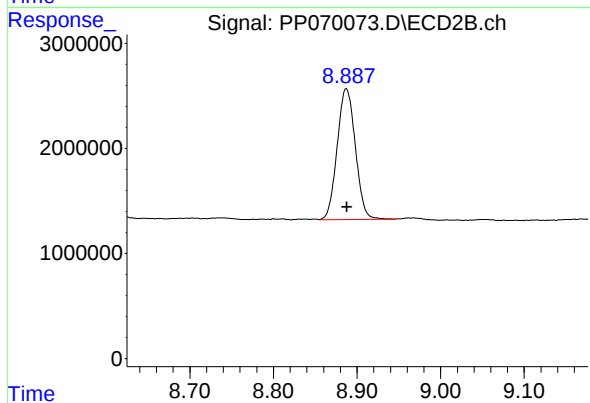

#2 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: 0.000 min
Response: 18813185
Conc: 17.35 ng/ml