

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP022719\  
 Data File : PP029175.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Feb 2019 10:10  
 Operator : EI\MA  
 Sample : I.BLK  
 Misc : hexane  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 28 03:35:57 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP022119.M  
 Quant Title : 8080.M  
 QLast Update : Fri Feb 22 02:24:04 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|--------|--------|----------|----------|---------|----------|
| -----                       |              |        |        |          |          |         |          |
| System Monitoring Compounds |              |        |        |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 11.940 | 12.128 | 12401536 | 15374252 | 412.609 | 405.092  |
| Target Compounds            |              |        |        |          |          |         |          |
| 11) T                       | 2,4,5-TP ... | 0.000  | 15.235 | 0        | 151026   | N.D.    | 0.742 #  |
| 12) T                       | 2,4,5-T      | 0.000  | 15.890 | 0        | 221454   | N.D.    | 1.338 #  |
| 14) T                       | DINOSEB      | 0.000  | 16.793 | 0        | 142650   | N.D.    | 1.088 #  |
| 15) T                       | Picloram     | 0.000  | 18.176 | 0        | 4998037  | N.D.    | 22.211 # |
| 16) T                       | DCPA         | 0.000  | 18.176 | 0        | 4998037  | N.D.    | 21.507 # |
| -----                       |              |        |        |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP022719\  
Data File : PP029175.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Feb 2019 10:10  
Operator : EI\MA  
Sample : I.BLK  
Misc : hexane  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 28 03:35:57 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP022119.M  
Quant Title : 8080.M  
QLast Update : Fri Feb 22 02:24:04 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

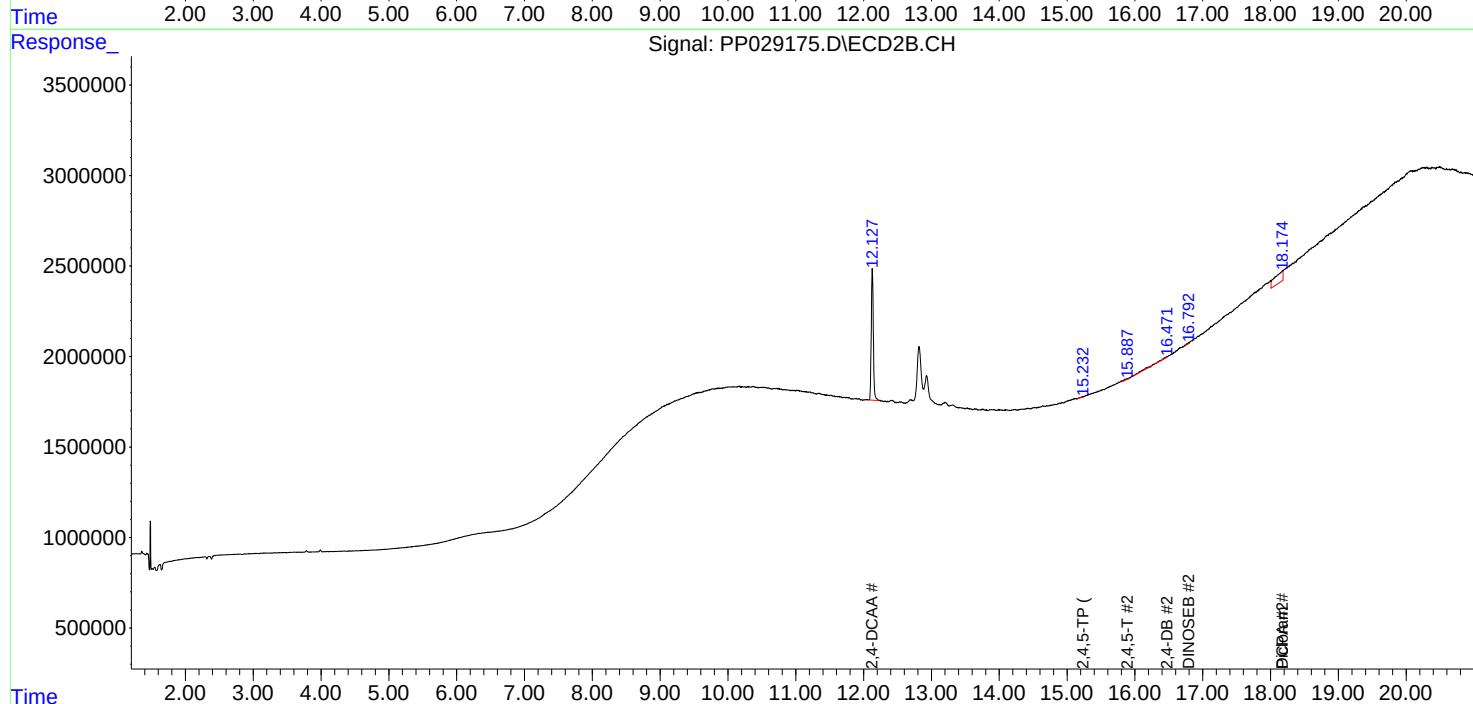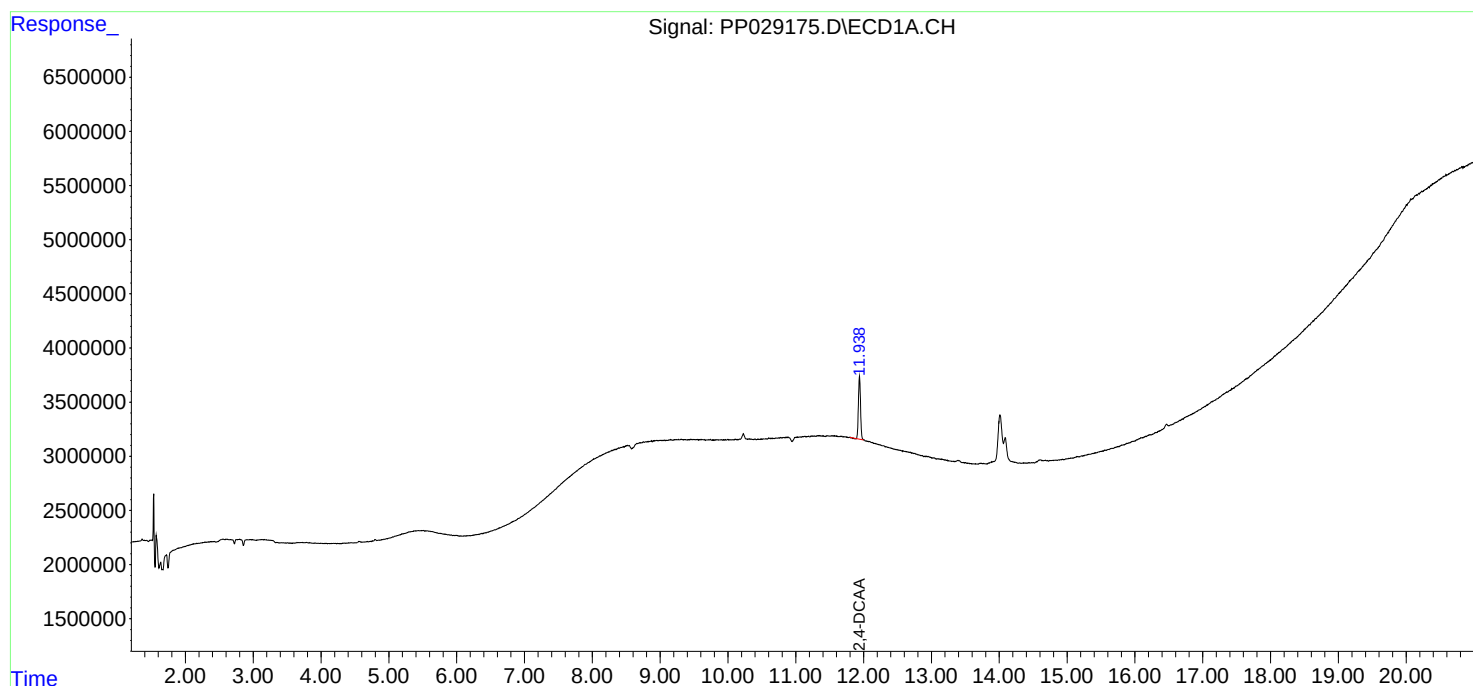


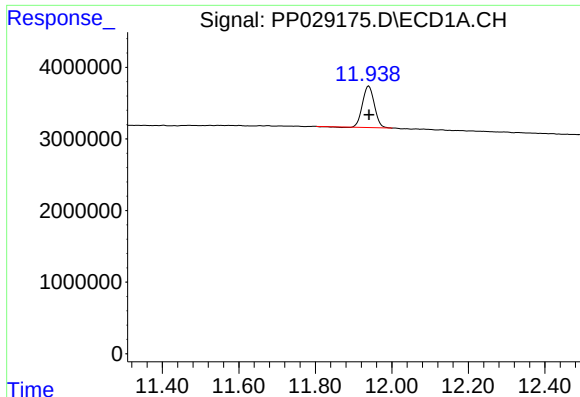

#4 2,4-DCAA


R.T.: 11.940 min  
Delta R.T.: 0.000 min  
Response: 12401536  
Conc: 412.61 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

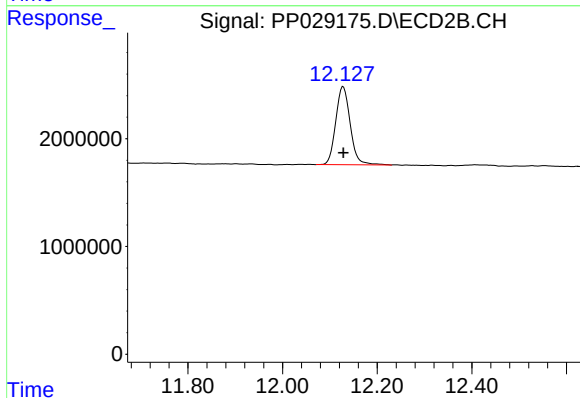


#4 2,4-DCAA

R.T.: 12.128 min  
Delta R.T.: 0.000 min  
Response: 15374252  
Conc: 405.09 ng/ml

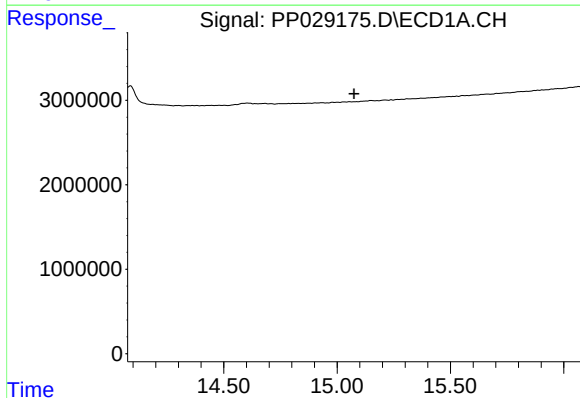


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T. : 15.075 min  
Response: 0  
Conc: N.D.

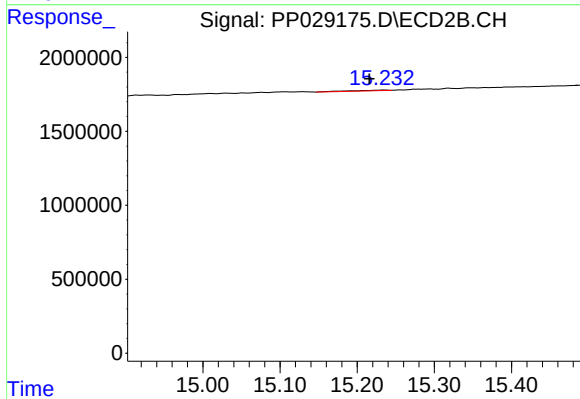

#11 2,4,5-TP (SILVEX)


R.T.: 15.235 min  
Delta R.T.: 0.019 min  
Response: 151026  
Conc: 0.74 ng/ml

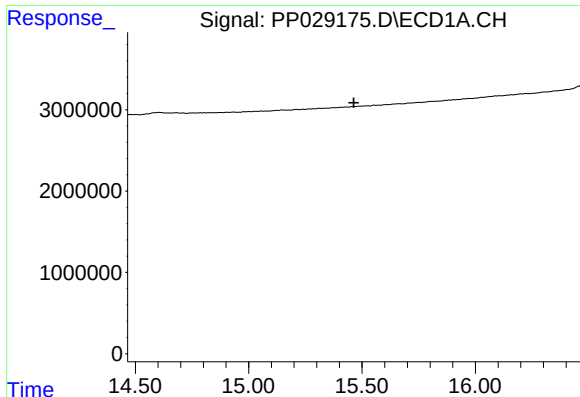

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T.: 15.464 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

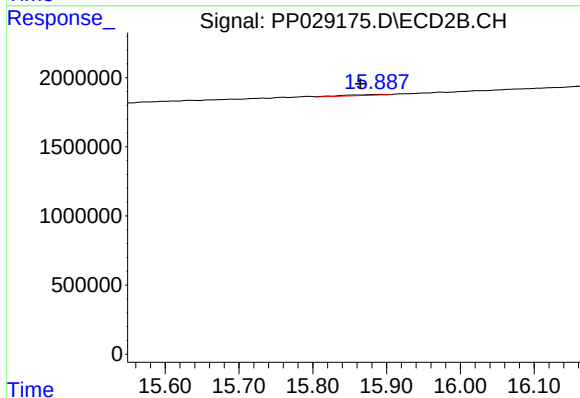


#12 2,4,5-T

R.T.: 15.890 min  
Delta R.T.: 0.025 min  
Response: 221454  
Conc: 1.34 ng/ml

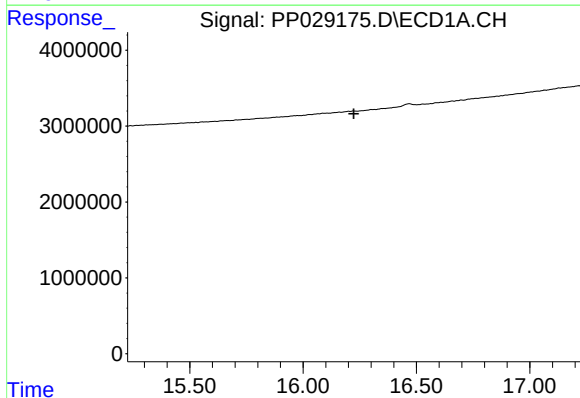


#13 2,4-DB

R.T.: 16.224 min  
Delta R.T.: 0.000 min  
Response: -5667054  
Conc: N.D.

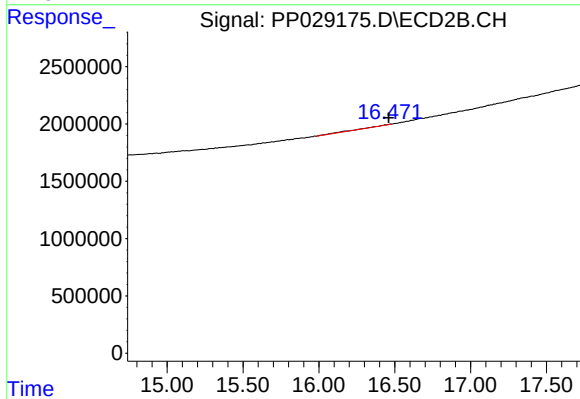

#13 2,4-DB


R.T.: 16.472 min  
Delta R.T.: 0.013 min  
Response: 616332  
Conc: 27.36 ng/ml

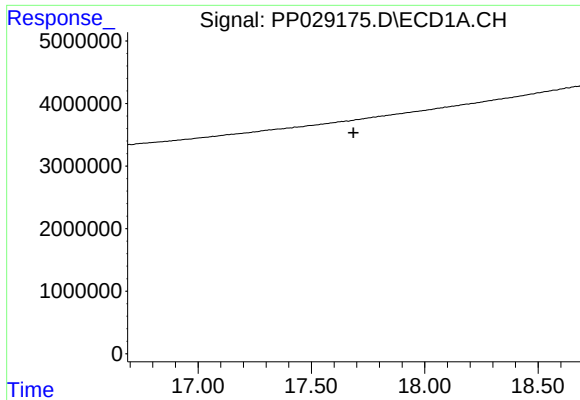

#14 DINOSEB


R.T.: 0.000 min  
Exp R.T. : 17.686 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

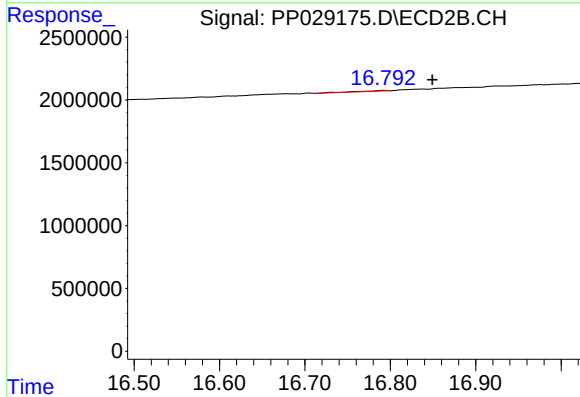


#14 DINOSEB

R.T.: 16.793 min  
Delta R.T.: -0.056 min  
Response: 142650  
Conc: 1.09 ng/ml

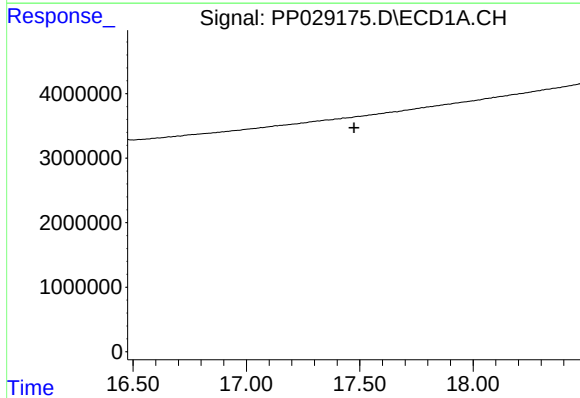


#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 17.475 min  
Response: 0  
Conc: N.D.

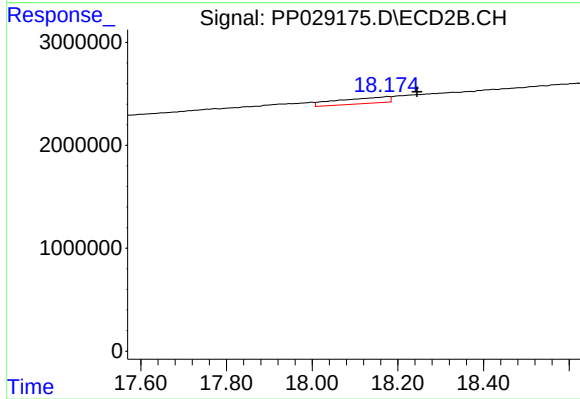

#15 Picloram


R.T.: 18.176 min  
Delta R.T.: -0.068 min  
Response: 4998037  
Conc: 22.21 ng/ml

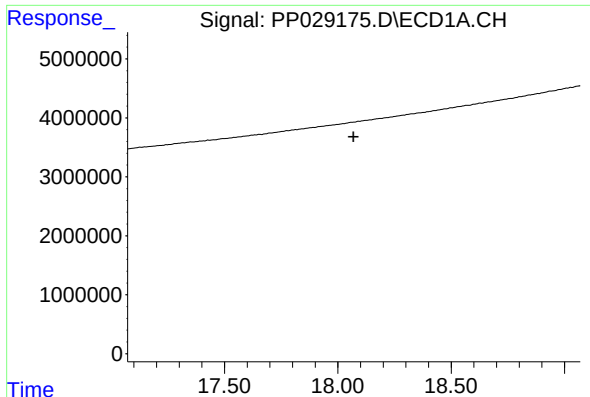

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 18.069 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

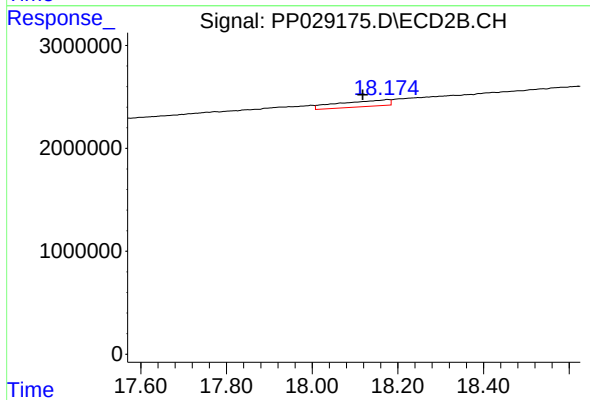

#16 DCPA

R.T.: 18.176 min  
Delta R.T.: 0.058 min  
Response: 4998037  
Conc: 21.51 ng/ml